

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031524\
 Data File : VV034666.D
 Acq On : 15 Mar 2024 20:41
 Operator : SY/MD
 Sample : P1740-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GH5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

Signal : TIC: VV034666.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	94	rVB	140798	151239	12.59%	1.581%
2	1.532	146	153	165	rBV	136389	155799	12.97%	1.629%
3	2.060	307	317	330	rBV	264384	382733	31.86%	4.001%
4	2.645	496	499	503	rVB	267	209	0.02%	0.002%
5	2.696	513	515	518	rBV2	352	184	0.02%	0.002%
6	2.896	574	577	579	rBV2	147	105	0.01%	0.001%
7	2.976	597	602	604	rBV	187	180	0.01%	0.002%
8	3.089	633	637	639	rBV2	155	115	0.01%	0.001%
9	3.272	690	694	695	rBV	188	143	0.01%	0.001%
10	3.304	701	704	707	rBV	173	99	0.01%	0.001%
11	3.333	710	713	714	rBV	239	97	0.01%	0.001%
12	3.359	717	721	726	rVB3	259	280	0.02%	0.003%
13	3.388	726	730	732	rBV	282	196	0.02%	0.002%
14	3.449	746	749	753	rVB2	284	149	0.01%	0.002%
15	3.500	761	765	771	rBV2	234	237	0.02%	0.002%
16	3.661	812	815	820	rBB2	162	119	0.01%	0.001%
17	3.687	820	823	829	rVB2	173	186	0.02%	0.002%
18	3.728	834	836	840	rBV	168	120	0.01%	0.001%
19	3.748	840	842	844	rBV	255	91	0.01%	0.001%
20	3.796	848	857	894	rBV	96865	296030	24.64%	3.095%
21	4.246	982	997	1031	rBV	191494	497483	41.41%	5.201%
22	4.523	1080	1083	1087	rBV2	487	359	0.03%	0.004%
23	4.616	1109	1112	1117	rBV3	423	360	0.03%	0.004%
24	4.696	1135	1137	1140	rVB2	350	143	0.01%	0.001%
25	4.719	1142	1144	1146	rBV	150	85	0.01%	0.001%
26	4.732	1146	1148	1150	rBV2	219	100	0.01%	0.001%
27	4.802	1167	1170	1171	rBV	217	103	0.01%	0.001%
28	4.831	1177	1179	1181	rBV2	159	84	0.01%	0.001%
29	4.870	1186	1191	1194	rBV3	367	359	0.03%	0.004%
30	4.953	1199	1217	1249	rBV2	449505	1201285	100.00%	12.559%
31	5.378	1345	1349	1353	rBV3	262	305	0.03%	0.003%
32	5.449	1368	1371	1373	rBV	249	145	0.01%	0.002%
33	5.532	1386	1397	1424	rBV	399577	832678	69.32%	8.705%
34	5.834	1482	1491	1513	rVB4	6980	16363	1.36%	0.171%
35	5.934	1519	1522	1523	rBV	267	157	0.01%	0.002%
36	5.989	1526	1539	1571	rVV	268951	561542	46.75%	5.871%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031524\
 Data File : VV034666.D
 Acq On : 15 Mar 2024 20:41
 Operator : SY/MD
 Sample : P1740-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GH5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	6.236	1615	1616	1617	rBV	301	97	0.01%	0.001%
38	6.278	1625	1629	1631	rBV2	365	256	0.02%	0.003%
39	6.342	1645	1649	1651	rBV2	204	124	0.01%	0.001%
40	6.365	1653	1656	1660	rVB2	237	179	0.01%	0.002%
41	6.387	1660	1663	1666	rBV	312	224	0.02%	0.002%
42	6.500	1695	1698	1699	rBV	190	91	0.01%	0.001%
43	6.558	1712	1716	1719	rBV2	218	194	0.02%	0.002%
44	6.606	1720	1731	1738	rBV6	1160	2367	0.20%	0.025%
45	6.860	1807	1810	1812	rBV	220	147	0.01%	0.002%
46	6.912	1816	1826	1850	rBV	128827	252167	20.99%	2.636%
47	7.243	1918	1929	1966	rBV	508861	912750	75.98%	9.542%
48	7.555	2016	2026	2051	rBV	88345	167798	13.97%	1.754%
49	7.783	2094	2097	2099	rBV2	217	151	0.01%	0.002%
50	7.799	2101	2102	2105	rBV2	183	107	0.01%	0.001%
51	7.825	2108	2110	2112	rVB2	269	125	0.01%	0.001%
52	7.924	2140	2141	2146	rBV2	406	229	0.02%	0.002%
53	8.024	2163	2172	2224	rBV	356606	721628	60.07%	7.544%
54	8.439	2299	2301	2304	rBV2	314	210	0.02%	0.002%
55	8.548	2332	2335	2337	rBV2	413	192	0.02%	0.002%
56	8.622	2355	2358	2361	rVB2	266	114	0.01%	0.001%
57	8.674	2369	2374	2378	rBV3	400	489	0.04%	0.005%
58	8.715	2384	2387	2388	rBV	176	87	0.01%	0.001%
59	8.748	2393	2397	2398	rBV	487	283	0.02%	0.003%
60	8.783	2398	2408	2441	rBV	611416	1005179	83.68%	10.509%
61	9.117	2508	2512	2515	rBV2	477	323	0.03%	0.003%
62	9.233	2545	2548	2553	rVB3	439	293	0.02%	0.003%
63	9.294	2564	2567	2570	rBV3	287	235	0.02%	0.002%
64	9.461	2616	2619	2622	rBV2	176	122	0.01%	0.001%
65	9.538	2640	2643	2647	rBV	197	198	0.02%	0.002%
66	9.580	2653	2656	2659	rVB	163	102	0.01%	0.001%
67	9.603	2659	2663	2666	rBV2	180	120	0.01%	0.001%
68	9.683	2685	2688	2691	rBV2	147	135	0.01%	0.001%
69	9.722	2697	2700	2703	rVB2	346	162	0.01%	0.002%
70	9.735	2703	2704	2707	rBV	180	89	0.01%	0.001%
71	9.850	2737	2740	2741	rBV	224	107	0.01%	0.001%
72	9.892	2749	2753	2756	rBV2	483	471	0.04%	0.005%
73	10.095	2813	2816	2818	rBV2	431	295	0.02%	0.003%
74	10.153	2818	2834	2859	rVV	385659	609883	50.77%	6.376%
75	10.329	2886	2889	2895	rVB3	556	451	0.04%	0.005%
76	10.374	2900	2903	2904	rBV	258	151	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031524\
 Data File : VV034666.D
 Acq On : 15 Mar 2024 20:41
 Operator : SY/MD
 Sample : P1740-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GH5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

77	10.471	2930	2933	2936	rVB3	190	105	0.01%	0.001%
78	10.493	2936	2940	2943	rBV2	382	342	0.03%	0.004%
79	10.580	2964	2967	2972	rBV2	266	152	0.01%	0.002%
80	10.603	2972	2974	2977	rVB2	181	103	0.01%	0.001%
81	10.622	2977	2980	2984	rBV	238	241	0.02%	0.003%
82	10.661	2989	2992	2995	rBV2	193	137	0.01%	0.001%
83	10.741	3014	3017	3019	rBV	159	101	0.01%	0.001%
84	10.789	3029	3032	3035	rVB	306	163	0.01%	0.002%
85	10.889	3060	3063	3071	rBV3	325	319	0.03%	0.003%
86	11.104	3126	3130	3134	rBV2	186	223	0.02%	0.002%
87	11.185	3144	3155	3183	rBV	584055	922976	76.83%	9.649%
88	11.558	3260	3271	3297	rBV	528580	851026	70.84%	8.897%
89	11.953	3387	3394	3396	rBV4	1085	1254	0.10%	0.013%
90	12.098	3437	3439	3443	rBV	191	156	0.01%	0.002%
91	12.226	3477	3479	3483	rBV	193	124	0.01%	0.001%
92	12.590	3591	3592	3593	rBV	379	89	0.01%	0.001%
93	12.754	3639	3643	3646	rBV	350	311	0.03%	0.003%
94	13.050	3732	3735	3741	rBV2	401	455	0.04%	0.005%
95	13.214	3780	3786	3787	rBV2	905	761	0.06%	0.008%
96	13.374	3834	3836	3838	rBV	395	175	0.01%	0.002%
97	13.410	3844	3847	3849	rBV	346	190	0.02%	0.002%
98	13.455	3855	3861	3876	rVB3	3403	5439	0.45%	0.057%
99	13.619	3911	3912	3916	rBV2	255	138	0.01%	0.001%
100	13.689	3928	3934	3942	rVB5	1362	1955	0.16%	0.020%




Sum of corrected areas: 9565122

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031524\
Data File : VV034666.D
Acq On : 15 Mar 2024 20:41
Operator : SY/MD
Sample : P1740-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GH5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

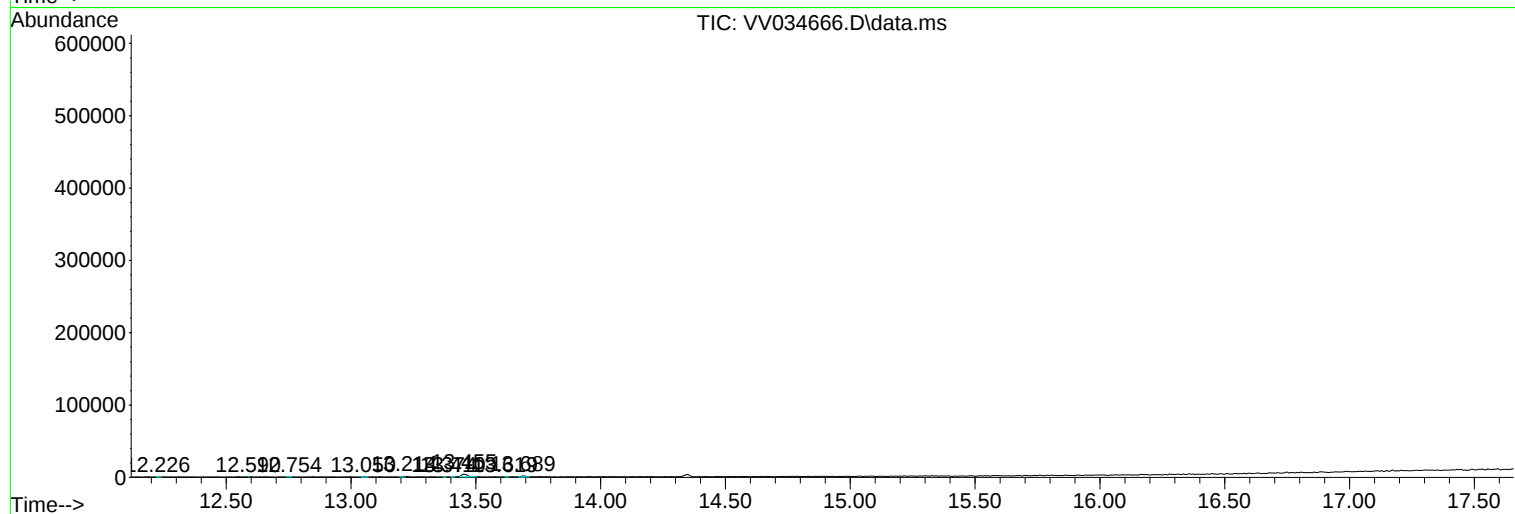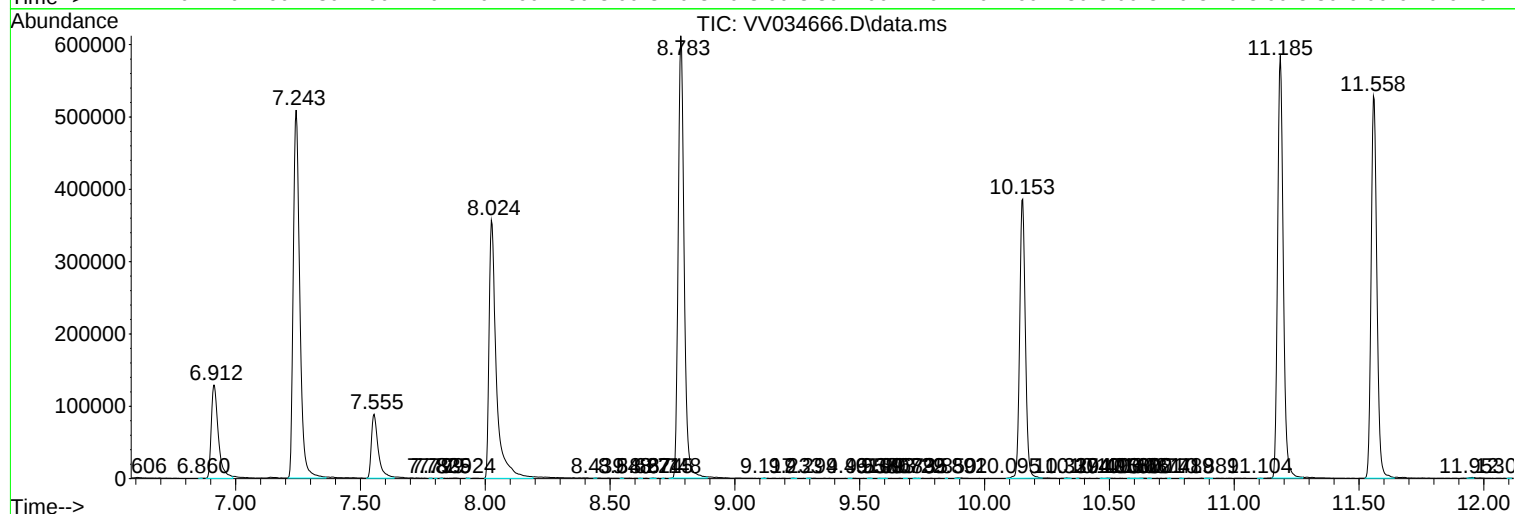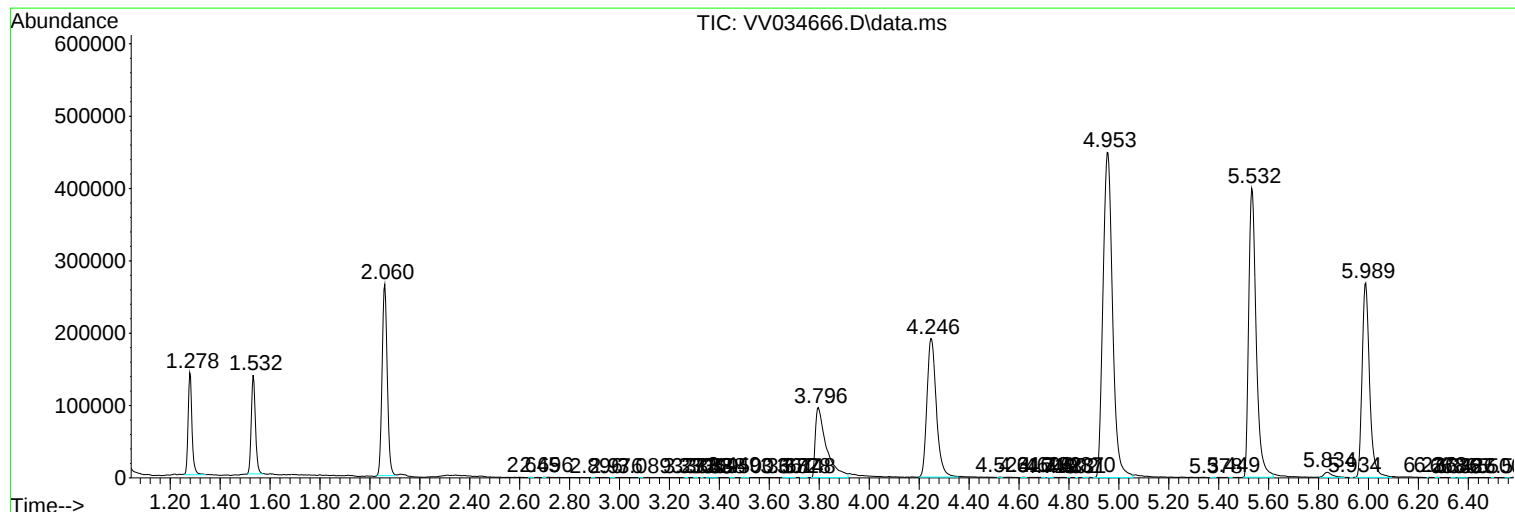

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031524\
Data File : VV034666.D
Acq On : 15 Mar 2024 20:41
Operator : SY/MD
Sample : P1740-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GH5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031524\
Data File : VV034666.D
Acq On : 15 Mar 2024 20:41
Operator : SY/MD
Sample : P1740-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GH5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc