

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031524\
 Data File : VV034671.D
 Acq On : 15 Mar 2024 22:40
 Operator : SY/MD
 Sample : P1740-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GJ2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

Signal : TIC: VV034671.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	94	rVB	139656	151493	12.83%	1.628%
2	1.529	145	152	168	rVB	135200	163758	13.87%	1.759%
3	2.056	306	316	331	rBV	260655	382598	32.40%	4.111%
4	2.481	445	448	449	rBV	318	131	0.01%	0.001%
5	2.523	459	461	465	rVB2	238	127	0.01%	0.001%
6	2.548	467	469	471	rBV2	441	258	0.02%	0.003%
7	2.661	503	504	505	rBV2	222	54	0.00%	0.001%
8	3.188	664	668	674	rBV	318	375	0.03%	0.004%
9	3.416	738	739	740	rVB	180	35	0.00%	0.000%
10	3.539	775	777	778	rBV	154	51	0.00%	0.001%
11	3.561	783	784	785	rVB	155	30	0.00%	0.000%
12	3.571	785	787	791	rBV	175	134	0.01%	0.001%
13	3.677	815	820	822	rBV2	164	157	0.01%	0.002%
14	3.703	826	828	832	rBV2	127	82	0.01%	0.001%
15	3.738	835	839	842	rBV2	255	140	0.01%	0.002%
16	3.789	846	855	888	rBV2	102336	291465	24.68%	3.132%
17	4.249	983	998	1030	rBV	190175	484913	41.06%	5.210%
18	4.571	1096	1098	1099	rBV	231	82	0.01%	0.001%
19	4.625	1113	1115	1116	rBV	163	62	0.01%	0.001%
20	4.696	1134	1137	1139	rBV	182	121	0.01%	0.001%
21	4.709	1139	1141	1144	rVB2	282	129	0.01%	0.001%
22	4.735	1144	1149	1152	rBV2	402	408	0.03%	0.004%
23	4.953	1199	1217	1255	rBV2	443796	1180962	100.00%	12.689%
24	5.252	1308	1310	1312	rBV2	441	249	0.02%	0.003%
25	5.368	1345	1346	1349	rVB	249	67	0.01%	0.001%
26	5.532	1386	1397	1430	rBV	398214	822911	69.68%	8.842%
27	5.834	1482	1491	1503	rBV4	6662	13293	1.13%	0.143%
28	5.940	1521	1524	1526	rBV2	372	197	0.02%	0.002%
29	5.989	1526	1539	1570	rBV	261156	543545	46.03%	5.840%
30	6.256	1619	1622	1623	rBV	227	116	0.01%	0.001%
31	6.371	1656	1658	1660	rBV2	191	70	0.01%	0.001%
32	6.387	1661	1663	1665	rVB	263	88	0.01%	0.001%
33	6.439	1674	1679	1680	rBV	210	134	0.01%	0.001%
34	6.490	1693	1695	1698	rBV2	269	142	0.01%	0.002%
35	6.593	1718	1727	1731	rBV5	885	1310	0.11%	0.014%
36	6.812	1792	1795	1796	rBV	159	68	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031524\
 Data File : VV034671.D
 Acq On : 15 Mar 2024 22:40
 Operator : SY/MD
 Sample : P1740-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GJ2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	6.866	1810	1812	1814	rBV	206	118	0.01%	0.001%
38	6.915	1816	1827	1864	rVV	124574	244853	20.73%	2.631%
39	7.149	1890	1900	1903	rBV5	953	1685	0.14%	0.018%
40	7.243	1918	1929	1955	rBV	498666	879650	74.49%	9.451%
41	7.555	2016	2026	2050	rBV	85216	160989	13.63%	1.730%
42	7.789	2097	2099	2104	rBV3	338	262	0.02%	0.003%
43	7.812	2104	2106	2107	rBV	148	65	0.01%	0.001%
44	7.931	2141	2143	2148	rBV2	242	178	0.02%	0.002%
45	8.024	2163	2172	2221	rBV	358681	687306	58.20%	7.385%
46	8.609	2350	2354	2355	rBV2	208	132	0.01%	0.001%
47	8.686	2376	2378	2381	rBV2	242	173	0.01%	0.002%
48	8.783	2397	2408	2434	rBV	589475	982886	83.23%	10.560%
49	9.066	2490	2496	2502	rVB3	365	494	0.04%	0.005%
50	9.098	2503	2506	2507	rBV3	189	104	0.01%	0.001%
51	9.130	2513	2516	2521	rVB2	280	201	0.02%	0.002%
52	9.188	2532	2534	2536	rBV	183	82	0.01%	0.001%
53	9.239	2548	2550	2552	rBV	157	79	0.01%	0.001%
54	9.284	2562	2564	2567	rVB	159	75	0.01%	0.001%
55	9.403	2598	2601	2608	rBV2	209	249	0.02%	0.003%
56	9.503	2631	2632	2633	rBV2	113	27	0.00%	0.000%
57	9.635	2670	2673	2676	rBV2	216	167	0.01%	0.002%
58	9.722	2698	2700	2703	rVB	309	175	0.01%	0.002%
59	9.747	2704	2708	2711	rVV3	329	234	0.02%	0.003%
60	9.799	2723	2724	2725	rBV	102	24	0.00%	0.000%
61	9.808	2725	2727	2728	rBV	168	55	0.00%	0.001%
62	10.005	2786	2788	2790	rBV2	114	65	0.01%	0.001%
63	10.043	2795	2800	2801	rBV	324	262	0.02%	0.003%
64	10.088	2813	2814	2816	rVB	138	51	0.00%	0.001%
65	10.153	2822	2834	2860	rBV	373449	588450	49.83%	6.322%
66	10.522	2945	2949	2955	rBV2	190	244	0.02%	0.003%
67	10.699	3000	3004	3008	rBV2	339	217	0.02%	0.002%
68	10.789	3029	3032	3037	rBV2	269	244	0.02%	0.003%
69	11.079	3121	3122	3123	rBV	295	72	0.01%	0.001%
70	11.185	3144	3155	3181	rBV	577557	893947	75.70%	9.605%
71	11.500	3250	3253	3256	rBV	226	142	0.01%	0.002%
72	11.561	3260	3272	3296	rBV	520866	821756	69.58%	8.829%
73	11.934	3386	3388	3389	rBV	248	113	0.01%	0.001%
74	12.001	3407	3409	3413	rVB2	323	177	0.01%	0.002%
75	12.021	3413	3415	3419	rBV	206	134	0.01%	0.001%
76	12.410	3534	3536	3537	rBV	314	103	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031524\
Data File : VV034671.D
Acq On : 15 Mar 2024 22:40
Operator : SY/MD
Sample : P1740-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GJ2

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Title : VOC Analysis

77	12.947	3701	3703	3707	rBV2	296	188	0.02%	0.002%
78	13.715	3940	3942	3944	rBV	274	126	0.01%	0.001%
79	14.117	4060	4067	4070	rBV4	747	991	0.08%	0.011%




Sum of corrected areas: 9307300

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031524\
Data File : VV034671.D
Acq On : 15 Mar 2024 22:40
Operator : SY/MD
Sample : P1740-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GJ2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

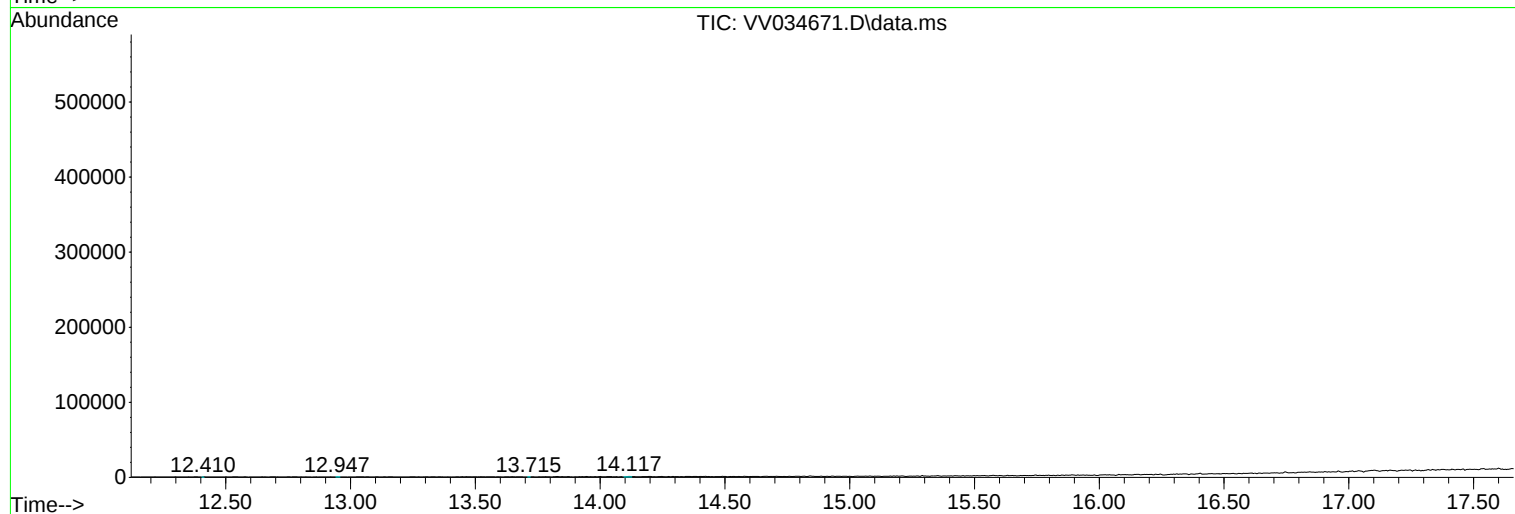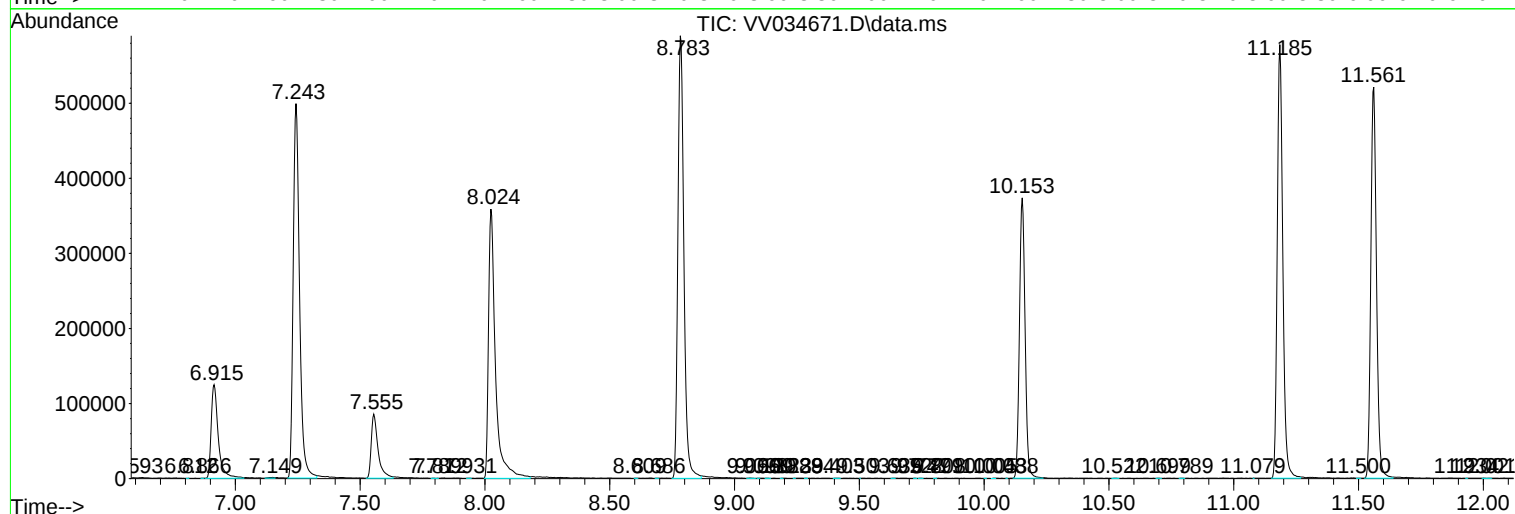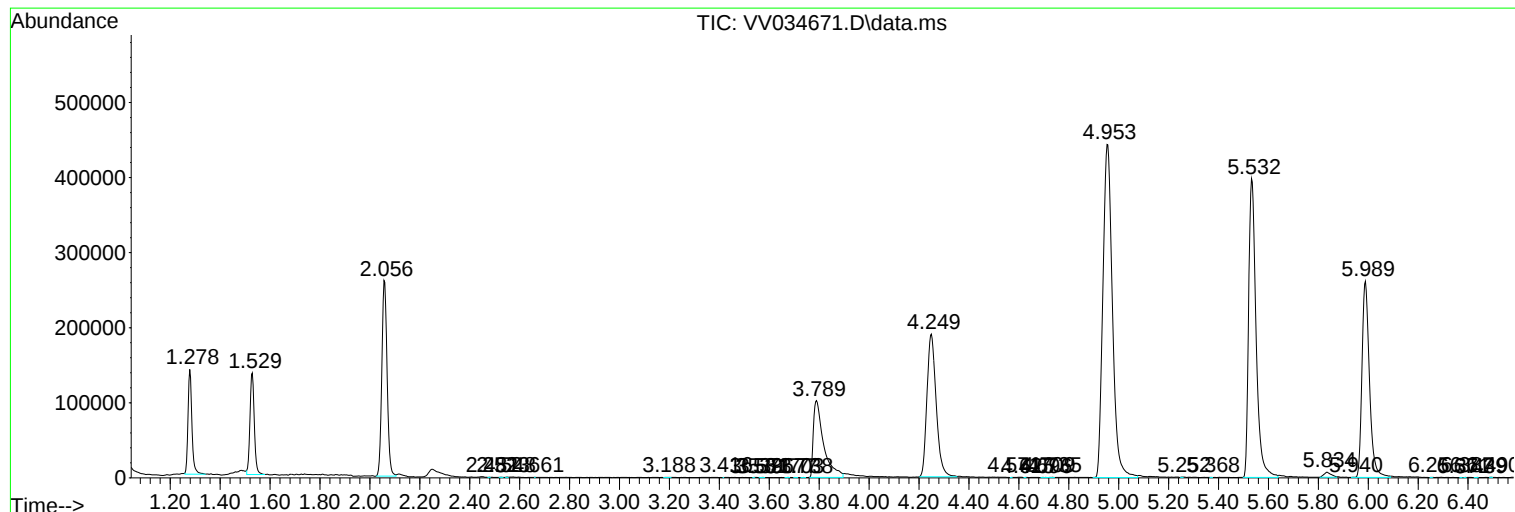

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031524\
Data File : VV034671.D
Acq On : 15 Mar 2024 22:40
Operator : SY/MD
Sample : P1740-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GJ2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031524\
Data File : VV034671.D
Acq On : 15 Mar 2024 22:40
Operator : SY/MD
Sample : P1740-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GJ2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc