

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031524\
 Data File : VV034675.D
 Acq On : 16 Mar 2024 00:16
 Operator : SY/MD
 Sample : P1740-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GJ8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

Signal : TIC: VV034675.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	90	rVB	138824	145383	12.00%	1.507%
2	1.529	145	152	168	rVB	137279	165426	13.65%	1.715%
3	2.056	307	316	330	rBV	261768	380344	31.38%	3.942%
4	2.256	364	378	395	rBV2	9830	35176	2.90%	0.365%
5	2.683	508	511	512	rBV2	315	173	0.01%	0.002%
6	3.159	657	659	662	rVB	225	89	0.01%	0.001%
7	3.204	670	673	679	rBV2	132	155	0.01%	0.002%
8	3.423	737	741	744	rBV2	231	220	0.02%	0.002%
9	3.641	806	809	816	rVB	164	171	0.01%	0.002%
10	3.674	816	819	823	rBV	192	184	0.02%	0.002%
11	3.789	846	855	896	rBV2	108426	312917	25.82%	3.243%
12	4.249	983	998	1032	rBV	192300	495816	40.91%	5.139%
13	4.580	1098	1101	1102	rBV2	370	208	0.02%	0.002%
14	4.625	1112	1115	1119	rBV3	501	376	0.03%	0.004%
15	4.699	1135	1138	1139	rBV	274	149	0.01%	0.002%
16	4.725	1144	1146	1151	rVB2	207	126	0.01%	0.001%
17	4.780	1160	1163	1165	rBV3	183	116	0.01%	0.001%
18	4.815	1168	1174	1175	rBV3	196	197	0.02%	0.002%
19	4.899	1198	1200	1201	rBV	319	96	0.01%	0.001%
20	4.953	1201	1217	1256	rBV2	453877	1211940	100.00%	12.561%
21	5.352	1338	1341	1344	rBV	295	220	0.02%	0.002%
22	5.474	1374	1379	1383	rBV3	319	310	0.03%	0.003%
23	5.532	1387	1397	1427	rBV	407243	837430	69.10%	8.679%
24	5.767	1468	1470	1472	rBV2	288	128	0.01%	0.001%
25	5.780	1472	1474	1477	rVV	454	277	0.02%	0.003%
26	5.841	1480	1493	1518	rVB5	29673	73306	6.05%	0.760%
27	5.989	1526	1539	1567	rBV	266720	557534	46.00%	5.779%
28	6.249	1618	1620	1622	rVV2	233	105	0.01%	0.001%
29	6.259	1622	1623	1628	rVB	266	136	0.01%	0.001%
30	6.355	1650	1653	1656	rBV2	331	212	0.02%	0.002%
31	6.381	1658	1661	1663	rVB	386	178	0.01%	0.002%
32	6.410	1666	1670	1675	rBV2	208	253	0.02%	0.003%
33	6.436	1675	1678	1680	rBV	194	100	0.01%	0.001%
34	6.516	1701	1703	1714	rVB2	148	197	0.02%	0.002%
35	6.593	1719	1727	1728	rBV4	1103	1119	0.09%	0.012%
36	6.719	1763	1766	1769	rVB3	264	160	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031524\
 Data File : VV034675.D
 Acq On : 16 Mar 2024 00:16
 Operator : SY/MD
 Sample : P1740-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GJ8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	6.738	1769	1772	1775	rBV	251	190	0.02%	0.002%
38	6.850	1801	1807	1810	rBV2	190	178	0.01%	0.002%
39	6.915	1816	1827	1853	rBV	130052	250434	20.66%	2.596%
40	7.143	1892	1898	1906	rBV6	1457	2191	0.18%	0.023%
41	7.243	1918	1929	1963	rBV	503951	900713	74.32%	9.335%
42	7.503	2008	2010	2013	rBV3	251	151	0.01%	0.002%
43	7.555	2016	2026	2056	rBV	88674	165924	13.69%	1.720%
44	7.821	2106	2109	2112	rBV2	208	156	0.01%	0.002%
45	7.879	2119	2127	2133	rVV3	397	551	0.05%	0.006%
46	8.024	2163	2172	2215	rBV	370616	726519	59.95%	7.530%
47	8.471	2309	2311	2313	rVB2	230	99	0.01%	0.001%
48	8.490	2313	2317	2322	rVB2	254	237	0.02%	0.002%
49	8.516	2322	2325	2328	rBV3	298	203	0.02%	0.002%
50	8.609	2350	2354	2356	rBV	205	170	0.01%	0.002%
51	8.622	2356	2358	2361	rVV2	347	185	0.02%	0.002%
52	8.648	2362	2366	2370	rVB3	576	477	0.04%	0.005%
53	8.693	2377	2380	2384	rBV2	335	182	0.02%	0.002%
54	8.715	2384	2387	2388	rBV	303	160	0.01%	0.002%
55	8.744	2393	2396	2397	rBV	257	133	0.01%	0.001%
56	8.783	2397	2408	2441	rBV	614679	1015947	83.83%	10.530%
57	9.043	2486	2489	2490	rBV2	255	119	0.01%	0.001%
58	9.095	2501	2505	2508	rBV4	400	396	0.03%	0.004%
59	9.127	2512	2515	2518	rBV	357	228	0.02%	0.002%
60	9.143	2518	2520	2525	rVV2	286	173	0.01%	0.002%
61	9.207	2536	2540	2543	rBV	294	162	0.01%	0.002%
62	9.265	2554	2558	2560	rBV2	180	134	0.01%	0.001%
63	9.313	2570	2573	2575	rVB2	234	112	0.01%	0.001%
64	9.407	2599	2602	2605	rBV	297	175	0.01%	0.002%
65	9.509	2631	2634	2637	rBV2	144	129	0.01%	0.001%
66	9.754	2706	2710	2713	rBV2	250	218	0.02%	0.002%
67	9.773	2714	2716	2720	rVB2	267	128	0.01%	0.001%
68	9.799	2720	2724	2726	rBV2	296	245	0.02%	0.003%
69	9.863	2742	2744	2749	rVB	229	136	0.01%	0.001%
70	9.889	2749	2752	2756	rVB	210	133	0.01%	0.001%
71	9.918	2756	2761	2763	rBV2	249	213	0.02%	0.002%
72	9.956	2770	2773	2777	rVB	180	117	0.01%	0.001%
73	10.021	2789	2793	2798	rBV	180	176	0.01%	0.002%
74	10.069	2806	2808	2812	rBV	234	157	0.01%	0.002%
75	10.152	2822	2834	2859	rBV	383415	611022	50.42%	6.333%
76	10.378	2899	2904	2907	rBV2	207	225	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031524\
 Data File : VV034675.D
 Acq On : 16 Mar 2024 00:16
 Operator : SY/MD
 Sample : P1740-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GJ8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

77	10.532	2949	2952	2956	rBV	146	101	0.01%	0.001%
78	10.715	3007	3009	3011	rBV2	224	129	0.01%	0.001%
79	10.934	3073	3077	3079	rBV2	262	212	0.02%	0.002%
80	11.011	3098	3101	3104	rBV2	249	132	0.01%	0.001%
81	11.053	3108	3114	3116	rBV2	209	197	0.02%	0.002%
82	11.185	3144	3155	3176	rBV	590269	909049	75.01%	9.422%
83	11.490	3248	3250	3255	rVB2	379	229	0.02%	0.002%
84	11.561	3260	3272	3300	rBV	528453	834331	68.84%	8.647%
85	11.892	3373	3375	3376	rBV	332	151	0.01%	0.002%
86	12.143	3451	3453	3459	rVB2	319	203	0.02%	0.002%
87	12.175	3459	3463	3466	rBV2	271	241	0.02%	0.002%
88	12.329	3508	3511	3514	rBV	349	169	0.01%	0.002%
89	12.397	3530	3532	3535	rVB2	255	113	0.01%	0.001%
90	12.567	3581	3585	3587	rVB	315	187	0.02%	0.002%
91	12.596	3592	3594	3596	rBV	308	148	0.01%	0.002%
92	12.641	3604	3608	3612	rBV2	239	242	0.02%	0.003%
93	12.802	3655	3658	3661	rBV3	335	250	0.02%	0.003%
94	13.024	3724	3727	3731	rBV2	270	207	0.02%	0.002%
95	13.043	3731	3733	3737	rBV2	205	129	0.01%	0.001%
96	13.377	3833	3837	3838	rBV	297	217	0.02%	0.002%
97	13.609	3906	3909	3915	rVB	708	610	0.05%	0.006%
98	13.738	3948	3949	3950	rVB	598	115	0.01%	0.001%
99	14.049	4044	4046	4048	rBV2	398	216	0.02%	0.002%
100	14.834	4288	4290	4294	rBV	876	668	0.06%	0.007%




Sum of corrected areas: 9648371

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031524\
Data File : VV034675.D
Acq On : 16 Mar 2024 00:16
Operator : SY/MD
Sample : P1740-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GJ8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

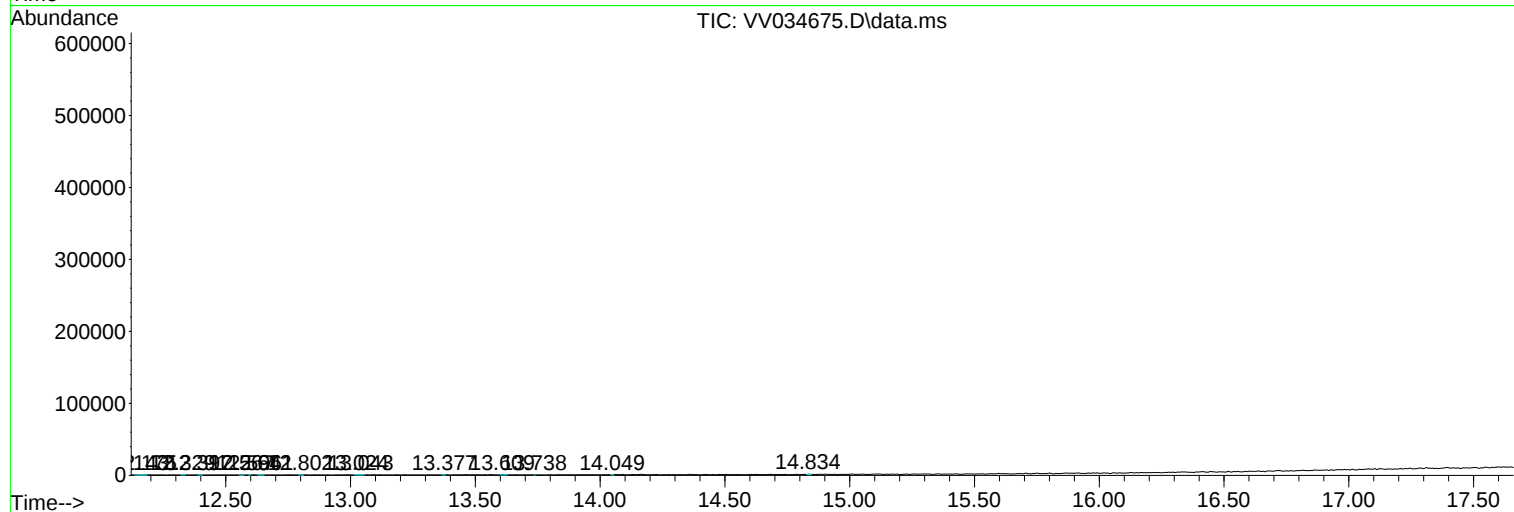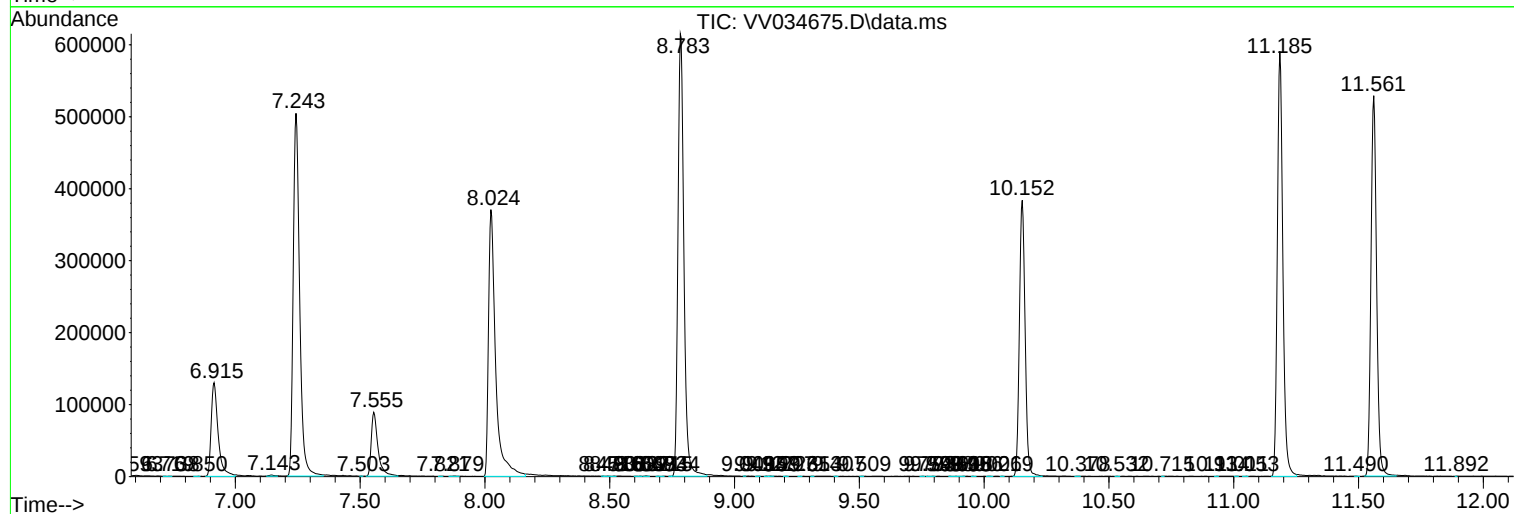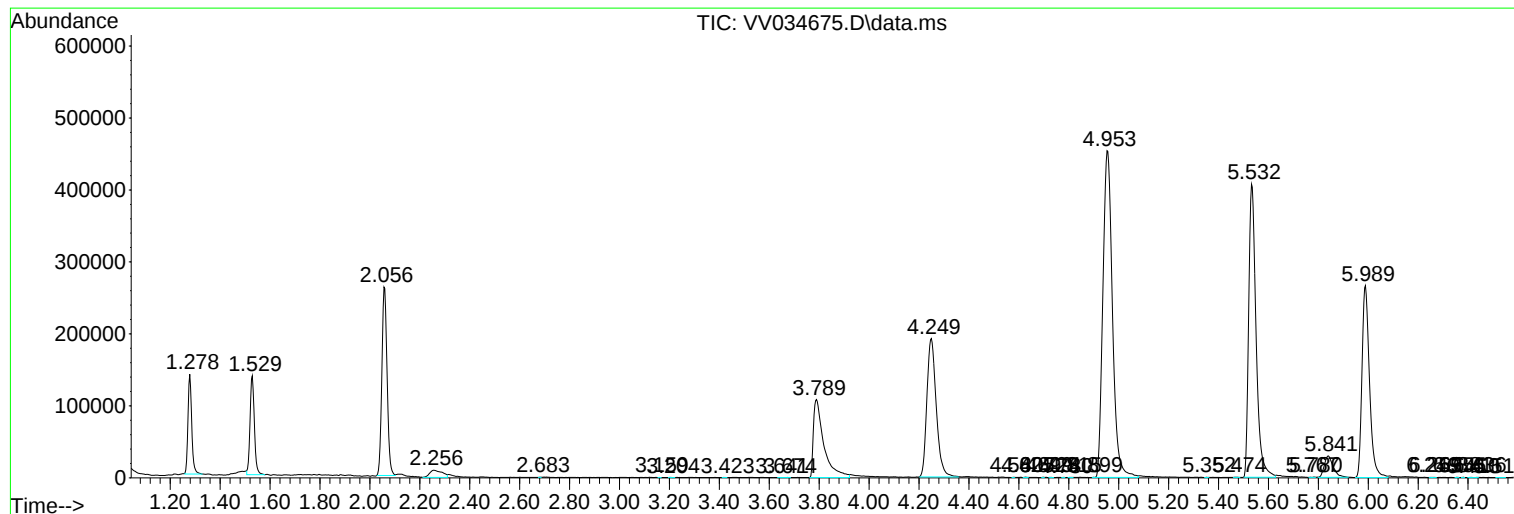

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031524\
Data File : VV034675.D
Acq On : 16 Mar 2024 00:16
Operator : SY/MD
Sample : P1740-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GJ8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031524\
Data File : VV034675.D
Acq On : 16 Mar 2024 00:16
Operator : SY/MD
Sample : P1740-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GJ8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------