

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031524\
 Data File : VV034676.D
 Acq On : 16 Mar 2024 00:40
 Operator : SY/MD
 Sample : P1740-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GK0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

Signal : TIC: VV034676.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	91	rVB	140688	149289	12.28%	1.537%
2	1.529	146	152	170	rVB	140596	166417	13.69%	1.713%
3	2.060	306	317	331	rBV2	286206	436596	35.91%	4.495%
4	2.445	431	437	440	rBV4	1248	1258	0.10%	0.013%
5	2.793	544	545	548	rVB2	270	69	0.01%	0.001%
6	3.069	627	631	636	rBV2	206	254	0.02%	0.003%
7	3.169	661	662	665	rVB2	211	82	0.01%	0.001%
8	3.185	665	667	671	rVB2	115	71	0.01%	0.001%
9	3.220	671	678	680	rBV	305	320	0.03%	0.003%
10	3.371	722	725	728	rBV	176	109	0.01%	0.001%
11	3.461	751	753	754	rBV	109	51	0.00%	0.001%
12	3.519	767	771	773	rBV	265	175	0.01%	0.002%
13	3.574	781	788	790	rBV2	243	257	0.02%	0.003%
14	3.699	826	827	828	rBV2	140	43	0.00%	0.000%
15	3.728	833	836	839	rBV2	162	109	0.01%	0.001%
16	3.789	846	855	894	rBV	116414	370493	30.47%	3.814%
17	4.249	981	998	1032	rBV	197798	509362	41.89%	5.244%
18	4.519	1069	1082	1101	rVB3	8866	22681	1.87%	0.233%
19	4.732	1145	1148	1149	rBV2	393	219	0.02%	0.002%
20	4.844	1181	1183	1185	rBV2	186	110	0.01%	0.001%
21	4.953	1201	1217	1250	rBV2	456178	1215940	100.00%	12.518%
22	5.410	1356	1359	1364	rVB4	480	395	0.03%	0.004%
23	5.432	1364	1366	1370	rVB3	393	208	0.02%	0.002%
24	5.452	1370	1372	1374	rBV	188	102	0.01%	0.001%
25	5.465	1374	1376	1382	rVB3	363	324	0.03%	0.003%
26	5.532	1386	1397	1428	rBV	402676	829972	68.26%	8.544%
27	5.834	1481	1491	1508	rBV5	9332	21279	1.75%	0.219%
28	5.989	1526	1539	1569	rBV	270133	557341	45.84%	5.738%
29	6.249	1618	1620	1621	rBV2	159	47	0.00%	0.000%
30	6.265	1621	1625	1627	rBV2	297	197	0.02%	0.002%
31	6.313	1639	1640	1643	rVB	331	156	0.01%	0.002%
32	6.349	1648	1651	1653	rBV	144	93	0.01%	0.001%
33	6.426	1673	1675	1682	rVB2	315	217	0.02%	0.002%
34	6.481	1689	1692	1694	rBV2	236	120	0.01%	0.001%
35	6.542	1709	1711	1717	rBV2	113	110	0.01%	0.001%
36	6.587	1717	1725	1726	rBV2	921	915	0.08%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031524\
 Data File : VV034676.D
 Acq On : 16 Mar 2024 00:40
 Operator : SY/MD
 Sample : P1740-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GK0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	6.764	1778	1780	1781	rBV2	225	87	0.01%	0.001%
38	6.776	1781	1784	1786	rVB2	208	99	0.01%	0.001%
39	6.857	1807	1809	1811	rVB	238	93	0.01%	0.001%
40	6.873	1811	1814	1816	rBV	176	108	0.01%	0.001%
41	6.915	1816	1827	1855	rBV	131493	254940	20.97%	2.625%
42	7.243	1918	1929	1963	rBV	514554	908465	74.71%	9.352%
43	7.555	2017	2026	2061	rBV2	92076	169320	13.93%	1.743%
44	7.786	2094	2098	2100	rVB	759	505	0.04%	0.005%
45	7.805	2100	2104	2106	rVB2	312	246	0.02%	0.003%
46	7.831	2110	2112	2115	rVB3	234	123	0.01%	0.001%
47	7.850	2115	2118	2119	rBV2	245	118	0.01%	0.001%
48	7.934	2139	2144	2147	rBV2	219	154	0.01%	0.002%
49	7.973	2151	2156	2159	rBV2	313	319	0.03%	0.003%
50	8.024	2163	2172	2210	rBV	377902	728439	59.91%	7.499%
51	8.413	2291	2293	2296	rBV2	335	192	0.02%	0.002%
52	8.638	2362	2363	2365	rBV	219	90	0.01%	0.001%
53	8.674	2371	2374	2376	rBV2	151	102	0.01%	0.001%
54	8.722	2387	2389	2397	rVB3	497	409	0.03%	0.004%
55	8.783	2397	2408	2442	rBV	596946	992485	81.62%	10.217%
56	9.050	2489	2491	2492	rBV	292	96	0.01%	0.001%
57	9.079	2497	2500	2501	rBV	288	168	0.01%	0.002%
58	9.162	2524	2526	2528	rBV	315	172	0.01%	0.002%
59	9.336	2577	2580	2581	rBV	169	86	0.01%	0.001%
60	9.365	2587	2589	2592	rVB	155	62	0.01%	0.001%
61	9.384	2592	2595	2597	rBV2	136	77	0.01%	0.001%
62	9.400	2597	2600	2601	rBV2	138	72	0.01%	0.001%
63	9.419	2603	2606	2609	rVB2	212	132	0.01%	0.001%
64	9.484	2625	2626	2629	rVB2	211	60	0.00%	0.001%
65	9.503	2630	2632	2634	rVV2	188	75	0.01%	0.001%
66	9.516	2634	2636	2643	rVB2	134	98	0.01%	0.001%
67	9.558	2643	2649	2653	rVB	265	283	0.02%	0.003%
68	9.583	2653	2657	2660	rBV2	480	278	0.02%	0.003%
69	9.751	2708	2709	2712	rVB	183	65	0.01%	0.001%
70	9.837	2734	2736	2738	rBV2	260	87	0.01%	0.001%
71	9.889	2750	2752	2755	rBV	208	108	0.01%	0.001%
72	9.934	2761	2766	2769	rBV2	276	254	0.02%	0.003%
73	9.966	2772	2776	2778	rBV2	182	155	0.01%	0.002%
74	10.037	2797	2798	2799	rBV2	139	40	0.00%	0.000%
75	10.088	2808	2814	2816	rBV2	182	143	0.01%	0.001%
76	10.153	2818	2834	2857	rBV	390626	614886	50.57%	6.330%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031524\
 Data File : VV034676.D
 Acq On : 16 Mar 2024 00:40
 Operator : SY/MD
 Sample : P1740-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GK0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

77	10.355	2894	2897	2905	rVB2	418	373	0.03%	0.004%
78	10.390	2905	2908	2910	rBV2	133	95	0.01%	0.001%
79	10.509	2942	2945	2947	rBV2	156	95	0.01%	0.001%
80	10.526	2947	2950	2952	rBV	224	133	0.01%	0.001%
81	10.738	3014	3016	3017	rBV	170	58	0.00%	0.001%
82	10.834	3043	3046	3054	rVB3	376	368	0.03%	0.004%
83	10.902	3064	3067	3073	rVB2	185	164	0.01%	0.002%
84	11.059	3112	3116	3119	rBV2	186	165	0.01%	0.002%
85	11.088	3122	3125	3127	rBV	136	100	0.01%	0.001%
86	11.185	3144	3155	3184	rBV	579910	906324	74.54%	9.330%
87	11.474	3239	3245	3247	rVB2	358	312	0.03%	0.003%
88	11.487	3247	3249	3253	rBV2	172	118	0.01%	0.001%
89	11.561	3260	3272	3292	rBV	528564	843866	69.40%	8.687%
90	11.844	3358	3360	3362	rVB	349	140	0.01%	0.001%
91	11.947	3390	3392	3395	rVB	363	149	0.01%	0.002%
92	12.056	3423	3426	3428	rBV	223	151	0.01%	0.002%
93	12.333	3509	3512	3514	rBV2	325	164	0.01%	0.002%
94	12.493	3560	3562	3567	rVB2	460	258	0.02%	0.003%
95	12.606	3595	3597	3600	rBV3	293	179	0.01%	0.002%
96	12.712	3628	3630	3631	rBV	145	44	0.00%	0.000%
97	13.120	3751	3757	3762	rBV4	447	620	0.05%	0.006%
98	13.181	3773	3776	3780	rBV	320	291	0.02%	0.003%
99	13.468	3862	3865	3866	rBV3	252	171	0.01%	0.002%
100	13.757	3952	3955	3957	rBV2	392	229	0.02%	0.002%




Sum of corrected areas: 9713639

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031524\
Data File : VV034676.D
Acq On : 16 Mar 2024 00:40
Operator : SY/MD
Sample : P1740-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GK0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

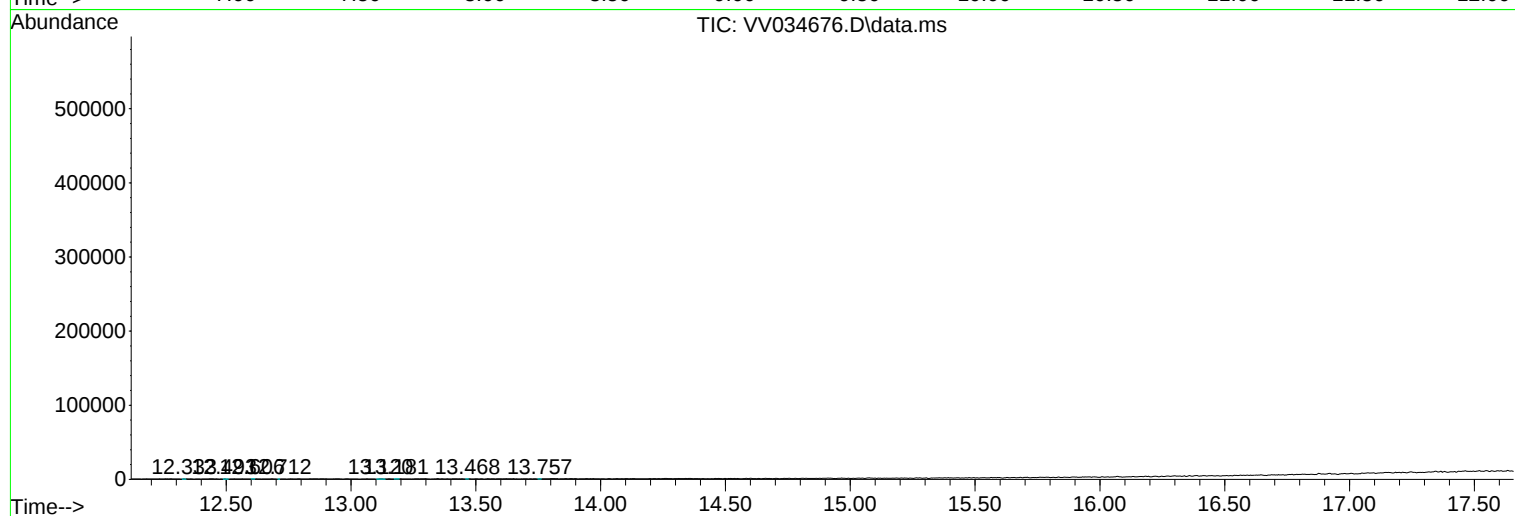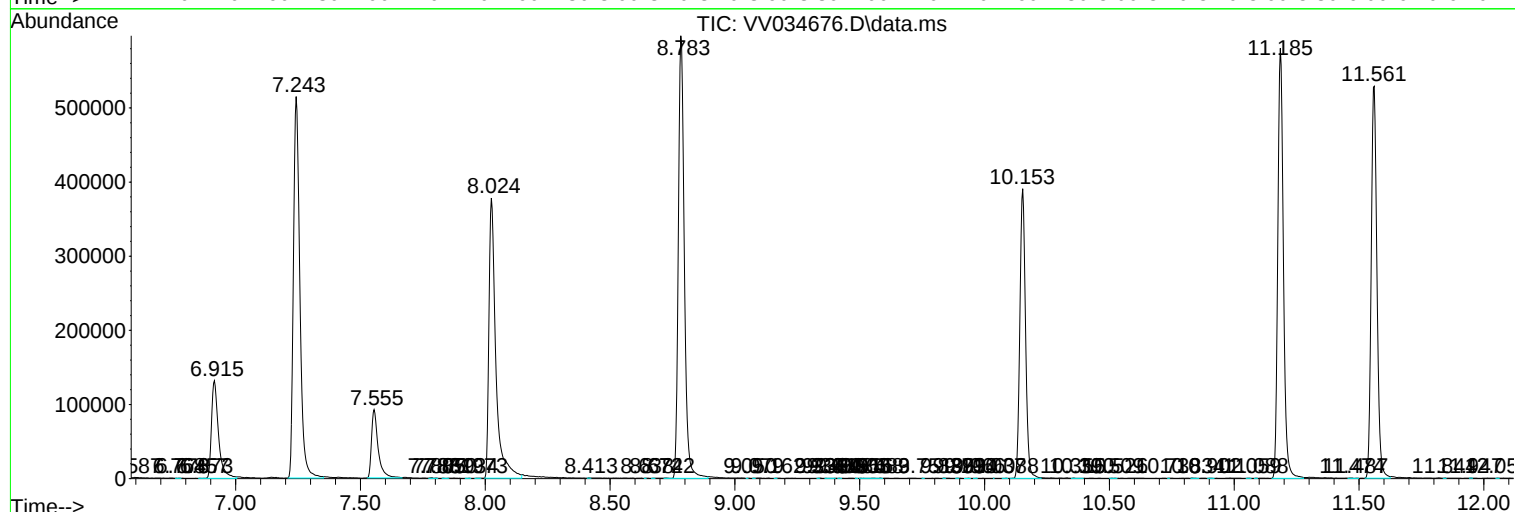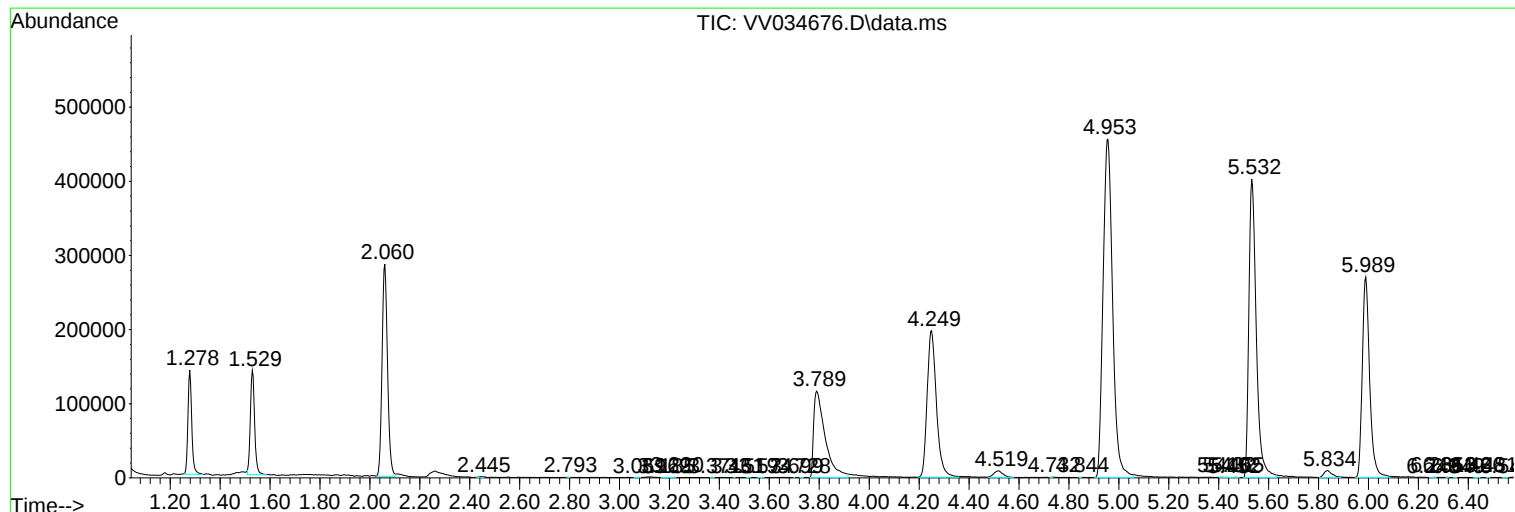

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031524\
Data File : VV034676.D
Acq On : 16 Mar 2024 00:40
Operator : SY/MD
Sample : P1740-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GK0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031524\
Data File : VV034676.D
Acq On : 16 Mar 2024 00:40
Operator : SY/MD
Sample : P1740-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GK0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
