

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031524\
 Data File : VV034678.D
 Acq On : 16 Mar 2024 01:28
 Operator : SY/MD
 Sample : P1740-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GK3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

Signal : TIC: VV034678.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	96	rVB	104427	115352	10.30%	1.317%
2	1.526	145	151	174	rVB	122190	153231	13.68%	1.750%
3	2.056	307	316	330	rBV2	204661	300810	26.86%	3.435%
4	2.442	431	436	440	rBV6	1698	1799	0.16%	0.021%
5	2.536	464	465	468	rVB2	258	111	0.01%	0.001%
6	2.558	468	472	477	rBV3	528	401	0.04%	0.005%
7	2.626	490	493	498	rBV2	332	268	0.02%	0.003%
8	2.703	514	517	518	rBV2	286	195	0.02%	0.002%
9	2.825	554	555	557	rBV2	297	130	0.01%	0.001%
10	2.899	573	578	582	rBV2	293	309	0.03%	0.004%
11	2.950	591	594	597	rBV2	254	217	0.02%	0.002%
12	2.986	603	605	610	rVB	233	155	0.01%	0.002%
13	3.021	610	616	620	rBV2	249	278	0.02%	0.003%
14	3.044	620	623	626	rBV2	212	160	0.01%	0.002%
15	3.214	674	676	681	rVB2	274	113	0.01%	0.001%
16	3.294	696	701	704	rBV2	216	161	0.01%	0.002%
17	3.336	711	714	717	rBV	163	110	0.01%	0.001%
18	3.372	721	725	728	rBV	301	242	0.02%	0.003%
19	3.394	729	732	739	rVB2	279	284	0.03%	0.003%
20	3.429	739	743	750	rBV2	301	351	0.03%	0.004%
21	3.632	802	806	808	rBV	277	152	0.01%	0.002%
22	3.687	820	823	824	rBV	202	107	0.01%	0.001%
23	3.725	829	835	840	rBV2	147	226	0.02%	0.003%
24	3.793	847	856	920	rBV	108976	348063	31.08%	3.975%
25	4.249	983	998	1024	rBV	180614	461730	41.23%	5.273%
26	4.462	1062	1064	1066	rBV	314	142	0.01%	0.002%
27	4.548	1088	1091	1094	rBV4	314	230	0.02%	0.003%
28	4.699	1134	1138	1139	rBV	179	122	0.01%	0.001%
29	4.738	1146	1150	1153	rBV2	204	217	0.02%	0.002%
30	4.860	1186	1188	1192	rVB2	363	183	0.02%	0.002%
31	4.886	1192	1196	1198	rBV3	397	217	0.02%	0.002%
32	4.953	1201	1217	1251	rBV2	423241	1119882	100.00%	12.789%
33	5.461	1372	1375	1378	rVB2	265	180	0.02%	0.002%
34	5.481	1378	1381	1382	rBV2	228	125	0.01%	0.001%
35	5.532	1386	1397	1436	rBV	365890	758871	67.76%	8.666%
36	5.838	1480	1492	1513	rBV9	11800	29509	2.64%	0.337%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031524\
 Data File : VV034678.D
 Acq On : 16 Mar 2024 01:28
 Operator : SY/MD
 Sample : P1740-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GK3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	5.941	1519	1524	1526	rBV3	579	620	0.06%	0.007%
38	5.989	1526	1539	1568	rVV	250840	526853	47.05%	6.017%
39	6.230	1613	1614	1622	rVB2	311	332	0.03%	0.004%
40	6.265	1622	1625	1627	rBV2	282	224	0.02%	0.003%
41	6.336	1643	1647	1648	rBV	352	217	0.02%	0.002%
42	6.568	1714	1719	1720	rBV	107	103	0.01%	0.001%
43	6.596	1720	1728	1731	rBV4	1098	1624	0.15%	0.019%
44	6.677	1751	1753	1758	rVB5	445	242	0.02%	0.003%
45	6.732	1766	1770	1772	rBV2	251	179	0.02%	0.002%
46	6.860	1805	1810	1813	rBV2	149	168	0.02%	0.002%
47	6.915	1817	1827	1856	rBV	122966	239531	21.39%	2.735%
48	7.143	1890	1898	1900	rBV4	1466	1680	0.15%	0.019%
49	7.243	1918	1929	1960	rBV	453251	808672	72.21%	9.235%
50	7.555	2016	2026	2057	rBV	86138	161331	14.41%	1.842%
51	7.793	2098	2100	2103	rBV2	252	117	0.01%	0.001%
52	7.831	2110	2112	2114	rBV2	308	154	0.01%	0.002%
53	7.915	2135	2138	2139	rBV	221	128	0.01%	0.001%
54	8.027	2163	2173	2210	rBV	368703	723423	64.60%	8.262%
55	8.455	2302	2306	2309	rBV3	415	308	0.03%	0.004%
56	8.522	2324	2327	2329	rBV	337	267	0.02%	0.003%
57	8.600	2348	2351	2355	rBV	294	181	0.02%	0.002%
58	8.638	2361	2363	2368	rBV3	240	103	0.01%	0.001%
59	8.748	2395	2397	2398	rBV	199	103	0.01%	0.001%
60	8.783	2398	2408	2439	rVV	541245	894932	79.91%	10.220%
61	9.047	2488	2490	2493	rVB2	258	119	0.01%	0.001%
62	9.069	2493	2497	2500	rBV	306	229	0.02%	0.003%
63	9.085	2500	2502	2508	rVV3	320	301	0.03%	0.003%
64	9.124	2510	2514	2516	rBV2	136	111	0.01%	0.001%
65	9.452	2611	2616	2619	rBV2	167	184	0.02%	0.002%
66	9.484	2622	2626	2630	rVB2	235	238	0.02%	0.003%
67	9.538	2640	2643	2646	rBV	142	130	0.01%	0.001%
68	9.992	2777	2784	2786	rBV	248	252	0.02%	0.003%
69	10.056	2801	2804	2807	rBV	294	214	0.02%	0.002%
70	10.095	2814	2816	2820	rBV2	252	145	0.01%	0.002%
71	10.153	2822	2834	2857	rBV	368969	580534	51.84%	6.630%
72	10.294	2876	2878	2880	rBV	288	191	0.02%	0.002%
73	10.352	2893	2896	2897	rBV	217	129	0.01%	0.001%
74	10.381	2901	2905	2907	rVV	304	190	0.02%	0.002%
75	10.490	2936	2939	2941	rBV2	178	108	0.01%	0.001%
76	10.545	2954	2956	2962	rVB2	283	180	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031524\
 Data File : VV034678.D
 Acq On : 16 Mar 2024 01:28
 Operator : SY/MD
 Sample : P1740-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GK3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

77	10.680	2995	2998	3003	rBV2	297	220	0.02%	0.003%
78	10.780	3025	3029	3030	rBV	145	102	0.01%	0.001%
79	10.899	3064	3066	3069	rBV2	195	102	0.01%	0.001%
80	10.924	3072	3074	3076	rBV2	174	114	0.01%	0.001%
81	11.069	3116	3119	3122	rBV2	193	134	0.01%	0.002%
82	11.185	3145	3155	3183	rBV	496543	777317	69.41%	8.877%
83	11.391	3218	3219	3222	rVB	357	111	0.01%	0.001%
84	11.561	3258	3272	3292	rBV	455145	735055	65.64%	8.394%
85	11.940	3387	3390	3393	rBV	325	188	0.02%	0.002%
86	12.111	3441	3443	3446	rBV	315	166	0.01%	0.002%
87	12.275	3491	3494	3495	rBV	270	131	0.01%	0.001%
88	12.789	3646	3654	3657	rBV2	286	418	0.04%	0.005%
89	12.873	3678	3680	3684	rVB	343	228	0.02%	0.003%
90	12.908	3688	3691	3692	rBV	177	109	0.01%	0.001%
91	12.918	3692	3694	3699	rVB3	323	204	0.02%	0.002%
92	13.259	3797	3800	3806	rVB2	539	393	0.04%	0.004%
93	13.291	3806	3810	3813	rBV2	328	343	0.03%	0.004%
94	13.477	3866	3868	3872	rVB3	292	171	0.02%	0.002%
95	13.519	3878	3881	3885	rBV2	412	253	0.02%	0.003%
96	13.664	3923	3926	3927	rBV2	360	204	0.02%	0.002%
97	13.712	3937	3941	3943	rBV2	598	391	0.03%	0.004%
98	14.201	4090	4093	4094	rBV2	288	129	0.01%	0.001%
99	14.474	4176	4178	4179	rBV	437	172	0.02%	0.002%
100	15.101	4369	4373	4374	rBV2	722	452	0.04%	0.005%




Sum of corrected areas: 8756487

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031524\
Data File : VV034678.D
Acq On : 16 Mar 2024 01:28
Operator : SY/MD
Sample : P1740-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GK3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

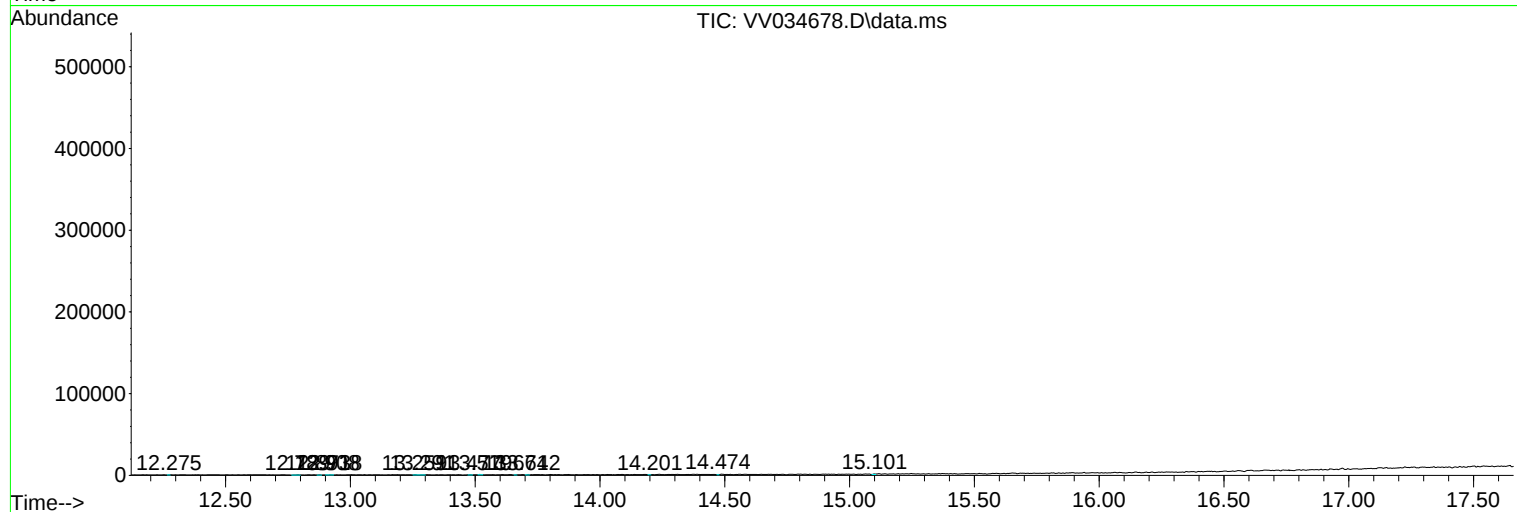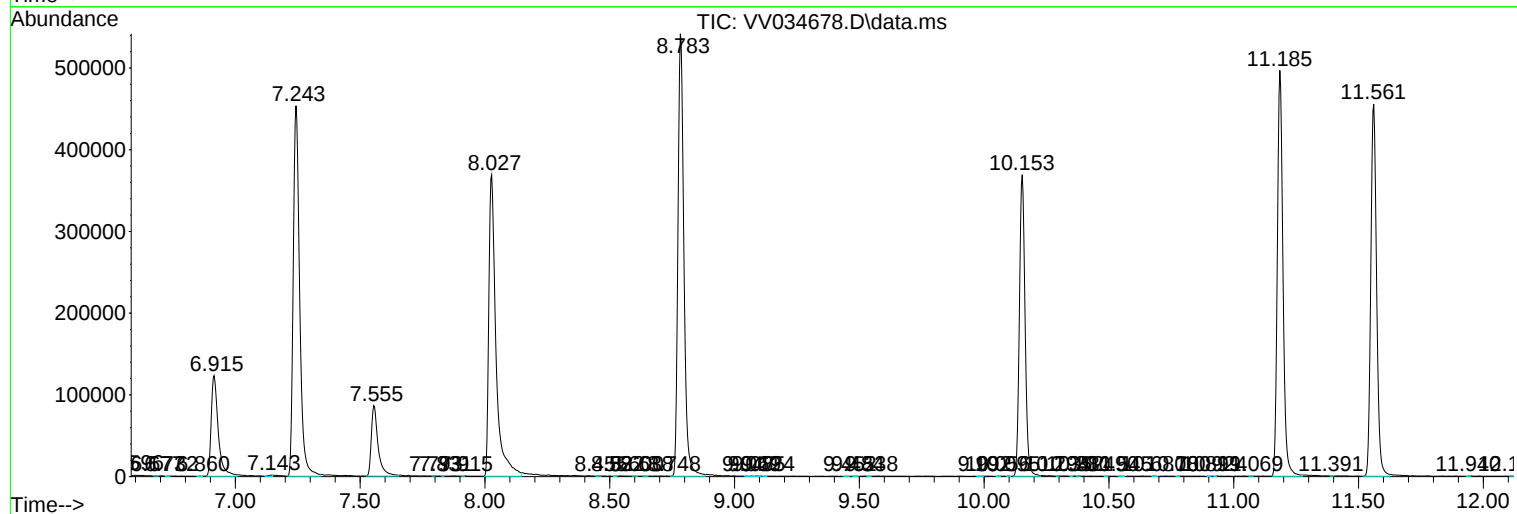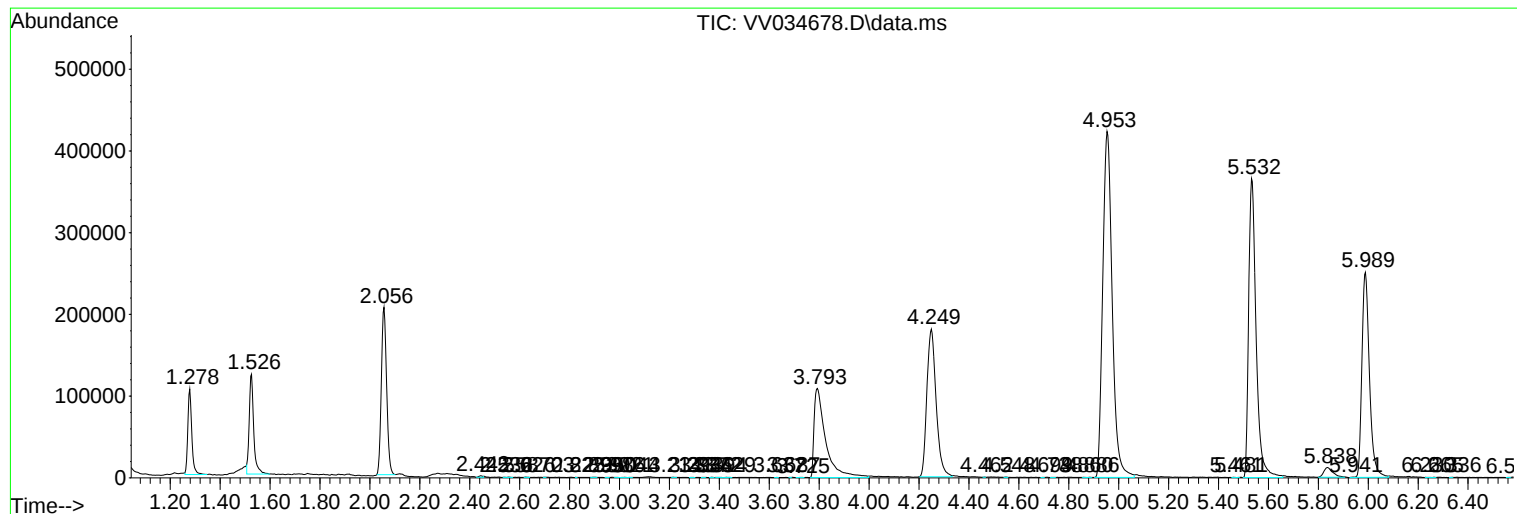

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031524\
Data File : VV034678.D
Acq On : 16 Mar 2024 01:28
Operator : SY/MD
Sample : P1740-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GK3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031524\
Data File : VV034678.D
Acq On : 16 Mar 2024 01:28
Operator : SY/MD
Sample : P1740-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GK3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc