

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031524\
 Data File : VV034680.D
 Acq On : 16 Mar 2024 02:16
 Operator : SY/MD
 Sample : P1740-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GK6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

Signal : TIC: VV034680.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	86	rVB	102416	110014	10.17%	1.311%
2	1.523	145	150	172	rVB	121146	149152	13.79%	1.778%
3	2.056	306	316	332	rBV	204758	297269	27.48%	3.543%
4	2.651	498	501	505	rVB2	291	167	0.02%	0.002%
5	2.741	524	529	535	rVB3	381	459	0.04%	0.005%
6	2.773	535	539	545	rBV2	282	286	0.03%	0.003%
7	2.847	560	562	564	rBV	220	123	0.01%	0.001%
8	2.876	568	571	576	rBV2	160	148	0.01%	0.002%
9	3.179	659	665	668	rBV2	284	262	0.02%	0.003%
10	3.236	675	683	691	rBV2	220	420	0.04%	0.005%
11	3.304	701	704	707	rBV	197	164	0.02%	0.002%
12	3.349	714	718	719	rBV2	230	131	0.01%	0.002%
13	3.407	733	736	740	rBV2	165	152	0.01%	0.002%
14	3.452	748	750	754	rVV2	227	115	0.01%	0.001%
15	3.490	757	762	765	rBV2	118	119	0.01%	0.001%
16	3.529	770	774	781	rBV2	154	235	0.02%	0.003%
17	3.561	781	784	788	rVB	205	140	0.01%	0.002%
18	3.590	790	793	796	rVB	196	114	0.01%	0.001%
19	3.683	819	822	826	rVV2	119	121	0.01%	0.001%
20	3.789	847	855	893	rBV	104386	299669	27.70%	3.571%
21	4.246	983	997	1021	rBV	170126	439369	40.61%	5.236%
22	4.516	1079	1081	1086	rVB4	329	190	0.02%	0.002%
23	4.567	1096	1097	1100	rVB	436	163	0.02%	0.002%
24	4.629	1113	1116	1118	rBV2	212	143	0.01%	0.002%
25	4.812	1170	1173	1176	rVB2	250	177	0.02%	0.002%
26	4.847	1181	1184	1187	rBV3	270	188	0.02%	0.002%
27	4.953	1202	1217	1261	rBV2	404896	1081829	100.00%	12.893%
28	5.358	1339	1343	1346	rBV2	315	268	0.02%	0.003%
29	5.387	1350	1352	1355	rVB2	352	162	0.01%	0.002%
30	5.436	1363	1367	1371	rBV	267	240	0.02%	0.003%
31	5.455	1371	1373	1377	rVB2	332	237	0.02%	0.003%
32	5.474	1377	1379	1381	rVB2	423	189	0.02%	0.002%
33	5.494	1381	1385	1386	rBV	225	114	0.01%	0.001%
34	5.532	1387	1397	1433	rBV	338727	708306	65.47%	8.442%
35	5.831	1482	1490	1491	rBV	8385	8000	0.74%	0.095%
36	5.989	1527	1539	1566	rBV	243338	509105	47.06%	6.067%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031524\
 Data File : VV034680.D
 Acq On : 16 Mar 2024 02:16
 Operator : SY/MD
 Sample : P1740-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GK6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	6.259	1621	1623	1629	rVB2	418	293	0.03%	0.003%
38	6.352	1646	1652	1655	rVB2	221	212	0.02%	0.003%
39	6.381	1655	1661	1664	rBV2	154	149	0.01%	0.002%
40	6.436	1672	1678	1682	rBV2	171	183	0.02%	0.002%
41	6.487	1691	1694	1698	rVB	369	286	0.03%	0.003%
42	6.510	1698	1701	1708	rBV2	206	200	0.02%	0.002%
43	6.545	1708	1712	1715	rBV2	318	249	0.02%	0.003%
44	6.583	1720	1724	1726	rBV	559	453	0.04%	0.005%
45	6.664	1744	1749	1754	rVB4	603	687	0.06%	0.008%
46	6.690	1754	1757	1761	rBV2	490	388	0.04%	0.005%
47	6.738	1770	1772	1776	rBV2	457	249	0.02%	0.003%
48	6.915	1816	1827	1859	rBV2	119073	232276	21.47%	2.768%
49	7.243	1918	1929	1957	rBV	438876	779865	72.09%	9.294%
50	7.555	2017	2026	2057	rBV	83781	158333	14.64%	1.887%
51	7.773	2092	2094	2097	rBV2	296	181	0.02%	0.002%
52	7.837	2112	2114	2117	rBV	227	111	0.01%	0.001%
53	7.873	2120	2125	2127	rBV2	424	427	0.04%	0.005%
54	7.940	2142	2146	2148	rVB	275	185	0.02%	0.002%
55	8.027	2163	2173	2213	rBV	358331	710479	65.67%	8.467%
56	8.397	2285	2288	2294	rBV4	419	406	0.04%	0.005%
57	8.461	2306	2308	2312	rVB2	519	357	0.03%	0.004%
58	8.619	2354	2357	2359	rBV3	285	222	0.02%	0.003%
59	8.670	2370	2373	2376	rVB3	338	198	0.02%	0.002%
60	8.696	2379	2381	2382	rBV	251	112	0.01%	0.001%
61	8.725	2387	2390	2394	rBV3	288	226	0.02%	0.003%
62	8.786	2398	2409	2442	rBV	516550	859415	79.44%	10.242%
63	9.104	2505	2508	2510	rBV2	261	167	0.02%	0.002%
64	9.127	2513	2515	2520	rVV3	543	406	0.04%	0.005%
65	9.165	2524	2527	2532	rVB	203	133	0.01%	0.002%
66	9.198	2535	2537	2540	rVV	266	147	0.01%	0.002%
67	9.246	2550	2552	2557	rVB3	244	175	0.02%	0.002%
68	9.281	2557	2563	2566	rBV2	405	366	0.03%	0.004%
69	9.326	2575	2577	2583	rVB2	286	172	0.02%	0.002%
70	9.358	2583	2587	2589	rBV2	234	205	0.02%	0.002%
71	9.464	2615	2620	2622	rVB2	324	242	0.02%	0.003%
72	9.477	2622	2624	2626	rBV	249	152	0.01%	0.002%
73	9.728	2697	2702	2708	rBV2	187	245	0.02%	0.003%
74	9.976	2778	2779	2783	rVV	254	145	0.01%	0.002%
75	9.998	2783	2786	2792	rVB2	190	198	0.02%	0.002%
76	10.152	2823	2834	2856	rBV	366549	572541	52.92%	6.823%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031524\
 Data File : VV034680.D
 Acq On : 16 Mar 2024 02:16
 Operator : SY/MD
 Sample : P1740-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GK6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

77	10.361	2896	2899	2902	rVB	451	225	0.02%	0.003%
78	10.583	2965	2968	2974	rBV	221	201	0.02%	0.002%
79	10.709	3004	3007	3010	rBV2	305	139	0.01%	0.002%
80	10.751	3010	3020	3022	rBV2	203	315	0.03%	0.004%
81	10.863	3050	3055	3060	rBV2	318	386	0.04%	0.005%
82	11.185	3144	3155	3182	rBV	468459	734405	67.89%	8.753%
83	11.435	3230	3233	3236	rBV2	471	353	0.03%	0.004%
84	11.480	3244	3247	3249	rBV	367	210	0.02%	0.003%
85	11.561	3260	3272	3292	rBV	456125	722023	66.74%	8.605%
86	11.902	3369	3378	3381	rBV2	294	461	0.04%	0.005%
87	11.931	3384	3387	3389	rBV2	177	135	0.01%	0.002%
88	12.095	3435	3438	3441	rBV	191	146	0.01%	0.002%
89	12.178	3462	3464	3465	rBV	245	114	0.01%	0.001%
90	12.332	3509	3512	3515	rBV	189	134	0.01%	0.002%
91	12.410	3533	3536	3539	rBV	274	141	0.01%	0.002%
92	12.538	3573	3576	3577	rBV	234	113	0.01%	0.001%
93	12.583	3587	3590	3592	rBV	182	137	0.01%	0.002%
94	12.625	3600	3603	3607	rVB3	446	339	0.03%	0.004%
95	12.715	3627	3631	3633	rBV	239	209	0.02%	0.002%
96	13.281	3805	3807	3810	rBV2	329	164	0.02%	0.002%
97	13.609	3907	3909	3911	rVB3	586	175	0.02%	0.002%
98	13.882	3990	3994	3996	rBV2	487	395	0.04%	0.005%
99	13.969	4018	4021	4023	rBV3	389	249	0.02%	0.003%
100	14.152	4076	4078	4081	rVB2	431	193	0.02%	0.002%




Sum of corrected areas: 8390738

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031524\
Data File : VV034680.D
Acq On : 16 Mar 2024 02:16
Operator : SY/MD
Sample : P1740-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GK6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

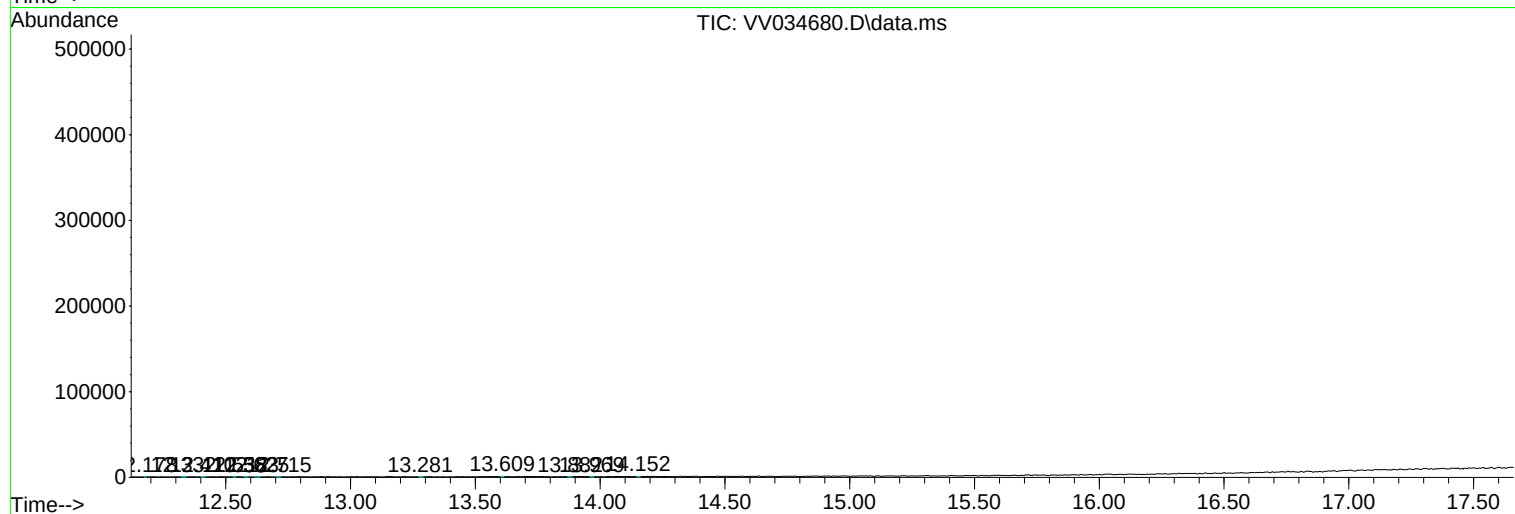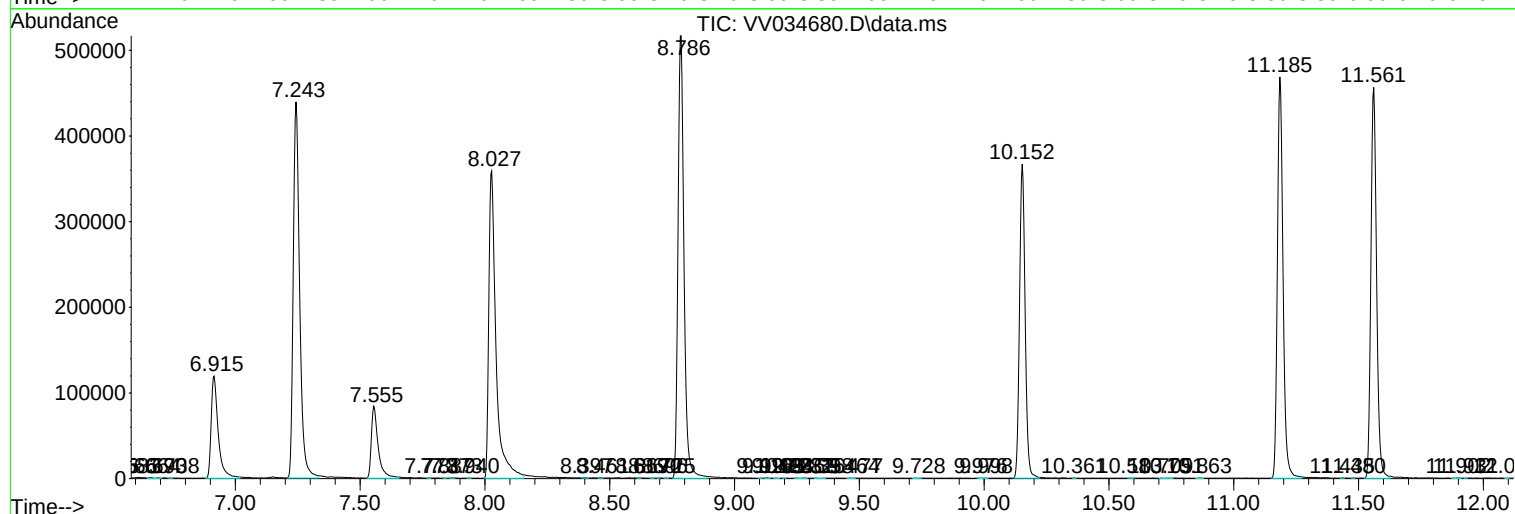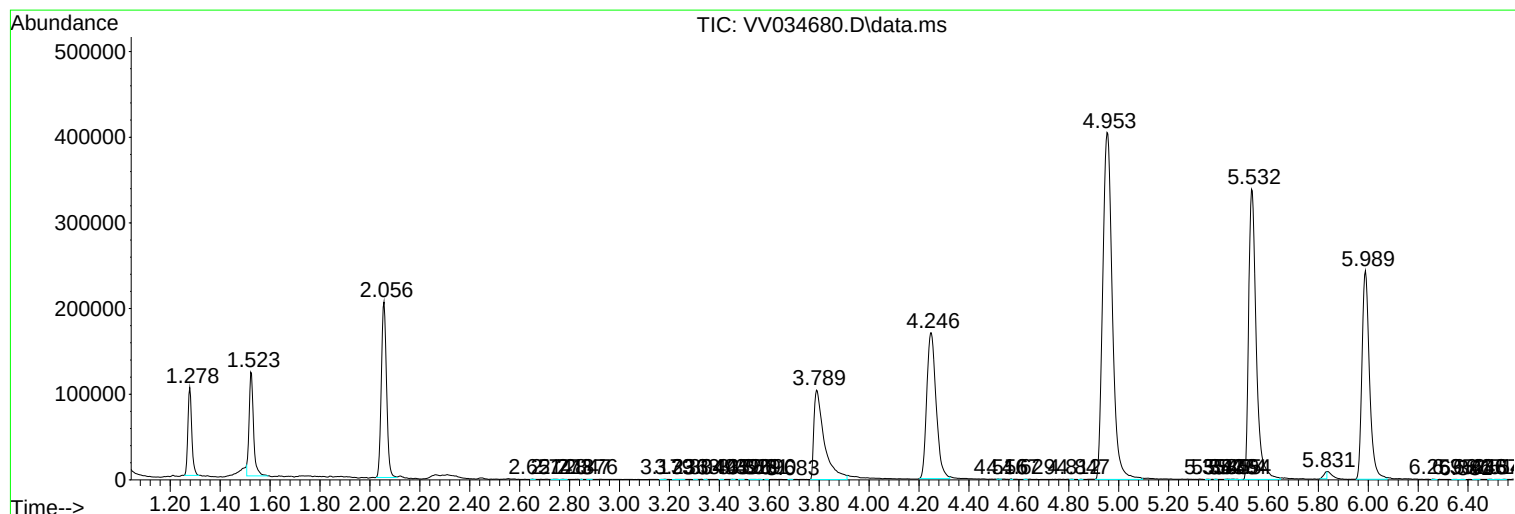

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031524\
Data File : VV034680.D
Acq On : 16 Mar 2024 02:16
Operator : SY/MD
Sample : P1740-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GK6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031524\
Data File : VV034680.D
Acq On : 16 Mar 2024 02:16
Operator : SY/MD
Sample : P1740-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GK6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc