
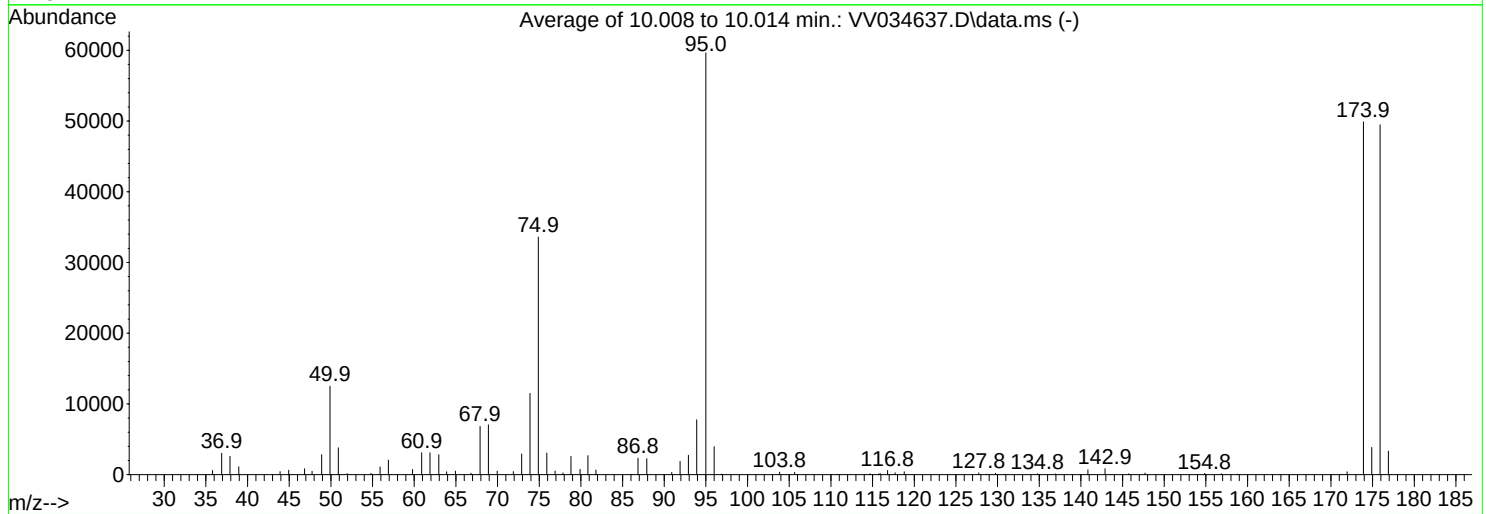


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031524\
Data File : VV034637.D
Acq On : 15 Mar 2024 08:25
Operator : SY/MD
Sample : BFB269
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB269

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Title : VOC Analysis
Last Update : Tue Mar 19 02:53:17 2024

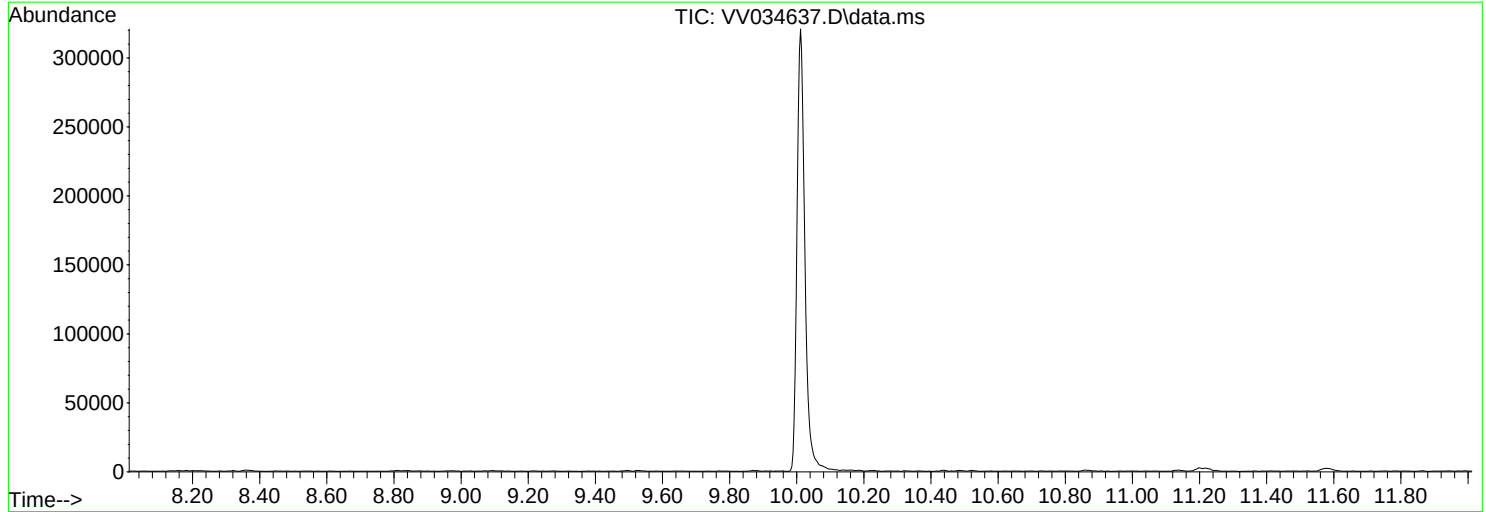

AutoFind: Scans 2789, 2790, 2791; Background Corrected with Scan 2779

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.0	12505	PASS
75	95	30	80	56.3	33600	PASS
95	95	100	100	100.0	59640	PASS
96	95	5	9	6.6	3966	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	83.6	49880	PASS
175	174	5	9	7.7	3839	PASS
176	174	95	105	99.2	49469	PASS
177	176	5	10	6.7	3316	PASS

m/z	Abundance
39.80	262.0
43.90	236.0

Instrument :
MSVOA_V
ClientSampleId :
BFB269

m/z	Abundance
35.80	597.0
36.90	3004.0
37.90	2726.0
38.90	1012.0
39.80	193.0
43.90	672.0
44.90	651.0
46.90	820.0
47.70	459.0
48.90	2602.0
49.90	12488.0
50.90	3822.0
51.90	191.0
54.80	202.0
55.90	1064.0
56.90	2014.0
59.80	764.0
60.90	3143.0
61.90	3119.0
62.90	2839.0
63.90	389.0
65.00	439.0
66.80	212.0
67.90	6784.0
68.90	7002.0
70.00	479.0
71.90	400.0
72.90	2941.0
73.90	11647.0
74.90	33256.0
75.90	2922.0
77.00	500.0
77.80	263.0
78.80	2606.0
79.90	722.0
80.80	2590.0
81.80	599.0
86.80	2437.0
87.90	2327.0
90.90	268.0
91.90	1850.0
92.90	2647.0
93.90	7787.0
95.00	58472.0
96.00	4042.0
103.80	337.0
105.60	303.0
110.80	109.0
114.70	113.0
115.70	246.0
116.80	651.0
117.70	245.0
118.70	418.0
127.70	222.0
128.70	123.0
129.90	227.0
134.80	136.0
137.00	128.0
140.80	642.0
142.90	797.0
145.00	113.0
145.70	145.0
147.70	205.0
154.80	161.0
156.80	148.0
171.20	108.0
171.90	451.0
173.90	48424.0
174.90	3573.0
175.90	47552.0
176.90	3207.0

Instrument :
MSVOA_V
ClientSampleId :
BFB269

m/z	Abundance
35.90	629.0
36.90	3131.0
37.90	2712.0
39.00	1127.0
39.90	208.0
43.90	694.0
44.90	647.0
46.90	865.0
47.70	499.0
48.90	2913.0
49.90	12934.0
50.90	3905.0
51.90	158.0
54.80	192.0
55.90	1136.0
56.90	2139.0
59.80	782.0
60.90	3219.0
61.90	3194.0
63.00	2957.0
63.90	433.0
64.90	534.0
66.80	213.0
67.90	7019.0
68.90	7198.0
69.90	506.0
71.90	463.0
72.90	2964.0
73.90	11900.0
74.90	34720.0
75.90	3250.0
76.90	515.0
77.90	258.0
78.80	2714.0
79.90	774.0
80.90	2773.0
81.80	698.0
86.80	2386.0
87.90	2341.0
90.90	326.0
91.90	1917.0
92.90	2798.0
93.90	7951.0
95.00	61624.0
96.00	4100.0
96.90	123.0
103.80	359.0
105.70	347.0
114.70	160.0
115.90	261.0
116.80	624.0
117.70	278.0
118.80	395.0
127.80	258.0
128.70	104.0
129.70	210.0
134.80	143.0
137.00	113.0
140.90	713.0
142.90	915.0
145.70	139.0
147.70	229.0
154.90	177.0
156.80	136.0
158.80	113.0
171.90	412.0
173.90	51568.0
174.90	3975.0
175.90	51344.0
176.90	3449.0

Instrument :
MSVOA_V
ClientSampleId :
BFB269

m/z	Abundance
35.00	559.0
36.00	2967.0
37.00	2379.0
39.00	1166.0
40.00	243.0
43.00	660.0
45.00	576.0
46.00	806.0
47.00	449.0
48.00	3000.0
49.00	12093.0
50.00	3701.0
52.00	128.0
54.00	147.0
55.00	1076.0
56.00	2030.0
59.00	640.0
60.00	2942.0
61.00	2957.0
63.00	2702.0
63.00	424.0
64.00	544.0
66.00	205.0
67.00	6730.0
68.00	6892.0
69.00	483.0
71.00	440.0
72.00	2876.0
73.00	10938.0
74.00	32824.0
75.00	3014.0
76.00	555.0
77.00	254.0
78.00	2442.0
79.00	748.0
80.00	2693.0
81.00	699.0
86.10	113.0
86.00	2170.0
87.00	2138.0
90.00	338.0
91.00	1864.0
92.00	2764.0
93.00	7562.0
95.00	58824.0
96.00	3756.0
96.00	142.0
103.00	331.0
105.70	336.0
114.70	164.0
115.00	287.0
116.80	502.0
117.70	278.0
118.00	389.0
127.80	260.0
129.70	185.0
130.80	108.0
134.80	128.0
136.90	102.0
140.90	695.0
142.90	801.0
145.80	116.0
147.70	214.0
154.90	181.0
156.90	121.0
158.80	105.0
172.00	380.0
173.90	49648.0
174.90	3969.0
175.90	49512.0
176.90	3291.0

Instrument :
MSVOA_V
ClientSampleId :
BFB269