

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031619\
 Data File : VV009686.D
 Acq On : 15 Mar 2019 15:06
 Operator : SY/MD
 Sample : VV0316MBL01
 Misc : 5.00µL/5.0mL/100µL/15.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK72

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031219WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.116	4	8	14	rBV2	2404	2200	0.39%	0.052%
2	1.319	64	71	83	rVB	74922	72917	12.82%	1.708%
3	1.570	143	149	165	rVB	69723	86373	15.19%	2.023%
4	2.126	313	322	336	rVB	180401	259631	45.66%	6.080%
5	2.682	489	495	499	rBV	580	729	0.13%	0.017%
6	3.049	605	609	612	rBV2	621	564	0.10%	0.013%
7	3.573	768	772	778	rBV2	727	670	0.12%	0.016%
8	3.602	778	781	783	rBV2	636	395	0.07%	0.009%
9	3.814	844	847	849	rBV	401	251	0.04%	0.006%
10	3.856	853	860	862	rBV2	574	635	0.11%	0.015%
11	3.926	871	882	904	rBV	43436	106669	18.76%	2.498%
12	4.261	983	986	990	rBV	625	405	0.07%	0.009%
13	4.399	1013	1029	1055	rBV	91097	228669	40.22%	5.355%
14	4.579	1082	1085	1087	rBV	336	210	0.04%	0.005%
15	4.618	1092	1097	1100	rBV	673	661	0.12%	0.015%
16	4.647	1100	1106	1109	rBV	643	705	0.12%	0.017%
17	4.698	1120	1122	1125	rBV2	552	361	0.06%	0.008%
18	4.785	1147	1149	1152	rVB	655	292	0.05%	0.007%
19	4.868	1171	1175	1179	rBV	774	746	0.13%	0.017%
20	5.093	1226	1245	1268	rBV3	220611	568570	100.00%	13.315%
21	5.515	1371	1376	1381	rBV2	761	964	0.17%	0.023%
22	5.605	1401	1404	1407	rBV	620	420	0.07%	0.010%
23	5.663	1409	1422	1437	rBV	161815	323637	56.92%	7.579%
24	6.116	1548	1563	1580	rBV	124534	253822	44.64%	5.944%
25	6.277	1611	1613	1615	rBV	460	219	0.04%	0.005%
26	6.380	1642	1645	1647	rBV	606	385	0.07%	0.009%
27	6.608	1712	1716	1717	rBV	644	413	0.07%	0.010%
28	6.653	1727	1730	1735	rBV2	618	601	0.11%	0.014%
29	6.756	1760	1762	1765	rBV2	349	237	0.04%	0.006%
30	6.974	1827	1830	1834	rVB2	557	386	0.07%	0.009%
31	7.029	1834	1847	1864	rBV2	69311	127455	22.42%	2.985%
32	7.180	1892	1894	1897	rBV2	365	258	0.05%	0.006%
33	7.357	1937	1949	1968	rBV	256836	461492	81.17%	10.807%
34	7.663	2034	2044	2063	rBV	48097	81239	14.29%	1.902%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031619\
 Data File : VV009686.D
 Acq On : 15 Mar 2019 15:06
 Operator : SY/MD
 Sample : VV0316MBL01
 Misc : 5.00g/5.0mL/100uL/15.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK72

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031219WMA.M
 Title : VOC Analysis

35	8.087	2173	2176	2177	rBV	499	284	0.05%	0.007%
36	8.132	2179	2190	2226	rVV	132468	263400	46.33%	6.168%
37	8.563	2321	2324	2326	rBV	359	223	0.04%	0.005%
38	8.894	2415	2427	2451	rBV	240548	416270	73.21%	9.748%
39	9.508	2615	2618	2621	rBV	558	337	0.06%	0.008%
40	9.576	2636	2639	2643	rBV2	589	593	0.10%	0.014%
41	9.646	2658	2661	2664	rBV	415	320	0.06%	0.007%
42	9.769	2696	2699	2702	rBV	568	375	0.07%	0.009%
43	10.080	2792	2796	2799	rBV	467	438	0.08%	0.010%
44	10.261	2841	2852	2874	rBV	176992	285813	50.27%	6.693%
45	10.556	2942	2944	2947	rVB2	579	326	0.06%	0.008%
46	10.576	2947	2950	2952	rBV	503	317	0.06%	0.007%
47	10.907	3050	3053	3057	rBV2	589	444	0.08%	0.010%
48	11.299	3163	3175	3192	rBV	193602	333915	58.73%	7.820%
49	11.408	3206	3209	3212	rBV	794	571	0.10%	0.013%
50	11.672	3280	3291	3312	rVB	224888	379180	66.69%	8.880%
51	12.489	3542	3545	3549	rBV	756	561	0.10%	0.013%
52	12.756	3624	3628	3632	rBV	767	645	0.11%	0.015%
53	12.797	3638	3641	3642	rBV	411	236	0.04%	0.006%
54	14.116	4044	4051	4053	rBV3	925	936	0.16%	0.022%
55	14.196	4069	4076	4079	rBV2	906	1079	0.19%	0.025%
56	14.444	4151	4153	4156	rBV	786	418	0.07%	0.010%
57	14.530	4177	4180	4181	rBV	614	354	0.06%	0.008%


Sum of corrected areas: 4270216

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV031619\
Data File : VV009686.D
Acq On : 15 Mar 2019 15:06
Operator : SY/MD
Sample : VV0316MBL01
Misc : 5.00µ/5.0mL/100uL/15.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK72

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

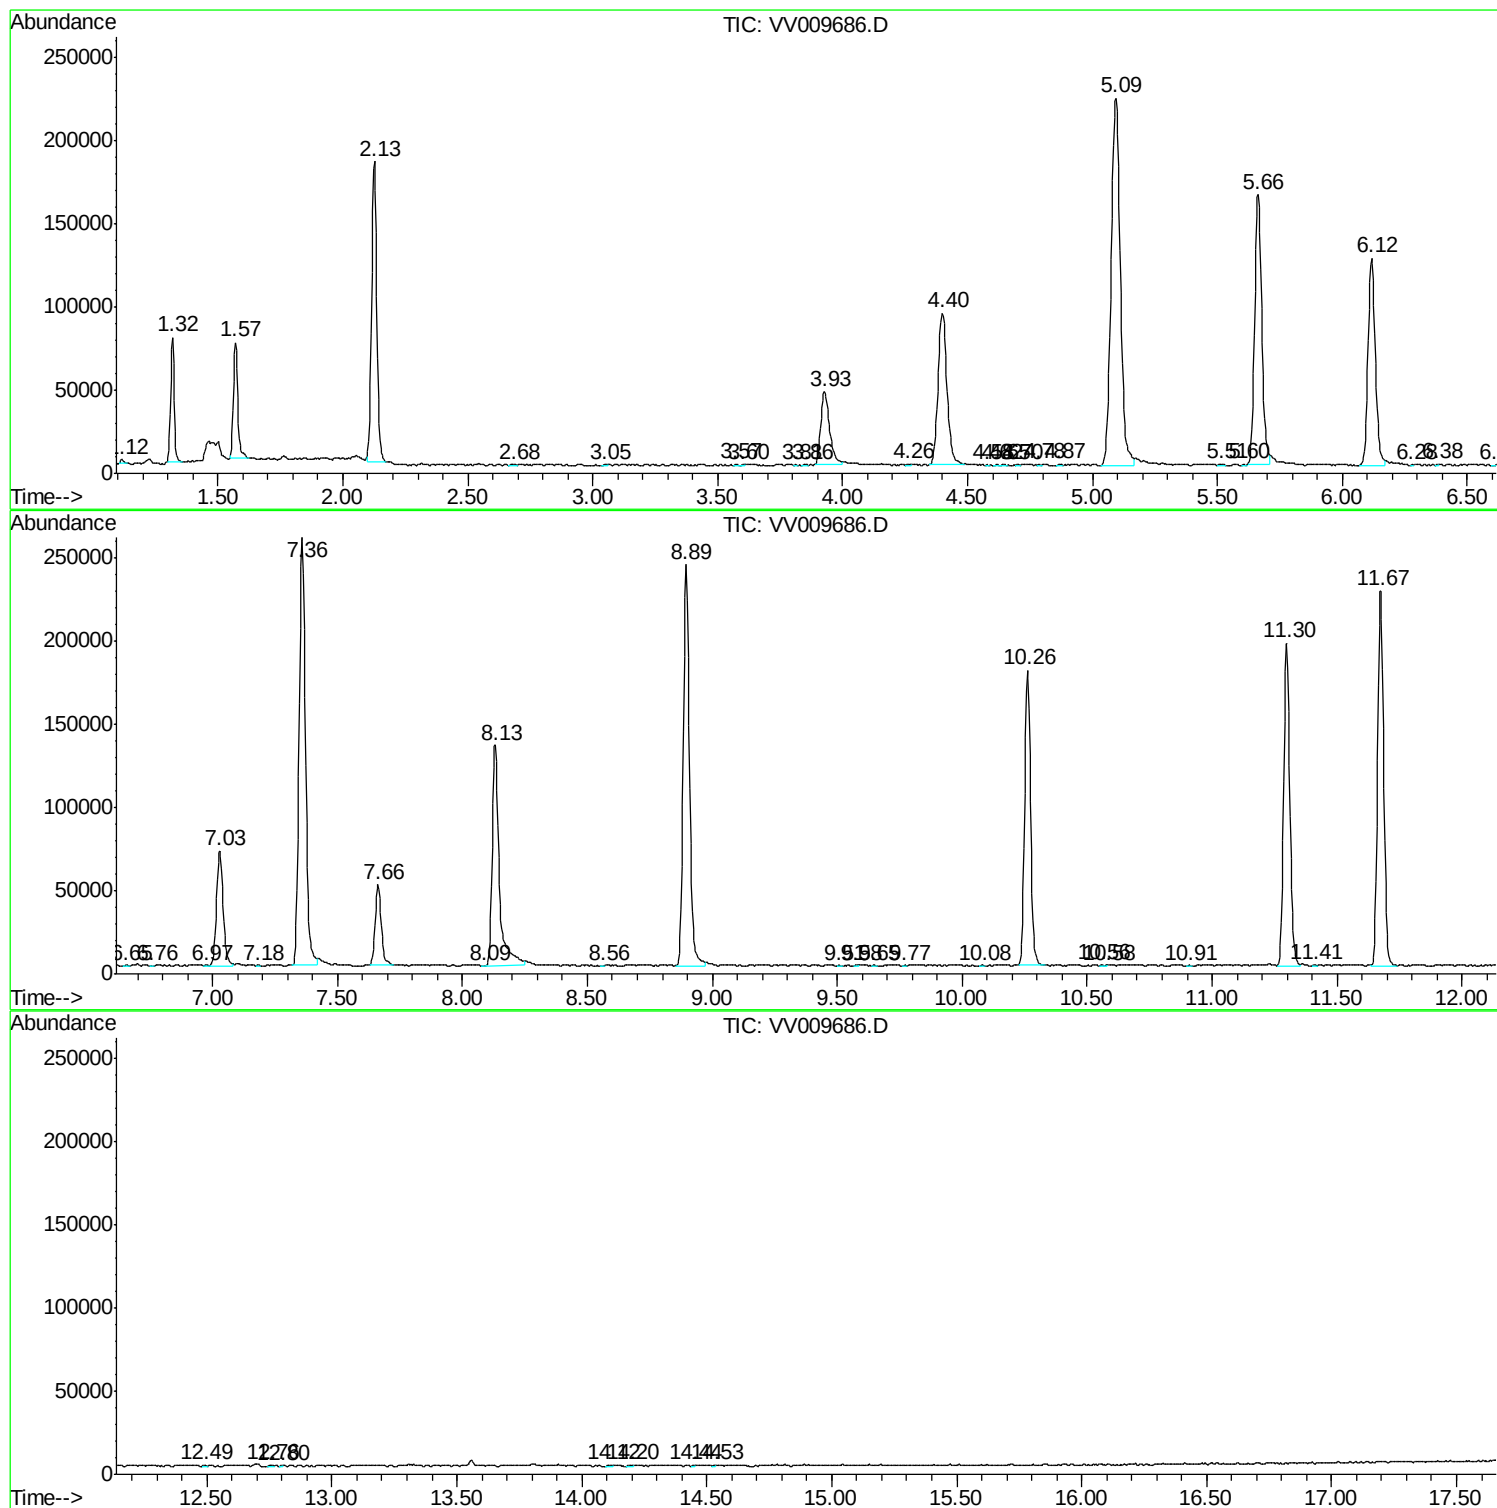

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV031619\
Data File : VV009686.D
Acq On : 15 Mar 2019 15:06
Operator : SY/MD
Sample : VV0316MBL01
Misc : 5.00g/5.0mL/100uL/15.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK72

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV031619\
Data File : VV009686.D
Acq On : 15 Mar 2019 15:06
Operator : SY/MD
Sample : VV0316MBL01
Misc : 5.00g/5.0mL/100uL/15.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK72

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc