

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031619\
 Data File : VV009690.D
 Acq On : 15 Mar 2019 17:03
 Operator : SY/MD
 Sample : K1939-07
 Misc : 5.85g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BF0T0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031219WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.109	3	6	12	rVB	2618	1974	0.36%	0.041%
2	1.315	61	70	91	rVB	52231	65608	11.98%	1.377%
3	1.450	106	112	118	rBV	9335	17171	3.14%	0.360%
4	2.097	304	313	326	rVB	158483	225062	41.09%	4.723%
5	2.408	408	410	415	rBV	652	535	0.10%	0.011%
6	2.524	440	446	451	rBV3	1282	1744	0.32%	0.037%
7	2.672	488	492	497	rBV	618	723	0.13%	0.015%
8	3.611	781	784	786	rBV	433	269	0.05%	0.006%
9	3.855	853	860	863	rBV2	719	898	0.16%	0.019%
10	3.952	876	890	919	rBV4	82657	230461	42.08%	4.836%
11	4.225	971	975	979	rBV2	742	720	0.13%	0.015%
12	4.302	997	999	1000	rBV	480	203	0.04%	0.004%
13	4.399	1013	1029	1053	rBV	89858	221399	40.42%	4.646%
14	4.640	1101	1104	1109	rBV2	706	550	0.10%	0.012%
15	4.797	1151	1153	1155	rBV2	354	197	0.04%	0.004%
16	4.868	1171	1175	1178	rBV	516	401	0.07%	0.008%
17	4.904	1184	1186	1192	rVB	630	444	0.08%	0.009%
18	5.090	1226	1244	1266	rBV3	224475	547711	100.00%	11.494%
19	5.476	1358	1364	1367	rBV	565	796	0.15%	0.017%
20	5.543	1381	1385	1386	rBV	402	212	0.04%	0.004%
21	5.662	1408	1422	1444	rBV	165639	347956	63.53%	7.302%
22	5.958	1501	1514	1529	rBV	88628	175163	31.98%	3.676%
23	6.116	1551	1563	1587	rVB	118942	244263	44.60%	5.126%
24	6.450	1665	1667	1669	rBV	236	125	0.02%	0.003%
25	6.672	1733	1736	1739	rBV	304	176	0.03%	0.004%
26	6.717	1739	1750	1761	rVV4	2912	6603	1.21%	0.139%
27	6.772	1764	1767	1771	rBV2	633	398	0.07%	0.008%
28	6.794	1771	1774	1776	rBV	397	256	0.05%	0.005%
29	6.952	1817	1823	1826	rBV	677	671	0.12%	0.014%
30	7.032	1836	1848	1868	rBV	65087	122935	22.45%	2.580%
31	7.180	1891	1894	1896	rBV	417	219	0.04%	0.005%
32	7.193	1896	1898	1904	rBV2	496	517	0.09%	0.011%
33	7.260	1914	1919	1921	rBV	659	575	0.10%	0.012%
34	7.276	1921	1924	1926	rBV	494	332	0.06%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031619\
 Data File : VV009690.D
 Acq On : 15 Mar 2019 17:03
 Operator : SY/MD
 Sample : K1939-07
 Misc : 5.85g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BF0T0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031219WMA.M
 Title : VOC Analysis

35	7.360	1936	1950	1967	rBV	254834	453848	82.86%	9.524%
36	7.569	2009	2015	2018	rBV2	601	747	0.14%	0.016%
37	7.665	2035	2045	2064	rBV	45314	83177	15.19%	1.746%
38	7.823	2086	2094	2096	rBV	984	1395	0.25%	0.029%
39	7.878	2108	2111	2114	rBV2	515	464	0.08%	0.010%
40	7.948	2131	2133	2135	rBV	204	86	0.02%	0.002%
41	7.965	2135	2138	2140	rBV2	266	166	0.03%	0.003%
42	8.019	2144	2155	2170	rVB	45566	79663	14.54%	1.672%
43	8.145	2181	2194	2222	rBV	145734	281076	51.32%	5.899%
44	8.453	2287	2290	2291	rBV	534	265	0.05%	0.006%
45	8.482	2296	2299	2302	rBV2	358	271	0.05%	0.006%
46	8.582	2326	2330	2334	rBV	628	590	0.11%	0.012%
47	8.672	2352	2358	2363	rBV	612	765	0.14%	0.016%
48	8.701	2363	2367	2373	rBV	766	860	0.16%	0.018%
49	8.781	2389	2392	2395	rBV	602	422	0.08%	0.009%
50	8.823	2402	2405	2408	rBV	502	373	0.07%	0.008%
51	8.900	2416	2429	2445	rBV	265753	458456	83.70%	9.621%
52	9.347	2564	2568	2570	rBV	651	516	0.09%	0.011%
53	9.473	2605	2607	2609	rBV2	562	271	0.05%	0.006%
54	9.646	2659	2661	2663	rBV	417	223	0.04%	0.005%
55	10.267	2842	2854	2871	rBV	201210	315885	57.67%	6.629%
56	10.386	2888	2891	2895	rBV	422	271	0.05%	0.006%
57	10.553	2941	2943	2948	rVB2	455	277	0.05%	0.006%
58	10.672	2977	2980	2984	rBV	410	421	0.08%	0.009%
59	10.788	3013	3016	3018	rBV2	391	209	0.04%	0.004%
60	10.919	3054	3057	3058	rBV	611	356	0.06%	0.007%
61	11.138	3122	3125	3126	rBV	359	218	0.04%	0.005%
62	11.299	3164	3175	3193	rVB	264641	421500	76.96%	8.845%
63	11.675	3281	3292	3308	rBV	272582	438137	79.99%	9.195%
64	11.836	3339	3342	3345	rBV2	406	304	0.06%	0.006%
65	12.341	3497	3499	3503	rBV	456	399	0.07%	0.008%
66	12.472	3536	3540	3541	rBV2	418	275	0.05%	0.006%
67	13.061	3720	3723	3727	rBV	556	453	0.08%	0.010%
68	13.553	3873	3876	3878	rBV	357	193	0.04%	0.004%
69	13.569	3878	3881	3885	rVV	526	351	0.06%	0.007%
70	13.826	3957	3961	3967	rBV2	852	1096	0.20%	0.023%
71	13.913	3985	3988	3992	rBV2	539	416	0.08%	0.009%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031619\
Data File : VV009690.D
Acq On : 15 Mar 2019 17:03
Operator : SY/MD
Sample : K1939-07
Misc : 5.85g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BF0T0

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031219WMA.M
Title : VOC Analysis

72	14.331	4115	4118	4121	rBV	632	518	0.09%	0.011%
73	14.382	4129	4134	4138	rVB2	652	697	0.13%	0.015%
74	14.405	4138	4141	4144	rBV2	411	335	0.06%	0.007%
75	14.421	4144	4146	4149	rBV	475	319	0.06%	0.007%
76	14.485	4163	4166	4168	rVB	657	370	0.07%	0.008%
77	14.514	4172	4175	4178	rBV	553	521	0.10%	0.011%
78	14.678	4223	4226	4232	rBV3	718	756	0.14%	0.016%


Sum of corrected areas: 4765178

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV031619\
Data File : VV009690.D
Acq On : 15 Mar 2019 17:03
Operator : SY/MD
Sample : K1939-07
Misc : 5.85µ/5.0mL/100µL/5.0mL/MSVOA_V/MEOH
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BF0T0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

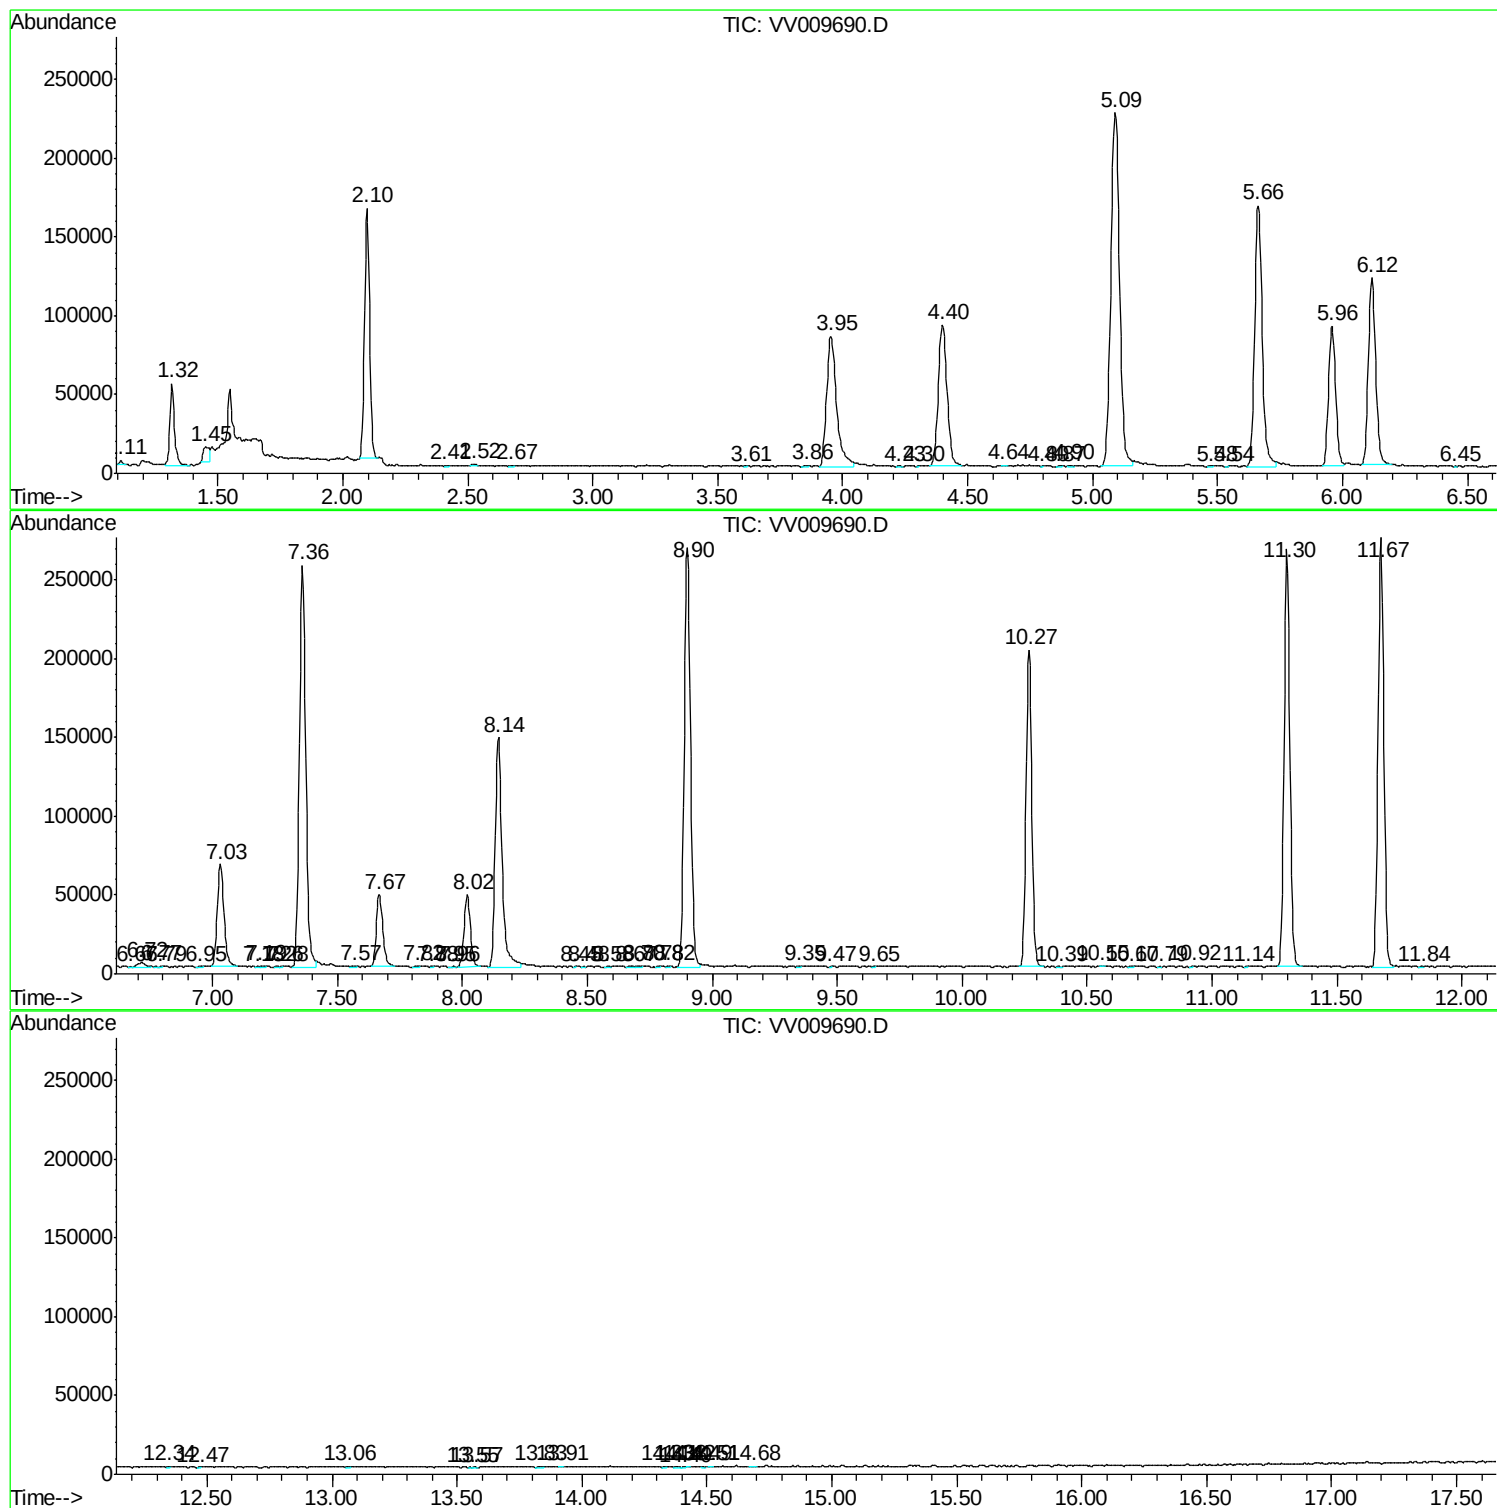

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV031619\
Data File : VV009690.D
Acq On : 15 Mar 2019 17:03
Operator : SY/MD
Sample : K1939-07
Misc : 5.85g/5.0mL/100uL/5.0mL/MSV0A_V/MEOH
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
BF0T0

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM031219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV031619\
Data File : VV009690.D
Acq On : 15 Mar 2019 17:03
Operator : SY/MD
Sample : K1939-07
Misc : 5.85g/5.0mL/100uL/5.0mL/MSV0A_V/MEOH
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
BF0T0

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM031219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc