

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031619\
 Data File : VV009703.D
 Acq On : 15 Mar 2019 22:22
 Operator : SY/MD
 Sample : K1939-20ME
 Misc : 5.30µ/5.0mL/100µL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BF0Y3ME

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031219WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.113	3	7	18	rVB2	3727	4098	0.74%	0.087%
2	1.203	31	35	39	rBV2	2561	3116	0.56%	0.066%
3	1.315	64	70	85	rVB	49819	61123	11.02%	1.292%
4	1.454	106	113	119	rBV3	10141	20012	3.61%	0.423%
5	2.100	305	314	327	rBV	158001	223874	40.36%	4.733%
6	2.460	423	426	430	rBV	900	864	0.16%	0.018%
7	2.524	441	446	451	rBV3	1192	1589	0.29%	0.034%
8	2.563	456	458	463	rBV	476	361	0.07%	0.008%
9	2.862	548	551	552	rBV	495	320	0.06%	0.007%
10	2.965	579	583	585	rBV	663	557	0.10%	0.012%
11	3.122	627	632	635	rBV2	813	734	0.13%	0.016%
12	3.444	728	732	733	rBV	506	350	0.06%	0.007%
13	3.563	765	769	772	rBV	607	510	0.09%	0.011%
14	3.582	772	775	779	rBV2	691	795	0.14%	0.017%
15	3.720	815	818	824	rVB	820	821	0.15%	0.017%
16	3.839	850	855	861	rVB	757	1006	0.18%	0.021%
17	3.872	861	865	868	rBV	857	825	0.15%	0.017%
18	3.949	877	889	933	rBV3	44066	141342	25.48%	2.988%
19	4.318	1001	1004	1008	rBV	702	770	0.14%	0.016%
20	4.399	1014	1029	1057	rBV2	91188	226881	40.90%	4.797%
21	4.621	1095	1098	1104	rVB	593	576	0.10%	0.012%
22	4.653	1104	1108	1112	rBV	451	489	0.09%	0.010%
23	5.090	1228	1244	1264	rBV2	231075	554731	100.00%	11.728%
24	5.322	1313	1316	1322	rBV2	807	1043	0.19%	0.022%
25	5.498	1367	1371	1377	rBV3	851	929	0.17%	0.020%
26	5.531	1377	1381	1387	rVB2	639	613	0.11%	0.013%
27	5.662	1409	1422	1444	rBV	191247	387242	69.81%	8.187%
28	5.904	1492	1497	1499	rBV	797	813	0.15%	0.017%
29	5.958	1504	1514	1529	rVB3	12844	25361	4.57%	0.536%
30	6.116	1550	1563	1589	rBV2	121105	255362	46.03%	5.399%
31	6.299	1617	1620	1623	rBV	762	659	0.12%	0.014%
32	6.560	1698	1701	1706	rBV	352	318	0.06%	0.007%
33	6.588	1706	1710	1715	rVB	560	536	0.10%	0.011%
34	6.691	1739	1742	1743	rBV2	1126	605	0.11%	0.013%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031619\
 Data File : VV009703.D
 Acq On : 15 Mar 2019 22:22
 Operator : SY/MD
 Sample : K1939-20ME
 Misc : 5.30µ/5.0mL/100µL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BF0Y3ME

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031219WMA.M
 Title : VOC Analysis

35	6.807	1775	1778	1780	rBV2	811	501	0.09%	0.011%
36	6.836	1784	1787	1789	rBV	496	334	0.06%	0.007%
37	6.933	1813	1817	1823	rVB	959	845	0.15%	0.018%
38	7.032	1836	1848	1864	rBV2	66533	122311	22.05%	2.586%
39	7.360	1936	1950	1975	rBV	257834	472387	85.16%	9.987%
40	7.511	1995	1997	2003	rBV3	676	678	0.12%	0.014%
41	7.669	2035	2046	2065	rBV	44114	82355	14.85%	1.741%
42	7.762	2072	2075	2079	rBV	511	356	0.06%	0.008%
43	7.823	2091	2094	2098	rBV	686	487	0.09%	0.010%
44	7.936	2124	2129	2131	rBV2	820	768	0.14%	0.016%
45	8.019	2147	2155	2164	rVB4	7913	13480	2.43%	0.285%
46	8.100	2176	2180	2182	rBV	896	678	0.12%	0.014%
47	8.141	2182	2193	2222	rVV	154121	297786	53.68%	6.296%
48	8.389	2266	2270	2273	rBV2	477	369	0.07%	0.008%
49	8.408	2273	2276	2278	rBV	506	364	0.07%	0.008%
50	8.440	2282	2286	2289	rBV	821	636	0.11%	0.013%
51	8.630	2341	2345	2349	rBV2	813	744	0.13%	0.016%
52	8.900	2416	2429	2447	rBV	306702	520673	93.86%	11.008%
53	9.318	2556	2559	2563	rVB	637	377	0.07%	0.008%
54	9.341	2563	2566	2569	rBV2	389	290	0.05%	0.006%
55	9.392	2579	2582	2584	rBV	694	494	0.09%	0.010%
56	9.569	2633	2637	2640	rBV	637	639	0.12%	0.014%
57	9.637	2655	2658	2660	rBV	443	375	0.07%	0.008%
58	9.836	2716	2720	2723	rBV	550	407	0.07%	0.009%
59	9.855	2723	2726	2731	rVB2	769	669	0.12%	0.014%
60	9.887	2731	2736	2739	rBV	853	824	0.15%	0.017%
61	10.038	2780	2783	2786	rBV	446	277	0.05%	0.006%
62	10.061	2786	2790	2793	rVB	709	482	0.09%	0.010%
63	10.151	2815	2818	2821	rBV	713	584	0.11%	0.012%
64	10.193	2828	2831	2833	rBV2	564	291	0.05%	0.006%
65	10.209	2833	2836	2839	rVV	537	368	0.07%	0.008%
66	10.267	2842	2854	2871	rVB	211464	335722	60.52%	7.098%
67	10.363	2880	2884	2887	rBV	663	579	0.10%	0.012%
68	10.408	2893	2898	2900	rBV2	586	446	0.08%	0.009%
69	10.559	2942	2945	2952	rVB2	658	762	0.14%	0.016%
70	10.595	2952	2956	2960	rVB	726	575	0.10%	0.012%
71	10.614	2960	2962	2965	rBV2	400	317	0.06%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031619\
 Data File : VV009703.D
 Acq On : 15 Mar 2019 22:22
 Operator : SY/MD
 Sample : K1939-20ME
 Misc : 5.30µ/5.0mL/100µL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BF0Y3ME

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031219WMA.M
 Title : VOC Analysis

72	10.633	2965	2968	2970	rBV	524	392	0.07%	0.008%
73	10.852	3033	3036	3040	rVB	513	360	0.06%	0.008%
74	10.874	3040	3043	3047	rBV	580	408	0.07%	0.009%
75	10.900	3047	3051	3055	rBV2	859	944	0.17%	0.020%
76	10.968	3069	3072	3074	rBV	490	336	0.06%	0.007%
77	11.154	3127	3130	3132	rBV	486	276	0.05%	0.006%
78	11.225	3149	3152	3155	rBV	497	387	0.07%	0.008%
79	11.299	3164	3175	3193	rVB	297492	479228	86.39%	10.131%
80	11.450	3218	3222	3225	rBV	603	481	0.09%	0.010%
81	11.501	3235	3238	3240	rBV	492	365	0.07%	0.008%
82	11.543	3248	3251	3254	rBV	497	343	0.06%	0.007%
83	11.675	3280	3292	3311	rBV	286098	454222	81.88%	9.603%
84	11.784	3323	3326	3330	rBV2	689	463	0.08%	0.010%
85	12.042	3403	3406	3409	rVV	932	553	0.10%	0.012%
86	12.106	3423	3426	3431	rVB2	1017	736	0.13%	0.016%
87	12.190	3449	3452	3456	rBB2	566	436	0.08%	0.009%
88	12.305	3483	3488	3492	rBV3	777	779	0.14%	0.016%
89	12.601	3576	3580	3583	rBV	645	645	0.12%	0.014%
90	12.768	3628	3632	3634	rBV	826	606	0.11%	0.013%
91	13.042	3714	3717	3722	rVB	746	597	0.11%	0.013%
92	13.067	3722	3725	3730	rBV	915	943	0.17%	0.020%
93	13.180	3757	3760	3768	rBV	699	747	0.13%	0.016%
94	13.292	3789	3795	3800	rBV2	905	1117	0.20%	0.024%
95	13.379	3816	3822	3825	rBV	852	858	0.15%	0.018%
96	13.633	3898	3901	3902	rBV	541	275	0.05%	0.006%
97	13.916	3983	3989	3992	rBV3	748	940	0.17%	0.020%
98	13.984	4006	4010	4021	rBV2	976	1583	0.29%	0.033%
99	14.183	4066	4072	4075	rBV2	544	574	0.10%	0.012%
100	15.119	4359	4363	4366	rBV	1222	1070	0.19%	0.023%


Sum of corrected areas: 4730119

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV031619\
Data File : VV009703.D
Acq On : 15 Mar 2019 22:22
Operator : SY/MD
Sample : K1939-20ME
Misc : 5.30uL/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BF0Y3ME

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

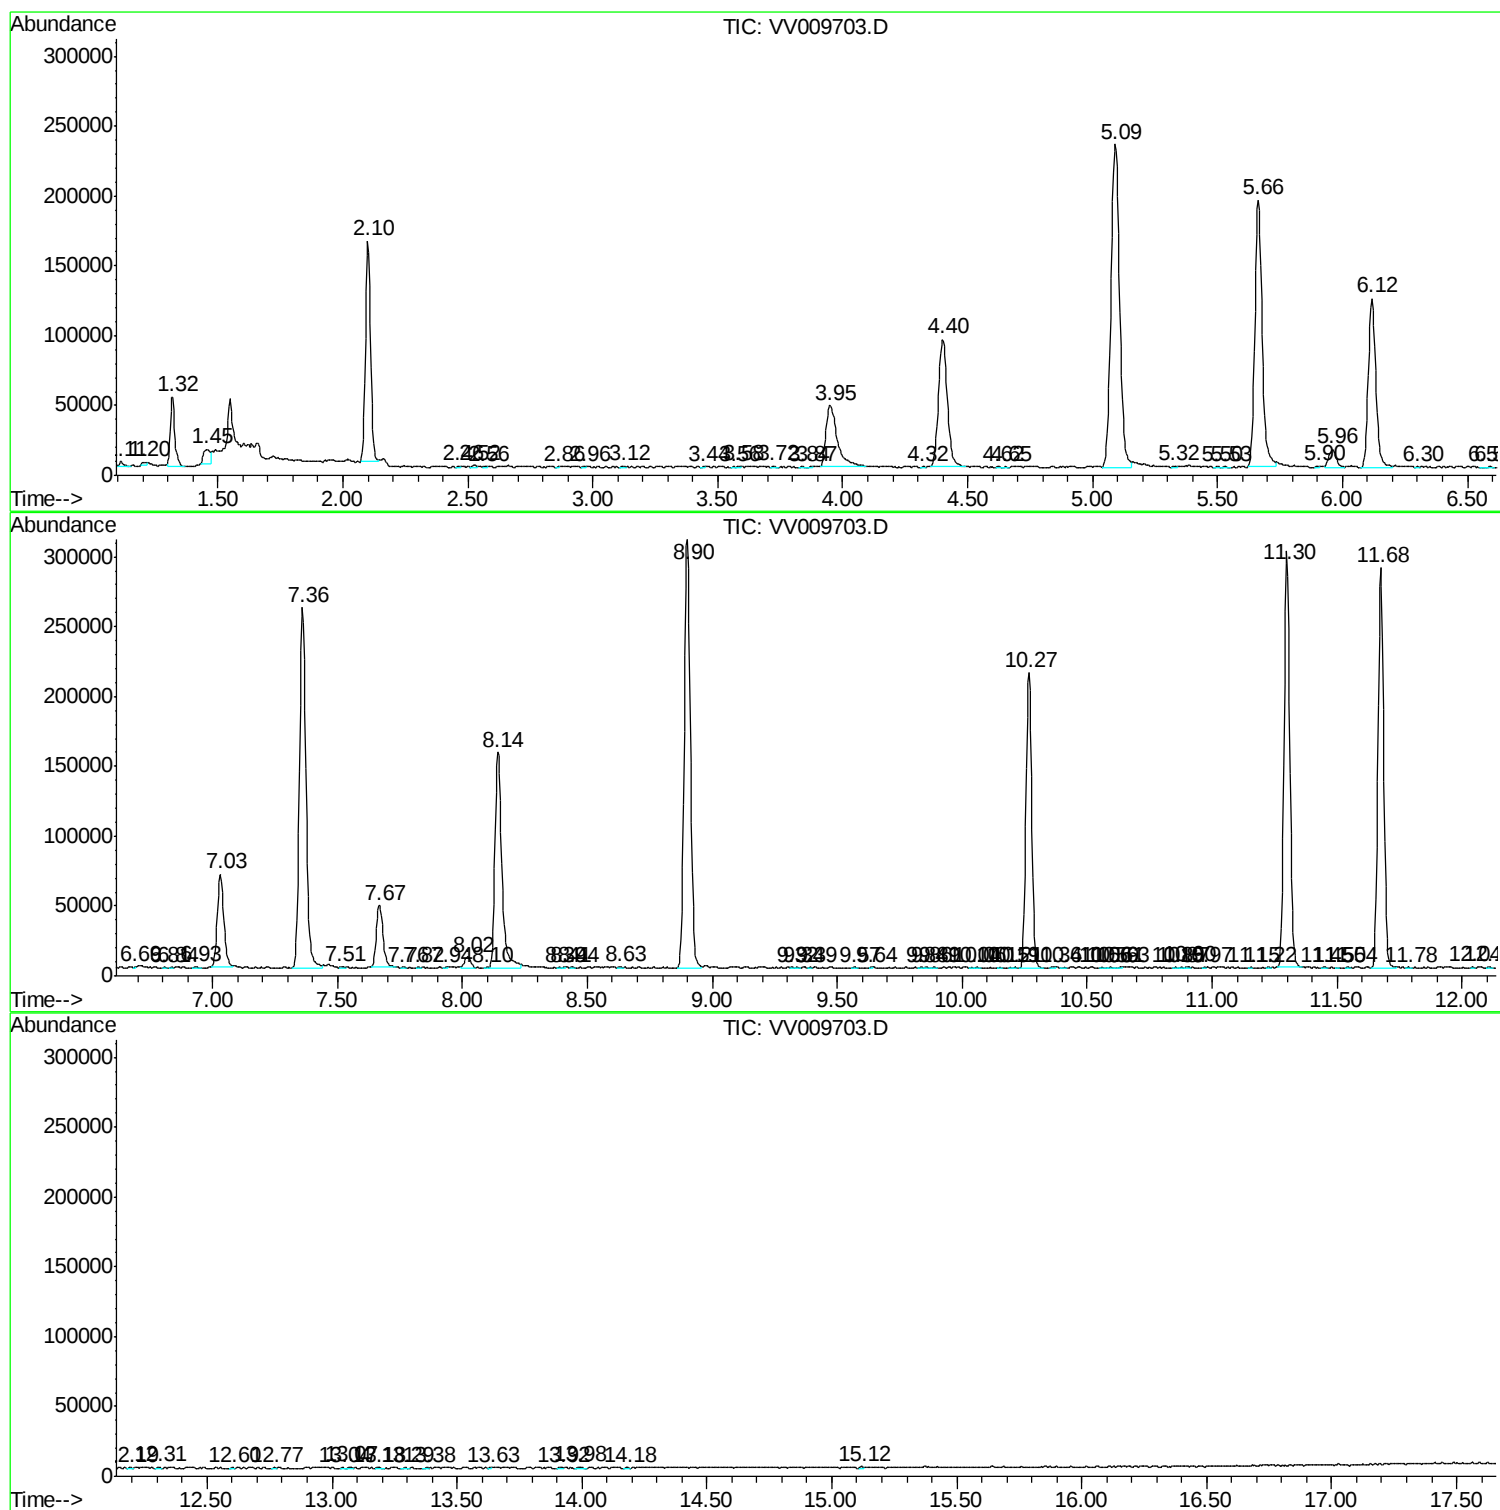

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV031619\
Data File : VV009703.D
Acq On : 15 Mar 2019 22:22
Operator : SY/MD
Sample : K1939-20ME
Misc : 5.30g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BF0Y3ME

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV031619\
Data File : VV009703.D
Acq On : 15 Mar 2019 22:22
Operator : SY/MD
Sample : K1939-20ME
Misc : 5.30g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BF0Y3ME

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc