

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031619\
 Data File : VV009724.D
 Acq On : 16 Mar 2019 07:21
 Operator : SY/MD
 Sample : K1936-18
 Misc : 4.60µ/5.0mL/100µL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFOX6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031219WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.113	3	7	12	rVB2	3225	2911	0.52%	0.062%
2	1.139	12	15	17	rBV	786	542	0.10%	0.012%
3	1.203	29	35	46	rBV3	3601	7017	1.26%	0.150%
4	1.319	64	71	84	rVB	49144	58760	10.55%	1.253%
5	1.450	104	112	116	rBV	11553	17599	3.16%	0.375%
6	2.100	305	314	326	rVB	147198	209066	37.54%	4.458%
7	2.325	379	384	386	rBV2	627	609	0.11%	0.013%
8	2.746	513	515	521	rBV	707	609	0.11%	0.013%
9	2.904	561	564	566	rBV2	555	434	0.08%	0.009%
10	3.032	601	604	608	rBV	876	701	0.13%	0.015%
11	3.087	618	621	624	rBV	755	609	0.11%	0.013%
12	3.389	712	715	716	rBV2	476	283	0.05%	0.006%
13	3.553	763	766	769	rBV	721	497	0.09%	0.011%
14	3.685	805	807	811	rBV	574	363	0.07%	0.008%
15	3.855	856	860	863	rBV	678	557	0.10%	0.012%
16	3.949	875	889	918	rBV2	31053	105973	19.03%	2.260%
17	4.267	980	988	990	rBV	600	799	0.14%	0.017%
18	4.312	1000	1002	1005	rBV	428	224	0.04%	0.005%
19	4.399	1014	1029	1058	rVB2	88444	224484	40.30%	4.787%
20	4.695	1118	1121	1124	rBV	829	635	0.11%	0.014%
21	4.936	1194	1196	1198	rBV	529	319	0.06%	0.007%
22	5.010	1216	1219	1220	rBV	843	497	0.09%	0.011%
23	5.090	1228	1244	1264	rBV2	230272	556965	100.00%	11.877%
24	5.453	1354	1357	1360	rBV	562	497	0.09%	0.011%
25	5.479	1363	1365	1368	rVB	909	483	0.09%	0.010%
26	5.505	1368	1373	1375	rBV2	538	513	0.09%	0.011%
27	5.524	1376	1379	1382	rBV	526	367	0.07%	0.008%
28	5.662	1406	1422	1447	rBV2	190767	408129	73.28%	8.703%
29	5.894	1491	1494	1499	rBV2	556	682	0.12%	0.015%
30	6.116	1551	1563	1580	rBV	118981	246442	44.25%	5.255%
31	6.363	1635	1640	1642	rBV	561	595	0.11%	0.013%
32	6.457	1664	1669	1673	rBV	908	967	0.17%	0.021%
33	6.617	1717	1719	1723	rVB	683	377	0.07%	0.008%
34	6.643	1723	1727	1733	rVB	758	641	0.12%	0.014%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031619\
 Data File : VV009724.D
 Acq On : 16 Mar 2019 07:21
 Operator : SY/MD
 Sample : K1936-18
 Misc : 4.60uL/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFOX6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031219WMA.M
 Title : VOC Analysis

35	6.949	1819	1822	1824	rBV	430	295	0.05%	0.006%
36	7.032	1834	1848	1866	rBV2	61316	118593	21.29%	2.529%
37	7.177	1890	1893	1896	rBV	661	509	0.09%	0.011%
38	7.280	1919	1925	1931	rVB	1125	1419	0.25%	0.030%
39	7.305	1931	1933	1935	rBV	390	236	0.04%	0.005%
40	7.360	1935	1950	1971	rBV	264099	474448	85.18%	10.117%
41	7.630	2031	2034	2035	rBV	504	282	0.05%	0.006%
42	7.666	2035	2045	2064	rVV2	42484	82023	14.73%	1.749%
43	7.765	2073	2076	2081	rBV	571	569	0.10%	0.012%
44	7.817	2088	2092	2094	rBV	478	382	0.07%	0.008%
45	7.952	2131	2134	2135	rBV	412	237	0.04%	0.005%
46	8.019	2145	2155	2169	rVB2	22422	39103	7.02%	0.834%
47	8.145	2181	2194	2221	rBV	145631	283049	50.82%	6.036%
48	8.360	2258	2261	2265	rBV	703	587	0.11%	0.013%
49	8.405	2272	2275	2278	rBV	701	600	0.11%	0.013%
50	8.633	2341	2346	2352	rBV	808	1144	0.21%	0.024%
51	8.900	2417	2429	2453	rVB	310213	530776	95.30%	11.318%
52	9.267	2539	2543	2545	rBV	507	456	0.08%	0.010%
53	9.347	2565	2568	2569	rBV	541	285	0.05%	0.006%
54	9.402	2579	2585	2588	rVV	841	982	0.18%	0.021%
55	9.437	2592	2596	2603	rVB	996	1002	0.18%	0.021%
56	9.469	2603	2606	2609	rBV	908	607	0.11%	0.013%
57	9.489	2609	2612	2616	rVV2	522	368	0.07%	0.008%
58	9.524	2620	2623	2627	rVB	841	562	0.10%	0.012%
59	9.579	2637	2640	2641	rBV2	464	249	0.04%	0.005%
60	9.749	2688	2693	2698	rBV2	632	729	0.13%	0.016%
61	9.826	2713	2717	2719	rBV	508	283	0.05%	0.006%
62	9.839	2719	2721	2723	rBV	306	187	0.03%	0.004%
63	10.029	2777	2780	2785	rBV	763	730	0.13%	0.016%
64	10.055	2785	2788	2790	rBV	571	400	0.07%	0.009%
65	10.267	2843	2854	2872	rVB	207395	326308	58.59%	6.958%
66	10.421	2899	2902	2906	rBV3	743	513	0.09%	0.011%
67	10.498	2923	2926	2931	rBV	459	349	0.06%	0.007%
68	10.710	2984	2992	2995	rBV	874	1221	0.22%	0.026%
69	10.752	3001	3005	3008	rBV	793	554	0.10%	0.012%
70	10.797	3015	3019	3025	rBV	631	764	0.14%	0.016%
71	10.961	3066	3070	3073	rBV	601	483	0.09%	0.010%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031619\
 Data File : VV009724.D
 Acq On : 16 Mar 2019 07:21
 Operator : SY/MD
 Sample : K1936-18
 Misc : 4.60µ/5.0mL/100µL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFOX6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031219WMA.M
 Title : VOC Analysis

72	11.106	3112	3115	3119	rVV	803	652	0.12%	0.014%
73	11.299	3163	3175	3193	rVB	315304	502191	90.17%	10.709%
74	11.363	3193	3195	3197	rBV	515	254	0.05%	0.005%
75	11.453	3218	3223	3224	rBV	376	341	0.06%	0.007%
76	11.556	3252	3255	3257	rBV	459	252	0.05%	0.005%
77	11.675	3280	3292	3307	rBV	283454	452533	81.25%	9.650%
78	11.858	3345	3349	3351	rBV	973	707	0.13%	0.015%
79	11.948	3374	3377	3379	rBV	596	387	0.07%	0.008%
80	11.990	3386	3390	3397	rBV	655	836	0.15%	0.018%
81	12.170	3443	3446	3448	rBV	691	473	0.08%	0.010%
82	12.225	3457	3463	3466	rBV2	470	591	0.11%	0.013%
83	12.408	3517	3520	3525	rVB	677	601	0.11%	0.013%
84	12.437	3525	3529	3533	rBV	1036	793	0.14%	0.017%
85	12.517	3550	3554	3556	rBV	563	459	0.08%	0.010%
86	12.611	3580	3583	3586	rBV	451	416	0.07%	0.009%
87	12.685	3602	3606	3608	rBV	554	404	0.07%	0.009%
88	12.726	3616	3619	3626	rBV2	527	604	0.11%	0.013%
89	12.897	3669	3672	3676	rVB	1066	692	0.12%	0.015%
90	13.292	3793	3795	3797	rBV	573	318	0.06%	0.007%
91	13.395	3824	3827	3829	rBV	492	376	0.07%	0.008%
92	13.431	3835	3838	3841	rBV	900	657	0.12%	0.014%
93	13.598	3887	3890	3893	rBV	488	333	0.06%	0.007%
94	13.739	3932	3934	3936	rBV	426	236	0.04%	0.005%
95	14.000	4012	4015	4018	rBV	640	436	0.08%	0.009%
96	14.077	4035	4039	4040	rBV	458	357	0.06%	0.008%
97	14.148	4057	4061	4065	rBV2	624	609	0.11%	0.013%
98	14.244	4088	4091	4095	rBV	493	299	0.05%	0.006%
99	14.701	4230	4233	4237	rBV2	1080	835	0.15%	0.018%
100	15.080	4347	4351	4352	rBV	730	529	0.09%	0.011%


Sum of corrected areas: 4689601

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV031619\
Data File : VV009724.D
Acq On : 16 Mar 2019 07:21
Operator : SY/MD
Sample : K1936-18
Misc : 4.60µ/5.0mL/100µL/5.0mL/MSVOA_V/MEOH
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
BFOX6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

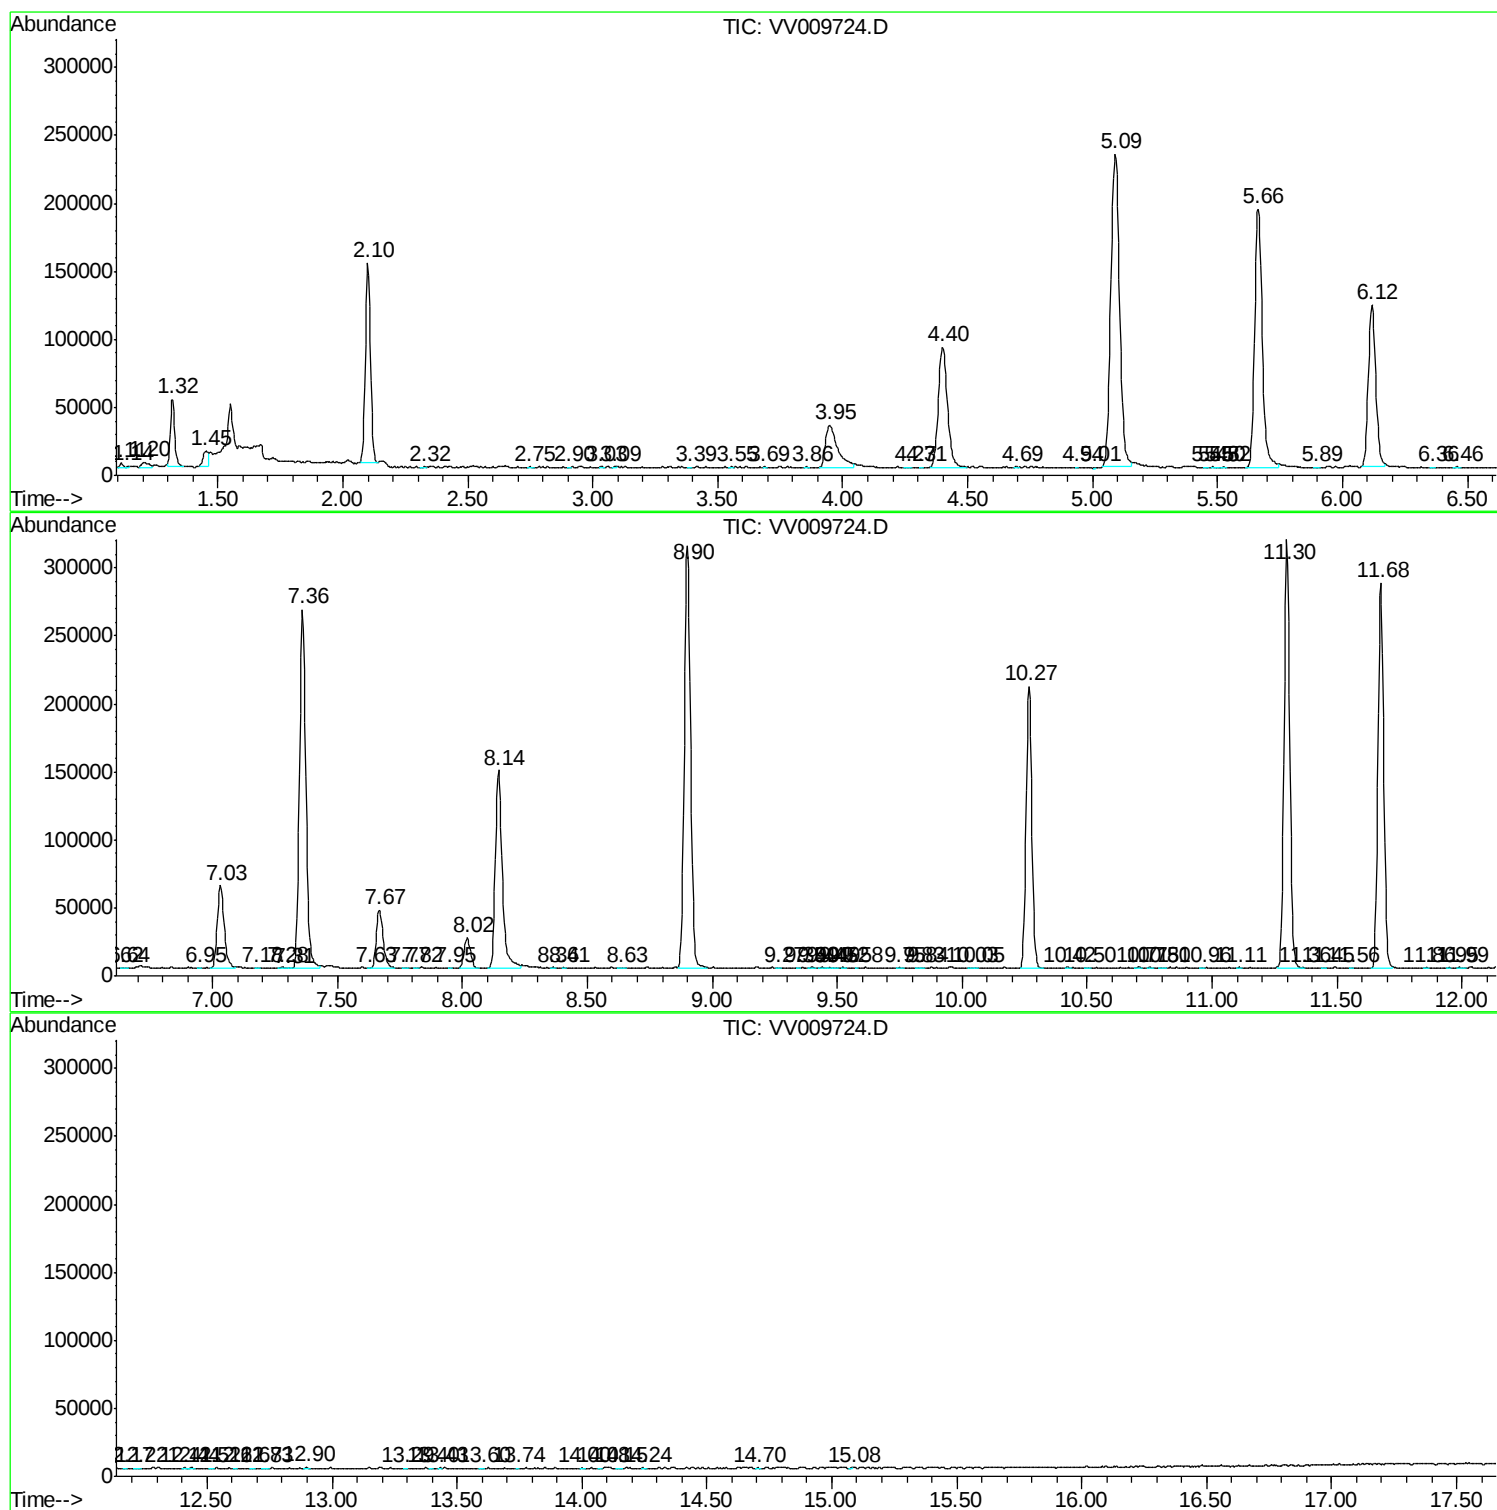

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV031619\
Data File : VV009724.D
Acq On : 16 Mar 2019 07:21
Operator : SY/MD
Sample : K1936-18
Misc : 4.60g/5.0mL/100uL/5.0mL/MSV0A_V/MEOH
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
BF0X6

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM031219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV031619\
Data File : VV009724.D
Acq On : 16 Mar 2019 07:21
Operator : SY/MD
Sample : K1936-18
Misc : 4.60g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BF0X6

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc