


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV031619\
Data File : VV009684.D
Acq On : 15 Mar 2019 13:58
Operator : SY/MD
Sample : BFB78
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB78

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031219WMA.M
Title : VOC Analysis
Last Update : Sat Mar 16 02:32:06 2019

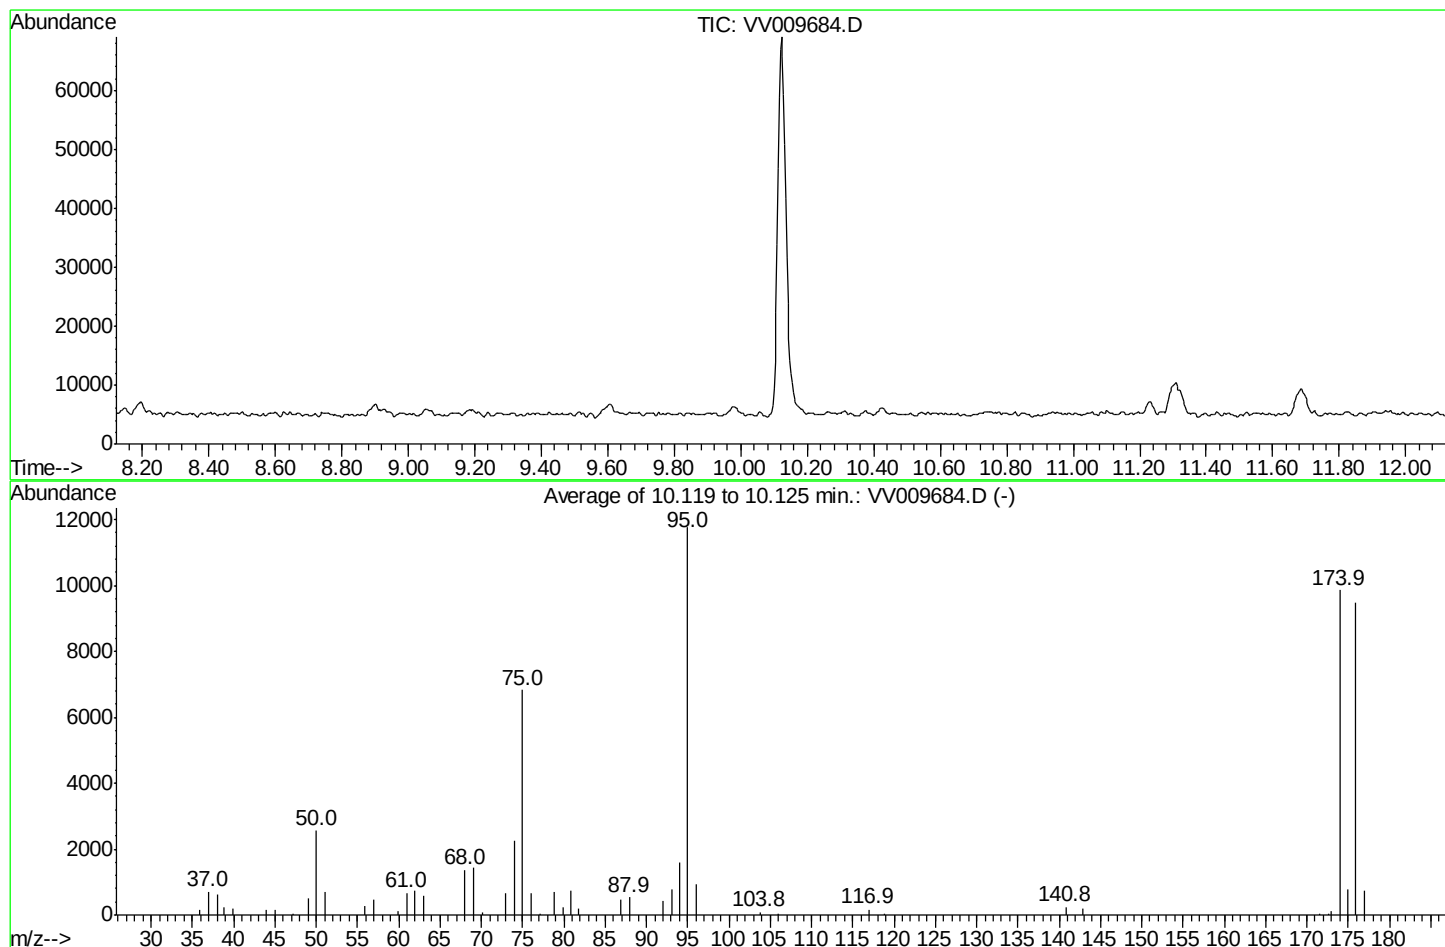

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2798

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.7	2553	PASS
75	95	30	80	58.0	6829	PASS
95	95	100	100	100.0	11766	PASS
96	95	5	9	7.9	933	PASS
173	174	0.00	2	1.1	113	PASS
174	95	50	120	83.8	9860	PASS
175	174	5	9	7.9	778	PASS
176	174	95	101	96.1	9480	PASS
177	176	5	9	7.6	721	PASS

Scan 2798 (10.087 min): VV009684.D
BFB78

m/z	Abundance
39.90	4738.0
43.90	185.0

Instrument :
MSVOA_V
ClientSampleId :
BFB78

m/z	Abundance
35.00	168.0
36.00	668.0
38.00	693.0
38.90	273.0
39.00	4933.0
44.00	277.0
44.90	165.0
49.00	468.0
50.00	2577.0
51.00	665.0
55.90	289.0
57.00	413.0
59.90	122.0
60.00	696.0
61.90	754.0
63.00	518.0
68.00	1412.0
69.00	1528.0
73.00	653.0
74.00	2215.0
75.00	6860.0
76.00	713.0
78.90	704.0
79.80	258.0
80.80	766.0
81.80	174.0
87.00	521.0
87.90	540.0
92.00	440.0
93.00	861.0
94.00	1655.0
95.00	11793.0
96.00	913.0
106.00	101.0
117.00	135.0
118.80	121.0
140.80	283.0
142.90	214.0
172.90	203.0
173.90	9607.0
175.00	755.0
175.90	9093.0
176.90	775.0

Instrument :
MSVOA_V
ClientSampleId :
BFB78

m/z	Abundance
35.80	159.0
36.90	751.0
38.00	654.0
38.80	237.0
39.90	4867.0
43.90	329.0
44.90	169.0
49.00	505.0
50.00	2647.0
51.00	725.0
55.90	283.0
57.00	485.0
59.80	136.0
60.90	703.0
61.90	755.0
63.00	598.0
68.00	1391.0
69.00	1477.0
70.10	119.0
73.00	674.0
74.00	2343.0
75.00	6969.0
76.00	708.0
78.90	727.0
79.80	263.0
80.90	745.0
81.80	201.0
86.90	500.0
87.90	553.0
92.00	456.0
93.10	842.0
94.00	1620.0
95.00	12066.0
96.00	958.0
103.70	109.0
116.90	163.0
140.80	240.0
142.90	208.0
171.60	101.0
172.90	136.0
174.00	10175.0
174.90	794.0
175.90	9785.0
176.90	755.0

Instrument :
MSVOA_V
ClientSampleId :
BFB78

m/z	Abundance
35.80	125.0
37.00	691.0
38.00	521.0
38.80	177.0
39.90	4955.0
43.90	371.0
45.00	150.0
47.20	112.0
49.00	490.0
50.00	2437.0
51.00	745.0
56.00	305.0
57.00	461.0
59.80	129.0
61.00	640.0
62.00	706.0
63.00	653.0
68.00	1303.0
69.00	1269.0
70.10	111.0
73.00	631.0
74.00	2190.0
75.00	6658.0
76.00	599.0
77.10	110.0
78.90	684.0
79.90	235.0
80.90	758.0
81.80	178.0
87.00	398.0
87.90	491.0
91.90	415.0
93.10	672.0
94.00	1474.0
95.00	11441.0
96.00	928.0
103.80	126.0
116.80	197.0
140.80	196.0
142.90	170.0
172.60	117.0
174.00	9799.0
174.90	786.0
175.90	9562.0
176.90	634.0

Instrument :
MSVOA_V
ClientSampleId :
BFB78