


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031620\
Data File : VV014952.D
Acq On : 16 Mar 2020 17:43
Operator : SY/MD
Sample : L1890-17
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 22 Sample Multiplier: 1

Quant Time: Mar 18 04:24:09 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Mar 18 03:17:46 2020
Response via : Initial Calibration

Instrument :
MSVOA_V
Client Sampled :
C0DH4

Manual Integrations
APPROVED

apatel
3/18/2020 3:12:24 PM

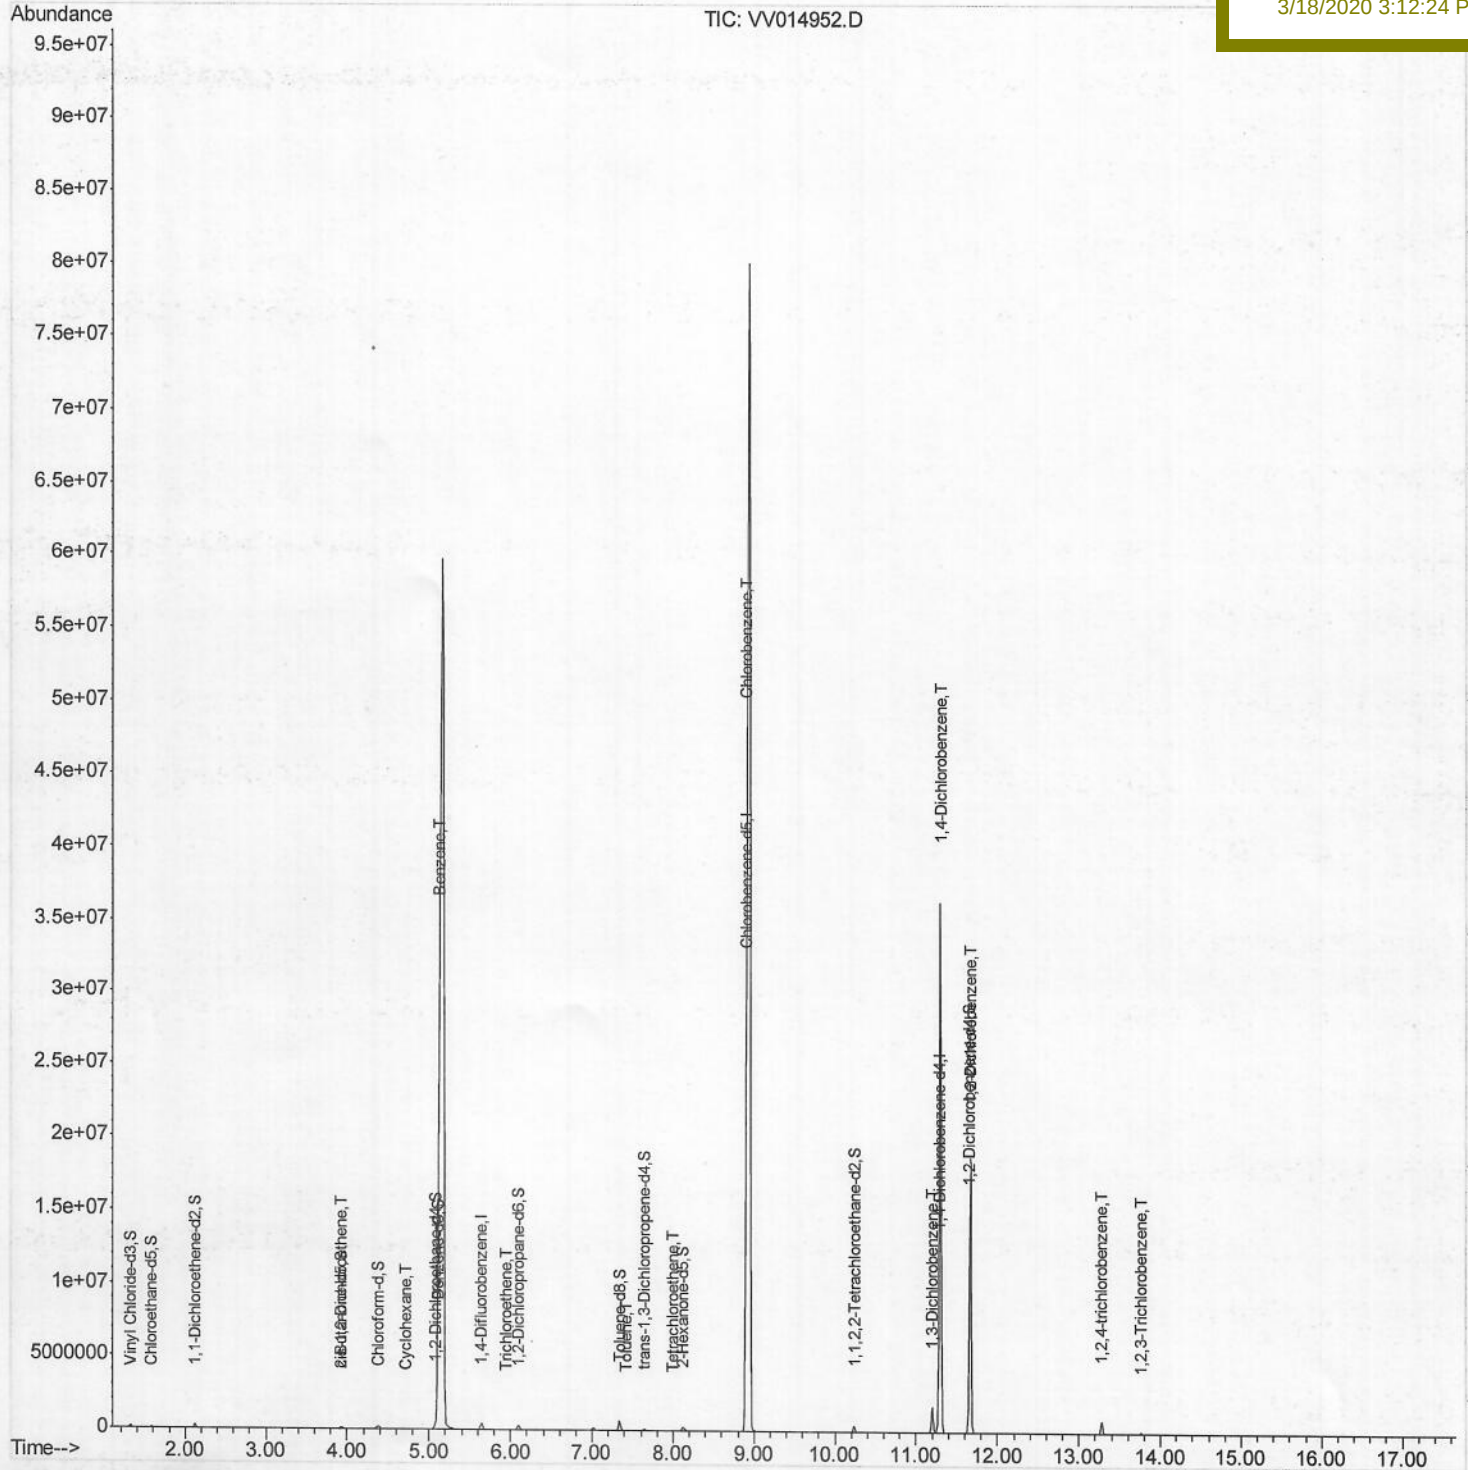

Quantitation Report (Qedit)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031620\

Data File : VV014952.D

Acq On : 16 Mar 2020 17:43

Operator : SY/MD

Sample : L1890-17

Misc : 5.0mL/MSVOA V/WATER

ALS Vial : 22 Sample Multiplier: 1

Quant Time: Mar 18 03:21:07 2020

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M

Quant Title : VOC Analysis

QLast Update : Wed Mar 18 03:17:46 2020

Response via : Initial Calibration

Instrument :

MSVOA_V

ClientSampleId :




C0DH4

Manual Integrations

APPROVED

apatel

3/18/2020 3:12:24 PM

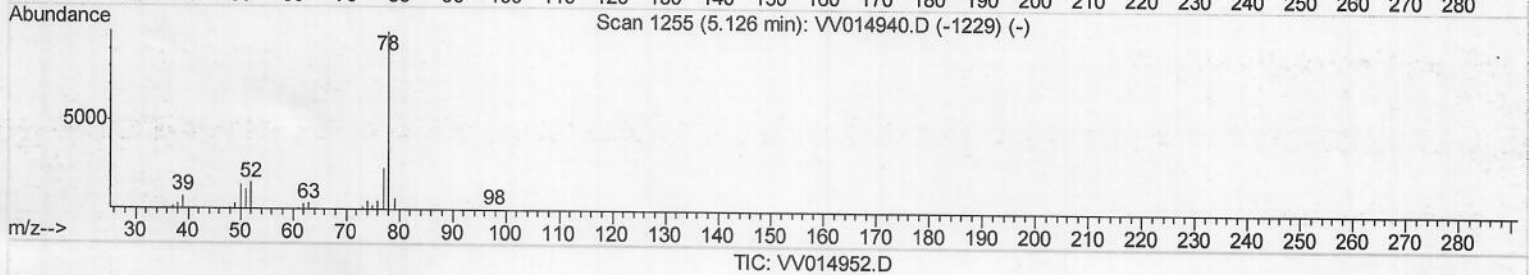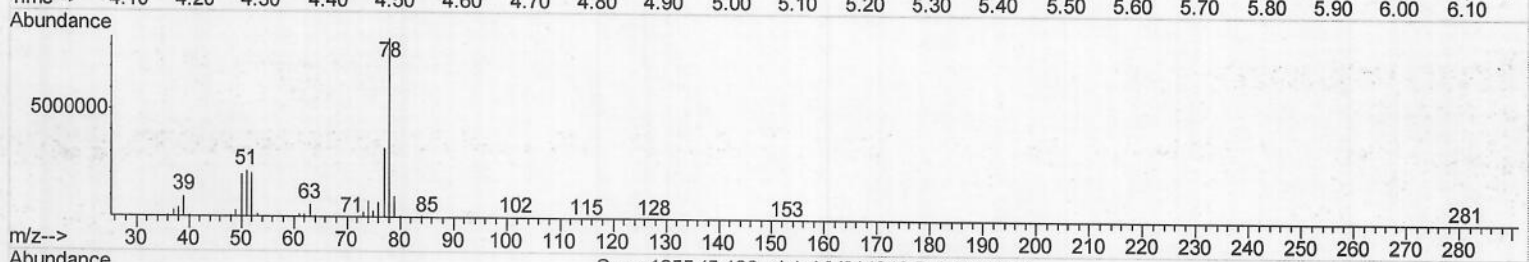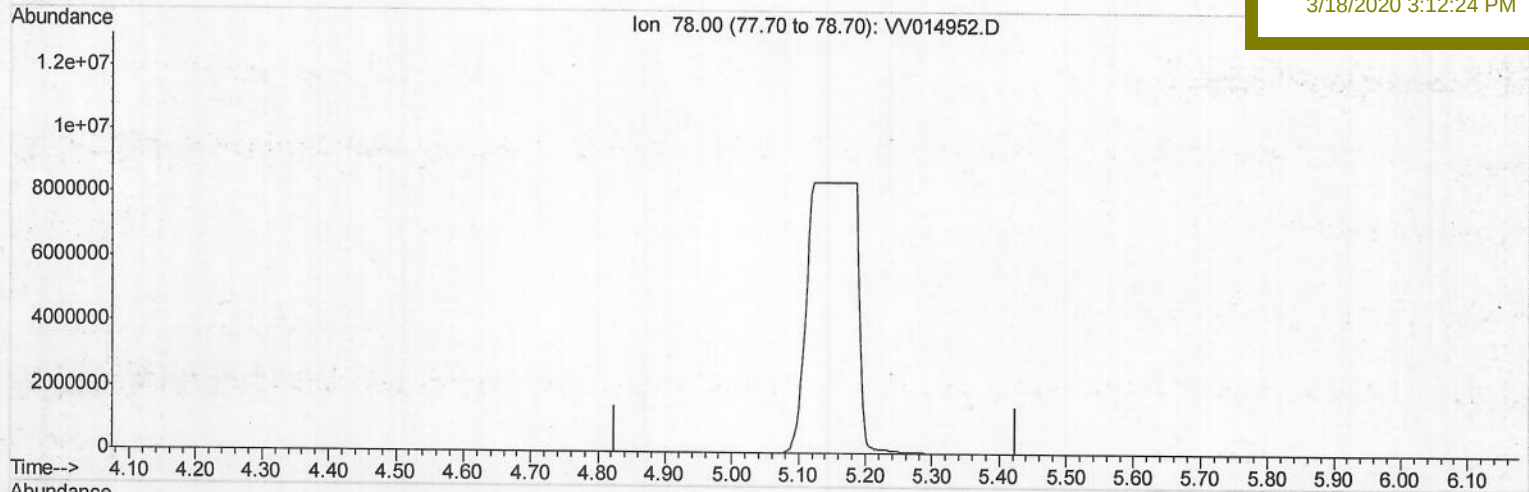

(33) Benzene (T)

5.126min (-5.126) 0.00ug/L

response 0

Ion	Exp%	Act%
78.00	100	0.00
0.00	0.00	0.00
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031620\
 Data File : VV014952.D
 Acq On : 16 Mar 2020 17:43
 Operator : SY/MD
 Sample : L1890-17
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
ClientSampleId :
 C0DH4

Manual Integrations
APPROVED

apatel
 3/18/2020 3:12:24 PM

Quant Time: Mar 18 03:21:07 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Mar 18 03:17:46 2020
 Response via : Initial Calibration

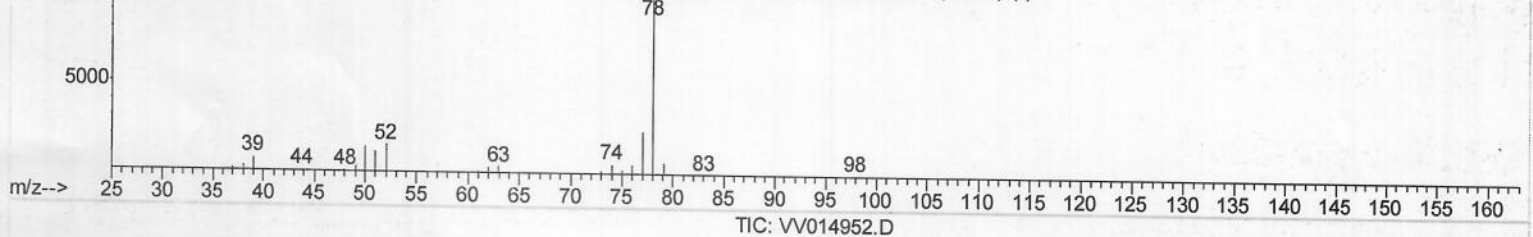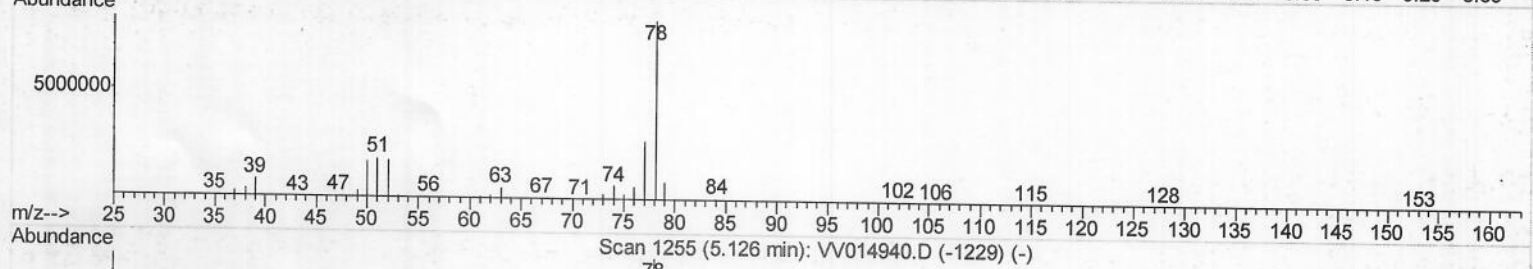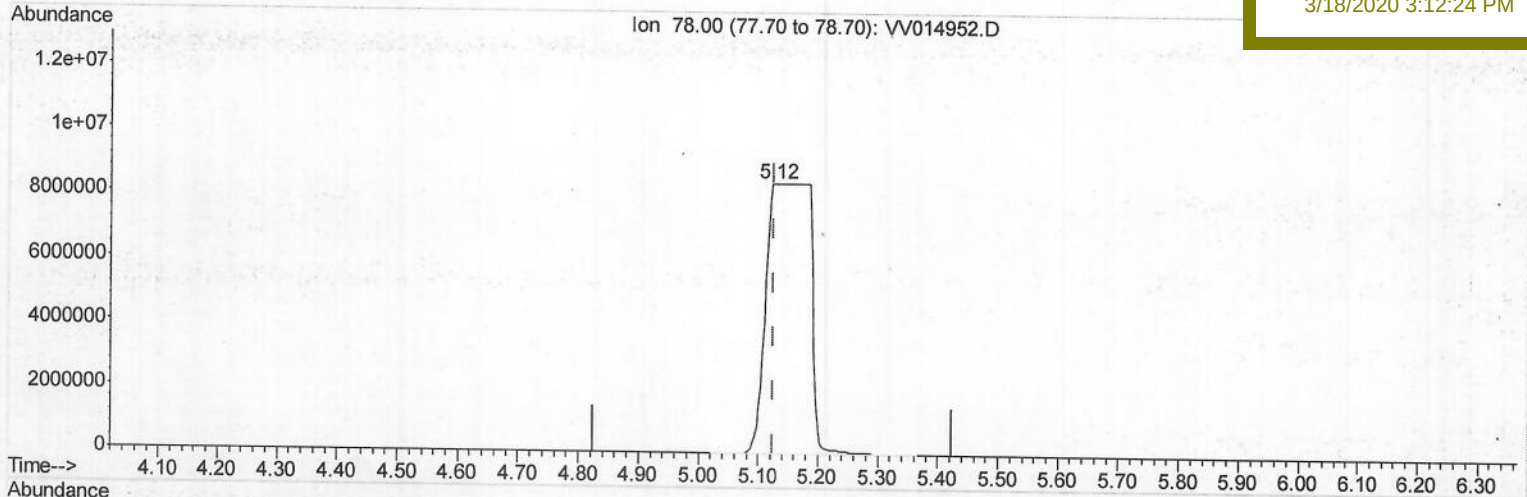

(33) Benzene (T)

5.122min (-0.003) 4150.71ug/L m

response 43042106

Ion	Exp%	Act%
78.00	100	100
0.00	0.00	0.00
0.00	0.00	0.00
0.00	0.00	0.00

M. 8
 03/20/20

Quantitation Report (Qedit)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031620\

Data File : VV014952.D

Acq On : 16 Mar 2020 17:43

Operator : SY/MD

Sample : L1890-17

Misc : 5.0mL/MSVOA V/WATER

ALS Vial : 22 Sample Multiplier: 1

Quant Time: Mar 18 03:21:07 2020

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M

Quant Title : VOC Analysis

QLast Update : Wed Mar 18 03:17:46 2020

Response via : Initial Calibration

Instrument :

MSVOA_V




ClientSampleId :

C0DH4

Manual Integrations
APPROVED

apatel

3/18/2020 3:12:24 PM

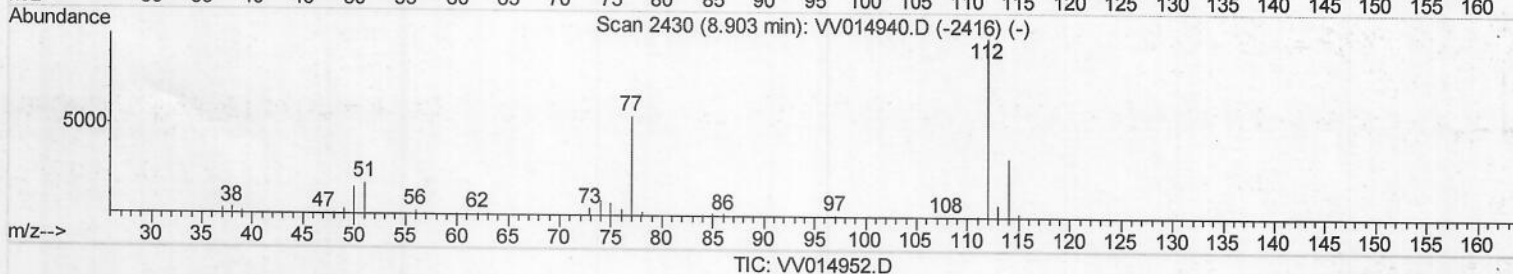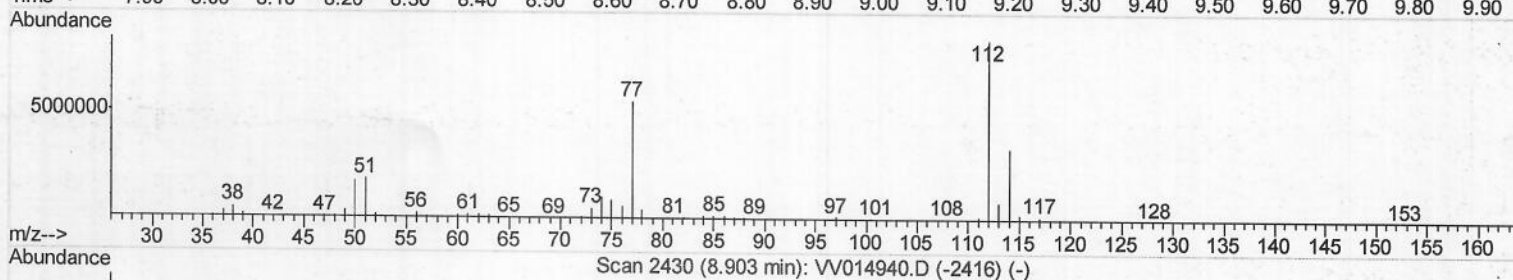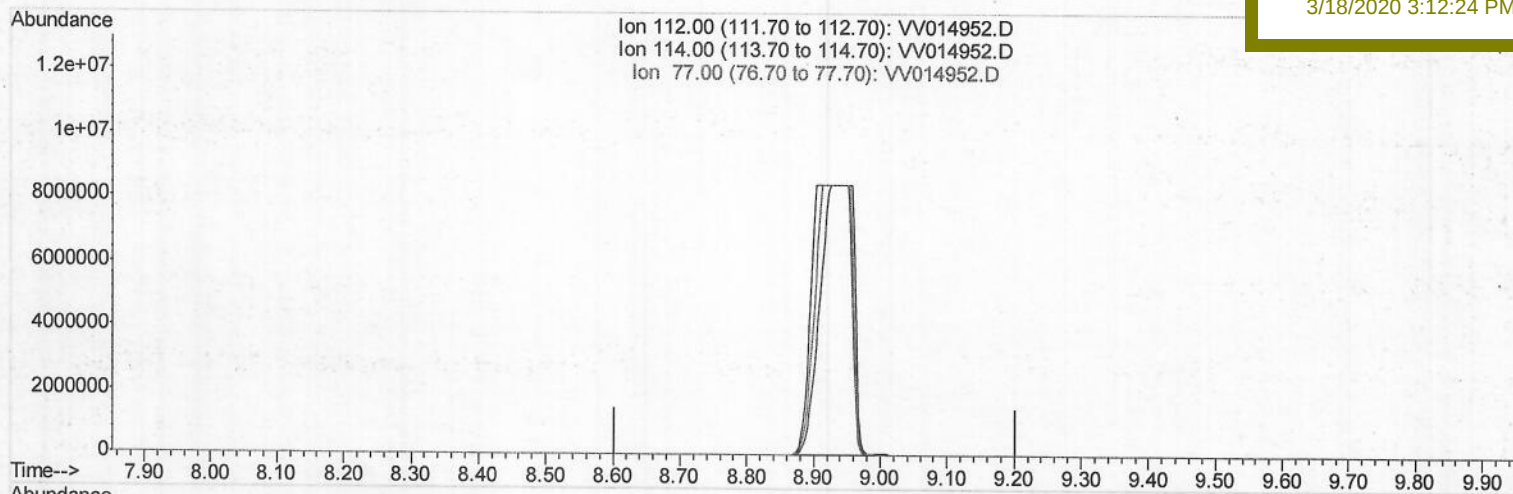

(51) Chlorobenzene (T)

8.903min (-8.903) 0.00ug/L

response 0

Ion	Exp%	Act%
112.00	100	0.00
114.00	32.60	0.00#
77.00	55.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031620\

Data File : VV014952.D

Acq On : 16 Mar 2020 17:43

Operator : SY/MD

Sample : L1890-17

Misc : 5.0mL/MSVOA V/WATER

ALS Vial : 22 Sample Multiplier: 1

Quant Time: Mar 18 03:21:07 2020

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M

Quant Title : VOC Analysis

QLast Update : Wed Mar 18 03:17:46 2020

Response via : Initial Calibration

Instrument :

MSVOA_V




ClientSampleId :

C0DH4

Manual Integrations
APPROVED

apatel

3/18/2020 3:12:24 PM

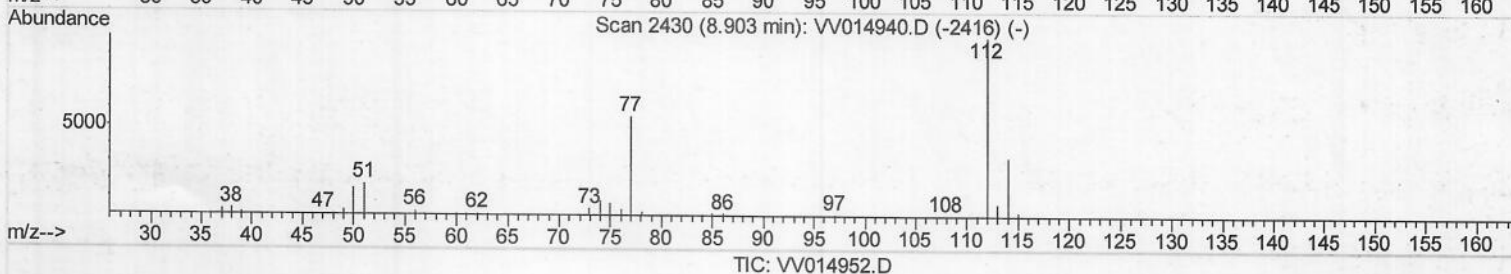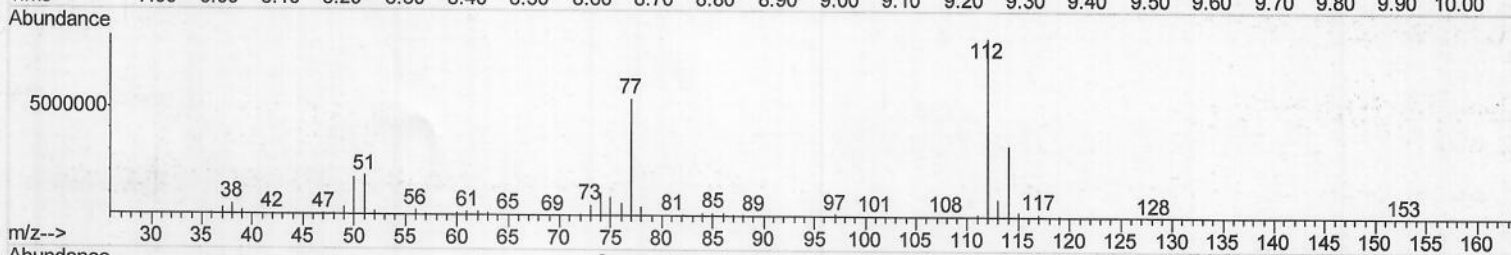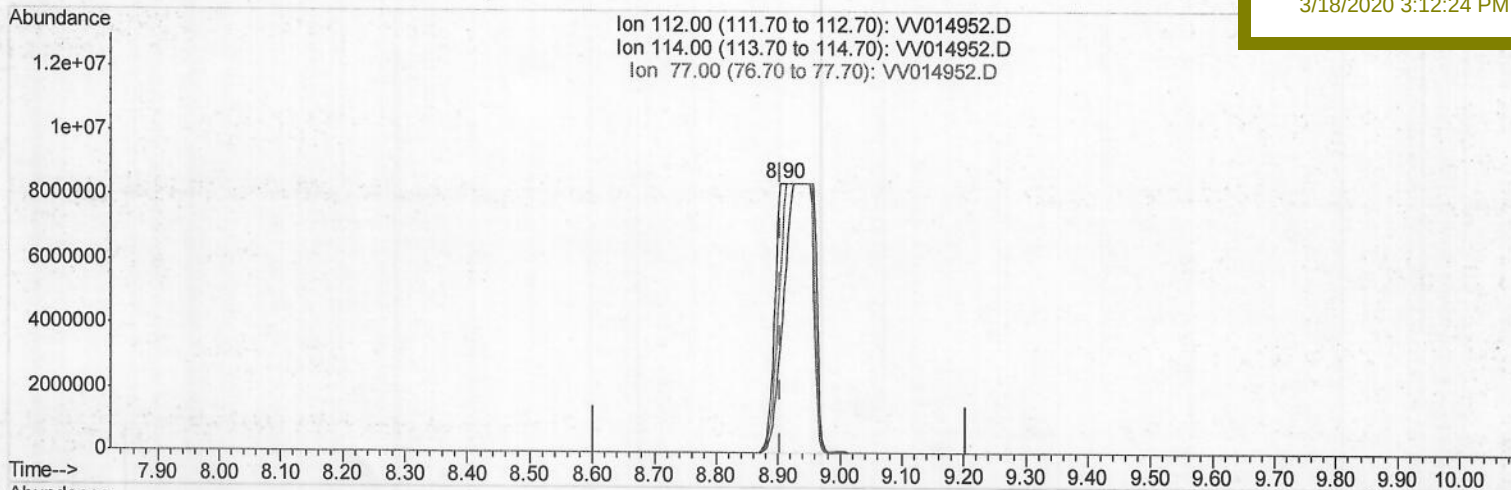

(51) Chlorobenzene (T)

8.903min (-0.000) 4469.45ug/L m

response 35913490

Ion	Exp%	Act%
112.00	100	100
114.00	32.60	39.94
77.00	55.60	65.23
0.00	0.00	0.00

M. 8

03/20/20

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031620\
 Data File : VV014952.D
 Acq On : 16 Mar 2020 17:43
 Operator : SY/MD
 Sample : L1890-17
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Quant Time: Mar 18 03:21:07 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Mar 18 03:17:46 2020
 Response via : Initial Calibration

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DH4

Manual Integrations
 APPROVED

apatel
 3/18/2020 3:12:24 PM

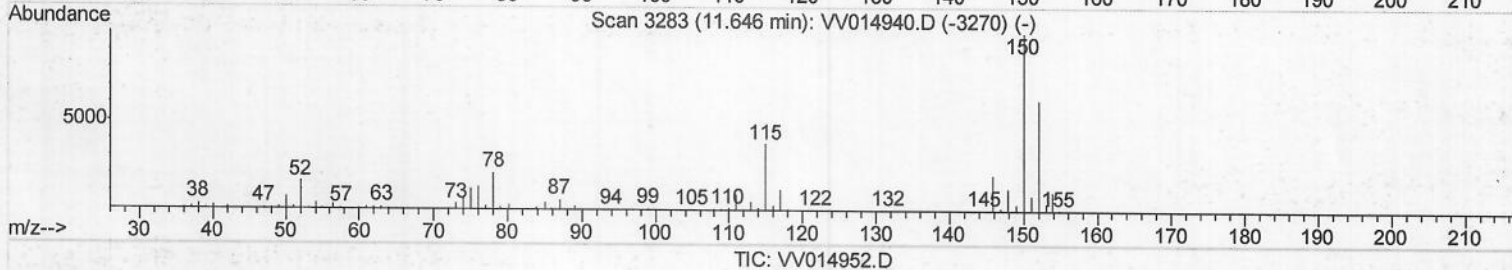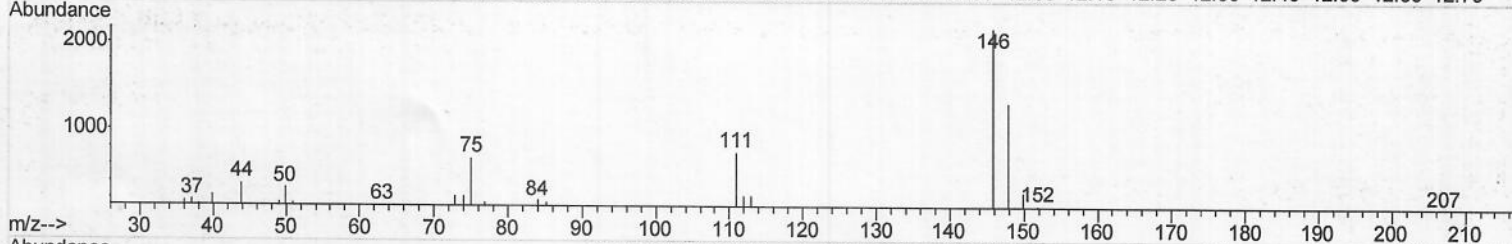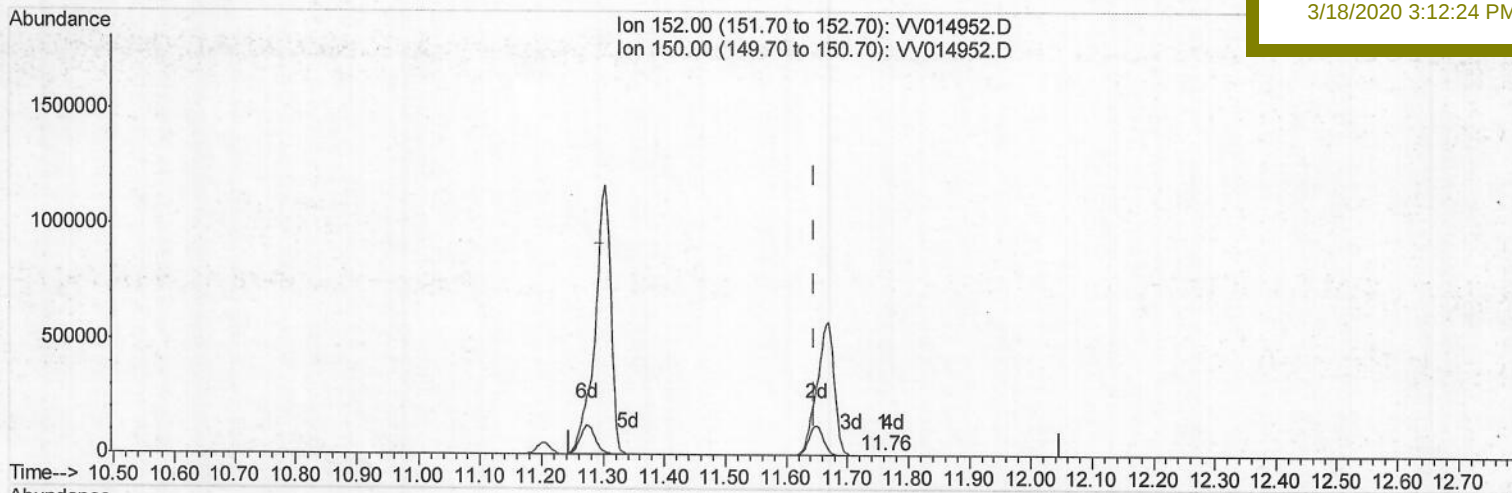

(64) 1,2-Dichlorobenzene-d4 (S)

11.759min (+0.112) 0.01ug/L

response 48

Ion	Exp%	Act%
152.00	100	100
150.00	172.10	125.00
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031620\

Data File : VV014952.D

Acq On : 16 Mar 2020 17:43

Operator : SY/MD

Sample : L1890-17

Misc : 5.0mL/MSVOA V/WATER

ALS Vial : 22 Sample Multiplier: 1

Quant Time: Mar 18 03:21:07 2020

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA V\METHOD\SOMVLM031620WMA.M

Quant Title : VOC Analysis

QLast Update : Wed Mar 18 03:17:46 2020

Response via : Initial Calibration

Instrument :

MSVOA_V

ClientSampleId :




C0DH4

Manual Integrations

APPROVED

apatel

3/18/2020 3:12:24 PM

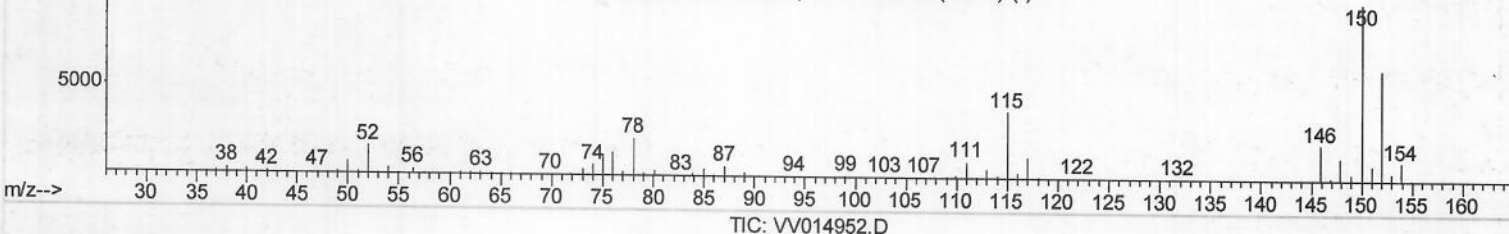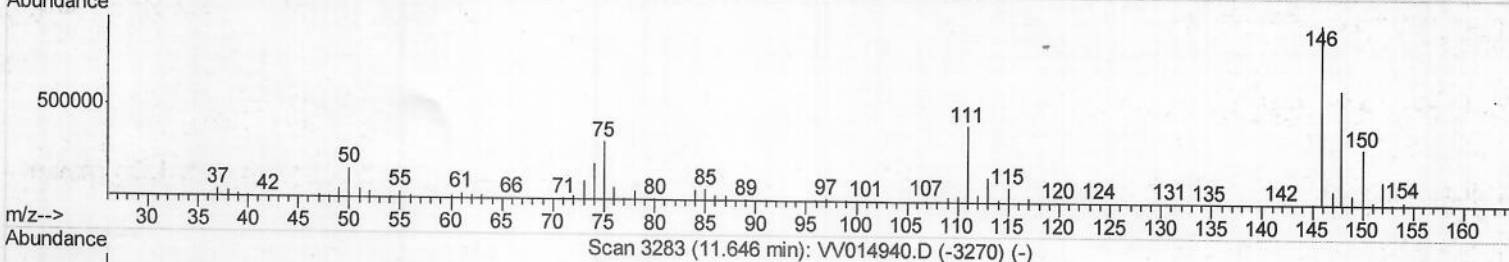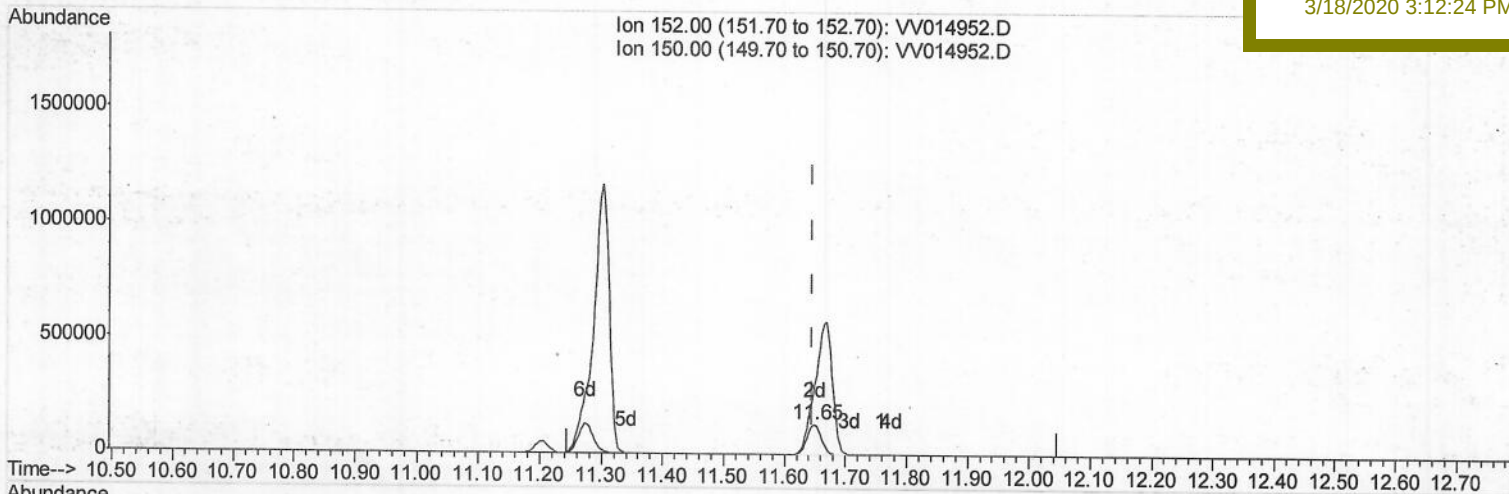

(64) 1,2-Dichlorobenzene-d4 (S)

11.649min (+0.003) 44.95ug/L m)

response 214103

Ion Exp% Act%

152.00 100 100

150.00 172.10 0.03#

0.00 0.00 0.00

0.00 0.00 0.00

M.8
03/20/20

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031620\
 Data File : VV014952.D
 Acq On : 16 Mar 2020 17:43
 Operator : SY/MD
 Sample : L1890-17
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DH4

Quant Time: Mar 18 04:24:09 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Mar 18 03:17:46 2020
 Response via : Initial Calibration

Manual Integrations
 APPROVED

apatel
 3/18/2020 3:12:24 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	374081	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	381089	50.00	ug/L	0.02
60) 1,4-Dichlorobenzene-d4	11.27	152	217422	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	106372	42.68	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	85.36%		
7) Chloroethane-d5	1.58	69	80226	43.34	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	86.68%		
11) 1,1-Dichloroethene-d2	2.12	63	130172	34.04	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	68.08%		
21) 2-Butanone-d5	3.93	46	120874	79.55	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	79.55%		
24) Chloroform-d	4.38	84	223318	43.01	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	86.02%		
26) 1,2-Dichloroethane-d4	5.07	65	152671	46.41	ug/L	0.01
Spiked Amount 50.000	Range 70 - 125		Recovery =	92.82%		
32) Benzene-d6	5.09	84	468868	44.66	ug/L	0.02
Spiked Amount 50.000	Range 70 - 125		Recovery =	89.32%		
36) 1,2-Dichloropropane-d6	6.10	67	135564	43.36	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	86.72%		
41) Toluene-d8	7.34	98	458513	44.16	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	88.32%		
43) trans-1,3-Dichloropropene-	7.64	79	68285	41.08	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	82.16%		
47) 2-Hexanone-d5	8.12	63	122046	86.49	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	86.49%		
57) 1,1,2,2-Tetrachloroethane-	10.24	84	193766	42.34	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	84.68%		
64) 1,2-Dichlorobenzene-d4	11.65	152	214103m	44.95	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	89.90%		

Target Compounds

					Ovalue
20) cis-1,2-Dichloroethene	3.94	96	6827	2.429	ug/L 97
29) Cyclohexane	4.71	56	6671	1.695	ug/L # 90
33) Benzene	5.12	78	43042106m	4150.711	ug/L
34) Trichloroethene	5.95	95	2156	0.775	ug/L 88
42) Toluene	7.41	91	12353	1.059	ug/L 96
46) Tetrachloroethene	8.00	164	1347	0.518	ug/L 82
51) Chlorobenzene	8.90	112	35913490m	4469.451	ug/L
62) 1,3-Dichlorobenzene	11.20	146	717413	100.129	ug/L 99
63) 1,4-Dichlorobenzene	11.30	146	14513349	2010.884	ug/L 90
65) 1,2-Dichlorobenzene	11.67	146	7663995	1070.831	ug/L 99
68) 1,2,4-trichlorobenzene	13.28	180	271666	54.258	ug/L 100
70) 1,2,3-Trichlorobenzene	13.76	180	21372	4.312	ug/L 97

(#) = qualifier out of range (m) = manual integration (+) = signals summed