

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031620\
 Data File : VV014941.D
 Acq On : 16 Mar 2020 13:17
 Operator : SY/MD
 Sample : VV0316WBL01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK61

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	84	rVB	185937	195457	13.74%	1.820%
2	1.579	145	152	171	rVB	130847	164309	11.55%	1.530%
3	2.122	311	321	339	rVB	281640	410196	28.84%	3.820%
4	2.376	398	400	402	rBV	499	204	0.01%	0.002%
5	2.476	429	431	434	rBV2	422	212	0.01%	0.002%
6	2.502	434	439	441	rBV	479	439	0.03%	0.004%
7	2.634	476	480	485	rBV2	749	697	0.05%	0.006%
8	2.682	489	495	500	rBV3	621	613	0.04%	0.006%
9	2.714	500	505	508	rBV3	379	339	0.02%	0.003%
10	2.785	519	527	529	rBV4	1023	1189	0.08%	0.011%
11	2.826	537	540	542	rBV2	297	193	0.01%	0.002%
12	2.852	544	548	553	rBV3	332	315	0.02%	0.003%
13	2.933	571	573	579	rVB2	455	361	0.03%	0.003%
14	2.987	588	590	593	rBV	522	214	0.02%	0.002%
15	3.032	599	604	606	rBV3	247	262	0.02%	0.002%
16	3.074	614	617	620	rBV	420	240	0.02%	0.002%
17	3.109	624	628	630	rBV	276	180	0.01%	0.002%
18	3.228	661	665	670	rVB2	666	654	0.05%	0.006%
19	3.257	670	674	679	rBV2	377	402	0.03%	0.004%
20	3.309	688	690	695	rVB2	530	307	0.02%	0.003%
21	3.383	710	713	715	rVV3	324	177	0.01%	0.002%
22	3.653	792	797	800	rBV2	369	263	0.02%	0.002%
23	3.711	810	815	816	rBV2	414	241	0.02%	0.002%
24	3.762	829	831	835	rVB	454	187	0.01%	0.002%
25	3.929	871	883	902	rBV2	55755	190450	13.39%	1.774%
26	4.379	1005	1023	1051	rBV	226612	565935	39.79%	5.271%
27	4.691	1117	1120	1121	rBV	495	299	0.02%	0.003%
28	4.859	1168	1172	1174	rBV4	586	462	0.03%	0.004%
29	4.974	1205	1208	1211	rBV3	328	222	0.02%	0.002%
30	5.074	1221	1239	1264	rBV3	562435	1422253	100.00%	13.246%
31	5.354	1323	1326	1329	rBV2	423	243	0.02%	0.002%
32	5.396	1336	1339	1343	rBV3	344	242	0.02%	0.002%
33	5.421	1343	1347	1350	rBV3	571	514	0.04%	0.005%
34	5.486	1363	1367	1373	rBV4	358	420	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031620\
 Data File : VV014941.D
 Acq On : 16 Mar 2020 13:17
 Operator : SY/MD
 Sample : VV0316WBL01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK61

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
 Title : VOC Analysis

35	5.643	1400	1416	1442	rVV	411051	816674	57.42%	7.606%
36	5.936	1497	1507	1516	rVV8	3134	5728	0.40%	0.053%
37	5.974	1516	1519	1522	rVB2	383	225	0.02%	0.002%
38	6.023	1531	1534	1537	rBV2	455	229	0.02%	0.002%
39	6.096	1538	1557	1576	rBV	308248	626262	44.03%	5.832%
40	6.418	1652	1657	1660	rBV	325	296	0.02%	0.003%
41	6.698	1740	1744	1749	rBV2	241	189	0.01%	0.002%
42	6.730	1749	1754	1756	rBV2	239	184	0.01%	0.002%
43	6.900	1804	1807	1813	rVB2	505	309	0.02%	0.003%
44	6.942	1818	1820	1825	rBV	330	338	0.02%	0.003%
45	7.010	1829	1841	1865	rBV	177725	322586	22.68%	3.004%
46	7.244	1911	1914	1916	rBV3	626	394	0.03%	0.004%
47	7.338	1931	1943	1963	rBV	709326	1229207	86.43%	11.448%
48	7.579	2016	2018	2021	rBV	413	223	0.02%	0.002%
49	7.643	2027	2038	2063	rBV	124440	214696	15.10%	2.000%
50	7.817	2090	2092	2097	rVB3	540	274	0.02%	0.003%
51	7.952	2131	2134	2135	rBV2	468	259	0.02%	0.002%
52	8.122	2175	2187	2234	rBV	312289	691232	48.60%	6.438%
53	8.418	2277	2279	2281	rBV2	319	235	0.02%	0.002%
54	8.492	2298	2302	2304	rBV2	419	325	0.02%	0.003%
55	8.559	2319	2323	2327	rBV2	338	335	0.02%	0.003%
56	8.807	2396	2400	2402	rBV2	275	210	0.01%	0.002%
57	8.874	2408	2421	2450	rVV	631059	1015270	71.38%	9.455%
58	9.035	2466	2471	2480	rVB4	1836	2605	0.18%	0.024%
59	9.080	2482	2485	2486	rBV3	545	329	0.02%	0.003%
60	9.161	2504	2510	2519	rBV5	1814	2649	0.19%	0.025%
61	9.238	2532	2534	2538	rVB	321	256	0.02%	0.002%
62	9.286	2545	2549	2550	rBV	278	191	0.01%	0.002%
63	9.424	2589	2592	2593	rBV	423	180	0.01%	0.002%
64	9.456	2600	2602	2606	rVB2	501	307	0.02%	0.003%
65	9.569	2631	2637	2640	rBV3	1493	1715	0.12%	0.016%
66	9.678	2667	2671	2674	rVB2	263	202	0.01%	0.002%
67	9.698	2674	2677	2681	rBV	401	284	0.02%	0.003%
68	9.759	2690	2696	2701	rBV3	374	490	0.03%	0.005%
69	9.955	2746	2757	2765	rBV8	1716	2868	0.20%	0.027%
70	10.016	2774	2776	2779	rVB	447	176	0.01%	0.002%
71	10.090	2797	2799	2802	rVB	404	179	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031620\
 Data File : VV014941.D
 Acq On : 16 Mar 2020 13:17
 Operator : SY/MD
 Sample : VV0316WBL01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK61

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
 Title : VOC Analysis

72	10.238	2832	2845	2861	rBV	438240	694870	48.86%	6.471%
73	10.405	2893	2897	2899	rBV3	452	376	0.03%	0.004%
74	10.485	2917	2922	2926	rBV2	379	368	0.03%	0.003%
75	10.553	2939	2943	2944	rBV2	919	600	0.04%	0.006%
76	10.640	2968	2970	2977	rVB	316	339	0.02%	0.003%
77	10.672	2977	2980	2984	rBV2	343	237	0.02%	0.002%
78	10.820	3024	3026	3029	rBV2	291	202	0.01%	0.002%
79	10.836	3029	3031	3033	rVB	430	203	0.01%	0.002%
80	10.871	3038	3042	3044	rBV	378	299	0.02%	0.003%
81	10.942	3057	3064	3074	rVB5	1859	2842	0.20%	0.026%
82	11.202	3138	3145	3154	rBV4	2811	4607	0.32%	0.043%
83	11.270	3154	3166	3185	rBV	635061	990726	69.66%	9.227%
84	11.646	3270	3283	3306	rBV	721029	1127865	79.30%	10.504%
85	11.791	3326	3328	3331	rBV2	497	243	0.02%	0.002%
86	11.923	3365	3369	3372	rBV	383	338	0.02%	0.003%
87	12.090	3419	3421	3427	rVB2	527	388	0.03%	0.004%
88	12.135	3431	3435	3440	rVB3	367	337	0.02%	0.003%
89	12.212	3456	3459	3462	rBV2	437	319	0.02%	0.003%
90	12.357	3502	3504	3508	rVB2	408	324	0.02%	0.003%
91	12.395	3514	3516	3519	rBV	338	181	0.01%	0.002%
92	12.588	3572	3576	3577	rBV2	511	331	0.02%	0.003%
93	12.669	3593	3601	3609	rBV4	4102	5989	0.42%	0.056%
94	12.778	3633	3635	3639	rVB2	484	262	0.02%	0.002%
95	13.038	3713	3716	3717	rVB2	501	190	0.01%	0.002%
96	13.054	3718	3721	3724	rBV2	436	357	0.03%	0.003%
97	13.183	3759	3761	3763	rBV	408	196	0.01%	0.002%
98	13.215	3769	3771	3774	rBV	553	329	0.02%	0.003%
99	13.762	3936	3941	3952	rVB5	3804	6672	0.47%	0.062%
100	14.675	4222	4225	4229	rBV	741	679	0.05%	0.006%


Sum of corrected areas: 10737471

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV031620\
Data File : VV014941.D
Acq On : 16 Mar 2020 13:17
Operator : SY/MD
Sample : VV0316WBL01
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK61

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

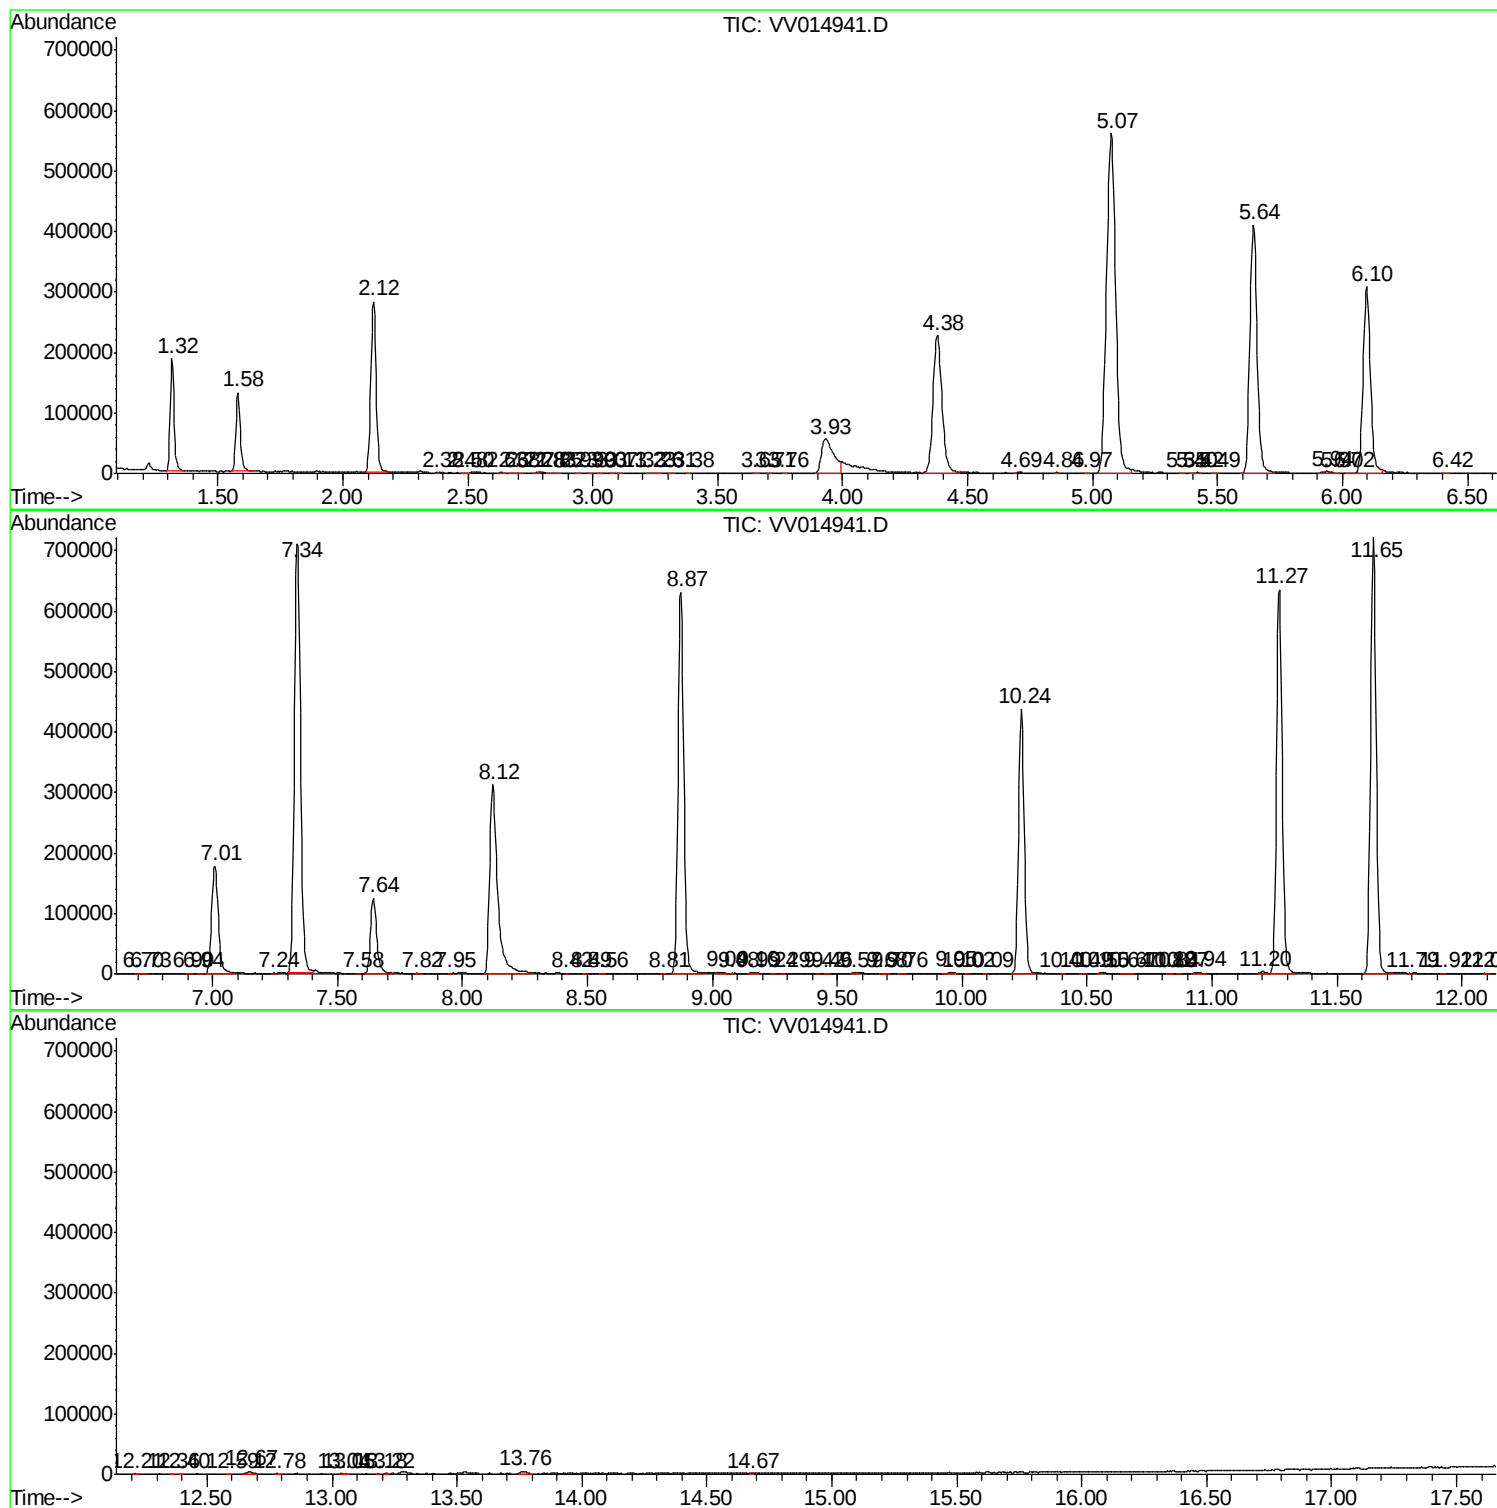

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV031620\
Data File : VV014941.D
Acq On : 16 Mar 2020 13:17
Operator : SY/MD
Sample : VV0316WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK61

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV031620\
Data File : VV014941.D
Acq On : 16 Mar 2020 13:17
Operator : SY/MD
Sample : VV0316WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK61

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc