

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031620\
 Data File : VV014946.D
 Acq On : 16 Mar 2020 15:18
 Operator : SY/MD
 Sample : L1890-11
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DD1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	85	rVB	178050	186026	0.35%	0.135%
2	1.579	144	152	166	rBV	124228	151760	0.29%	0.110%
3	2.119	310	320	335	rVB	272403	387523	0.74%	0.282%
4	2.946	575	577	578	rBV	511	210	0.00%	0.000%
5	3.000	591	594	599	rVB3	766	577	0.00%	0.000%
6	3.039	604	606	608	rBV2	446	238	0.00%	0.000%
7	3.209	655	659	661	rBV2	928	714	0.00%	0.001%
8	3.338	693	699	702	rBV	280	265	0.00%	0.000%
9	3.434	722	729	732	rBV2	282	238	0.00%	0.000%
10	3.675	799	804	809	rBV2	458	382	0.00%	0.000%
11	3.736	816	823	824	rBV	182	192	0.00%	0.000%
12	3.791	830	840	849	rVB5	2935	5953	0.01%	0.004%
13	3.878	863	867	870	rBV2	276	181	0.00%	0.000%
14	3.933	870	884	928	rBV2	59898	380819	0.72%	0.277%
15	4.376	1008	1022	1050	rVB	220398	555604	1.05%	0.404%
16	4.778	1146	1147	1153	rBV3	399	325	0.00%	0.000%
17	4.807	1153	1156	1157	rBV2	316	183	0.00%	0.000%
18	5.074	1221	1239	1243	rBV2	558379	1166688	2.21%	0.848%
19	5.643	1402	1416	1441	rBV	413922	817803	1.55%	0.595%
20	5.826	1472	1473	1478	rVB	471	289	0.00%	0.000%
21	5.933	1497	1506	1510	rBV8	2242	3089	0.01%	0.002%
22	5.974	1516	1519	1520	rBV8	346	195	0.00%	0.000%
23	6.097	1539	1557	1588	rBV	297231	610767	1.16%	0.444%
24	6.289	1616	1617	1620	rVB2	478	189	0.00%	0.000%
25	6.309	1620	1623	1626	rBV	491	307	0.00%	0.000%
26	6.347	1632	1635	1639	rBV	403	314	0.00%	0.000%
27	6.396	1646	1650	1654	rVB2	524	453	0.00%	0.000%
28	6.428	1658	1660	1664	rVB2	595	361	0.00%	0.000%
29	6.685	1737	1740	1744	rVB2	622	443	0.00%	0.000%
30	6.762	1762	1764	1766	rBV	457	190	0.00%	0.000%
31	6.820	1773	1782	1796	rVV3	4880	9496	0.02%	0.007%
32	6.868	1796	1797	1799	rVB3	674	209	0.00%	0.000%
33	6.910	1808	1810	1813	rBV	332	191	0.00%	0.000%
34	6.965	1823	1827	1828	rBV	336	201	0.00%	0.000%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031620\
 Data File : VV014946.D
 Acq On : 16 Mar 2020 15:18
 Operator : SY/MD
 Sample : L1890-11
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DD1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
 Title : VOC Analysis

35	7.010	1828	1841	1865	rBV	174863	317162	0.60%	0.231%
36	7.161	1886	1888	1892	rVV2	467	274	0.00%	0.000%
37	7.232	1907	1910	1912	rBV	440	190	0.00%	0.000%
38	7.264	1917	1920	1921	rBV2	389	212	0.00%	0.000%
39	7.338	1929	1943	1962	rBV	711744	1210165	2.30%	0.880%
40	7.595	2019	2023	2026	rBV2	253	222	0.00%	0.000%
41	7.643	2026	2038	2057	rBV	123697	214282	0.41%	0.156%
42	7.791	2082	2084	2089	rVB2	500	288	0.00%	0.000%
43	7.820	2089	2093	2095	rBV3	433	312	0.00%	0.000%
44	7.865	2105	2107	2111	rVB3	422	289	0.00%	0.000%
45	7.887	2111	2114	2116	rBV2	447	223	0.00%	0.000%
46	7.968	2125	2139	2144	rBV3	3193	5373	0.01%	0.004%
47	8.119	2173	2186	2220	rBV	306041	660939	1.25%	0.481%
48	8.373	2263	2265	2268	rBV2	405	223	0.00%	0.000%
49	8.440	2284	2286	2289	rBV3	392	302	0.00%	0.000%
50	8.482	2295	2299	2302	rBB3	398	295	0.00%	0.000%
51	8.595	2332	2334	2338	rVB2	494	379	0.00%	0.000%
52	8.630	2338	2345	2351	rBV3	706	725	0.00%	0.001%
53	8.662	2353	2355	2359	rBV	317	241	0.00%	0.000%
54	8.820	2403	2404	2408	rVB	407	189	0.00%	0.000%
55	8.910	2408	2432	2476	rBV	30245781	52701555	100.00%	38.322%
56	9.559	2630	2634	2637	rBV4	1710	1718	0.00%	0.001%
57	9.666	2665	2667	2670	rBV3	308	197	0.00%	0.000%
58	9.723	2682	2685	2688	rBV3	497	356	0.00%	0.000%
59	9.813	2709	2713	2716	rBV2	582	469	0.00%	0.000%
60	9.936	2749	2751	2753	rBV3	461	202	0.00%	0.000%
61	9.952	2753	2756	2759	rBV2	717	487	0.00%	0.000%
62	10.122	2806	2809	2814	rVV2	350	288	0.00%	0.000%
63	10.190	2821	2830	2834	rBV	7783	11302	0.02%	0.008%
64	10.238	2834	2845	2864	rVB	435874	687980	1.31%	0.500%
65	10.399	2885	2895	2904	rVV2	4531	8088	0.02%	0.006%
66	10.450	2906	2911	2919	rVB5	2964	4047	0.01%	0.003%
67	10.508	2925	2929	2932	rBV2	708	483	0.00%	0.000%
68	10.566	2939	2947	2953	rVV6	2672	3680	0.01%	0.003%
69	10.627	2963	2966	2972	rVB2	419	366	0.00%	0.000%
70	10.723	2994	2996	3001	rVB2	403	263	0.00%	0.000%
71	10.752	3001	3005	3009	rBV2	391	441	0.00%	0.000%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031620\
 Data File : VV014946.D
 Acq On : 16 Mar 2020 15:18
 Operator : SY/MD
 Sample : L1890-11
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DD1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
 Title : VOC Analysis

72	10.836	3028	3031	3034	rVV2	341	244	0.00%	0.000%
73	10.874	3037	3043	3049	rVB4	1095	1051	0.00%	0.001%
74	10.942	3056	3064	3066	rBV3	1105	1437	0.00%	0.001%
75	10.974	3073	3074	3077	rVB	537	215	0.00%	0.000%
76	11.061	3097	3101	3104	rBV2	330	224	0.00%	0.000%
77	11.109	3112	3116	3119	rBV3	364	298	0.00%	0.000%
78	11.199	3131	3144	3156	rBV	2561754	3931600	7.46%	2.859%
79	11.296	3157	3174	3200	rVB	15601018	24354828	46.21%	17.710%
80	11.665	3271	3289	3310	rBV	14559882	23267802	44.15%	16.919%
81	11.997	3389	3392	3397	rVB4	727	614	0.00%	0.000%
82	12.135	3428	3435	3445	rVB4	6792	10096	0.02%	0.007%
83	12.254	3467	3472	3473	rBV2	751	519	0.00%	0.000%
84	12.357	3496	3504	3512	rBV5	4686	6941	0.01%	0.005%
85	12.415	3512	3522	3539	rVB	169633	258064	0.49%	0.188%
86	12.595	3567	3578	3591	rBV3	57346	140855	0.27%	0.102%
87	12.665	3593	3600	3612	rVB2	35314	53113	0.10%	0.039%
88	12.710	3612	3614	3616	rBV	601	270	0.00%	0.000%
89	12.768	3621	3632	3647	rBV2	92598	145331	0.28%	0.106%
90	12.823	3647	3649	3653	rBV3	453	195	0.00%	0.000%
91	12.910	3670	3676	3678	rBV3	578	586	0.00%	0.000%
92	13.016	3700	3709	3719	rVB3	12213	19935	0.04%	0.014%
93	13.141	3745	3748	3751	rBV2	733	511	0.00%	0.000%
94	13.199	3763	3766	3769	rVB2	784	435	0.00%	0.000%
95	13.218	3770	3772	3777	rBV	357	223	0.00%	0.000%
96	13.283	3777	3792	3817	rBV	12898019	19488735	36.98%	14.171%
97	13.524	3861	3867	3876	rVB2	4135	6899	0.01%	0.005%
98	13.765	3927	3942	3961	rBV	3210940	4933858	9.36%	3.588%
99	14.839	4261	4276	4291	rVB	110091	223431	0.42%	0.162%
100	15.418	4445	4456	4469	rBV	357400	557607	1.06%	0.405%


Sum of corrected areas: 137522499

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031620\
Data File : VV014946.D
Acq On : 16 Mar 2020 15:18
Operator : SY/MD
Sample : L1890-11
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DD1

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

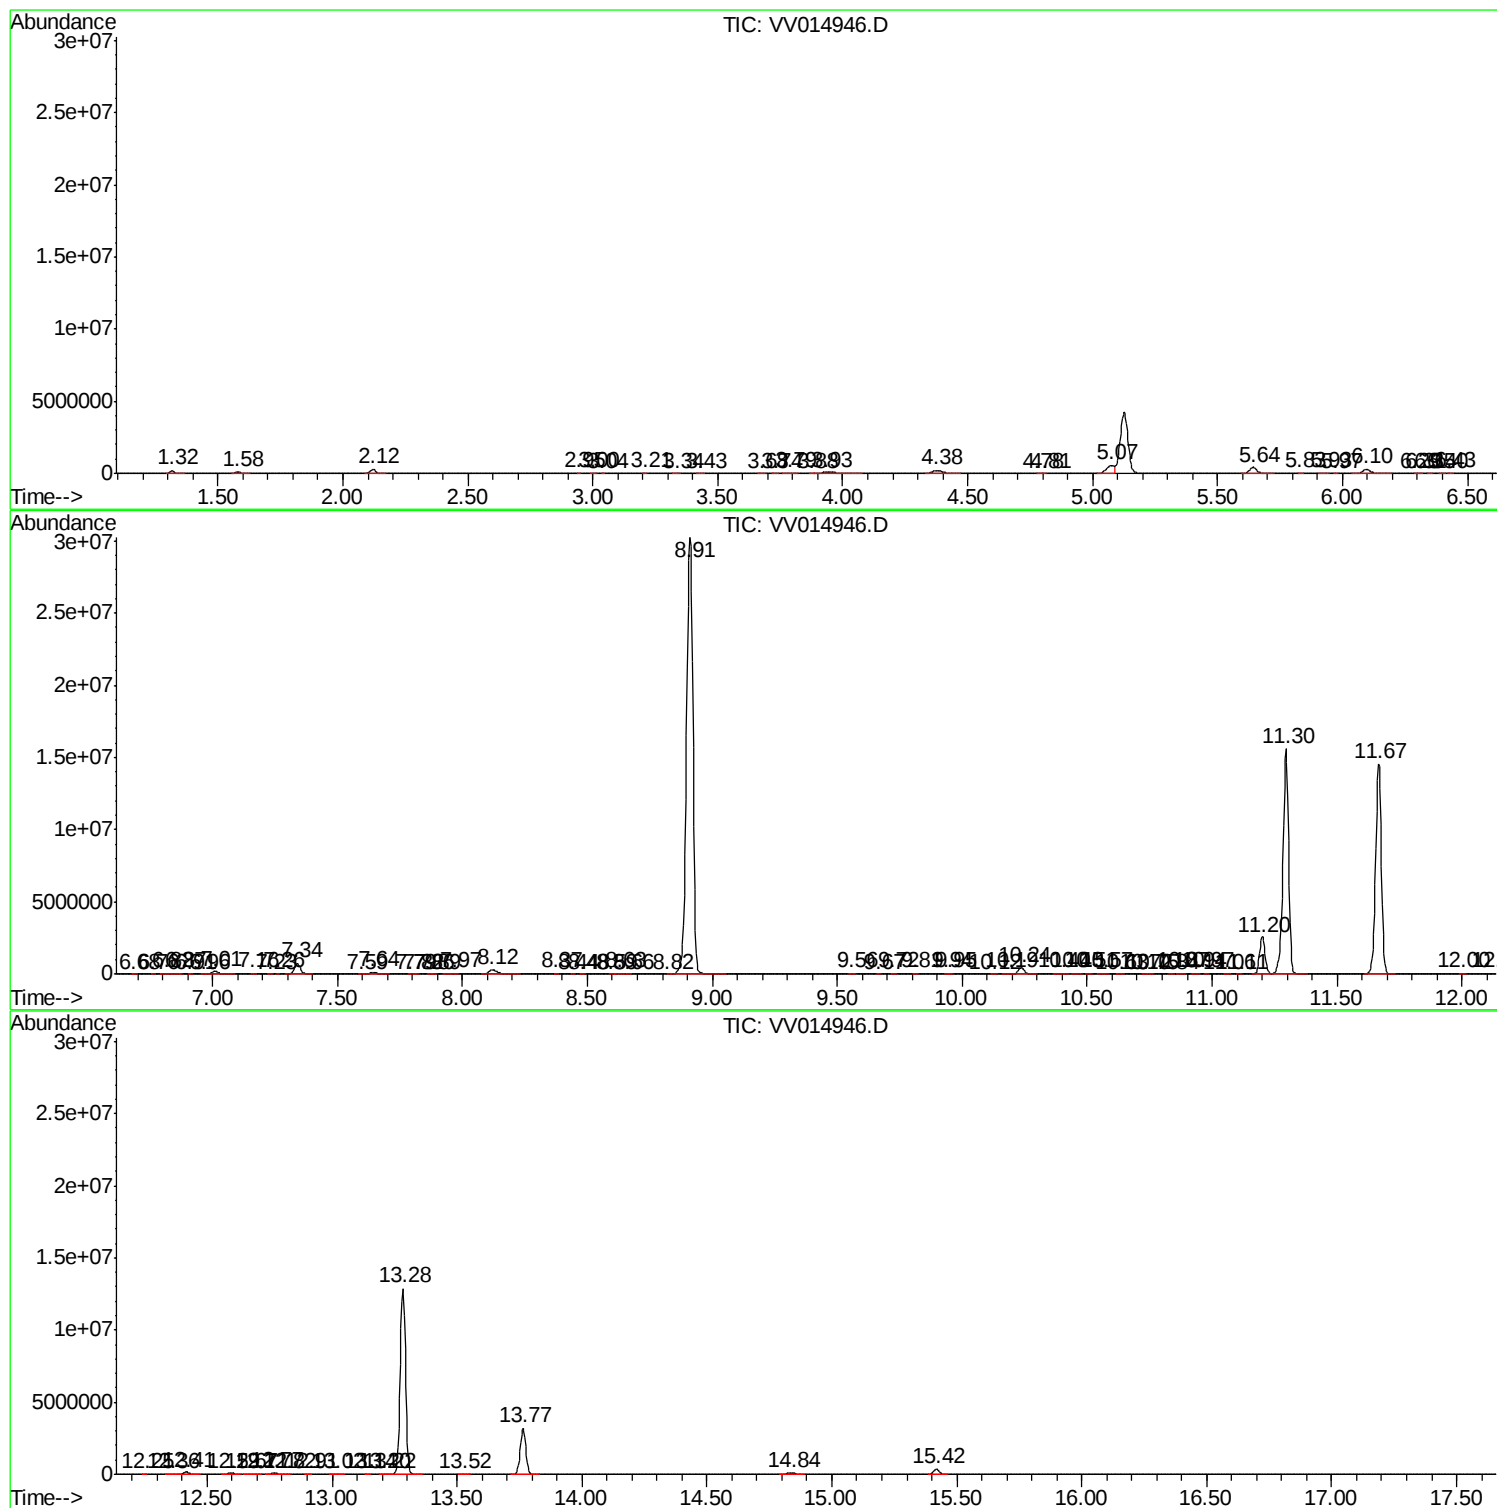

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV031620\
Data File : VV014946.D
Acq On : 16 Mar 2020 15:18
Operator : SY/MD
Sample : L1890-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DD1

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV031620\
Data File : VV014946.D
Acq On : 16 Mar 2020 15:18
Operator : SY/MD
Sample : L1890-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DD1

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc