

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031620\
 Data File : VV014947.D
 Acq On : 16 Mar 2020 15:42
 Operator : SY/MD
 Sample : L1890-12
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DD2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	85	rVB	169329	177829	0.34%	0.130%
2	1.579	145	152	171	rVB	124097	149856	0.29%	0.109%
3	2.123	311	321	337	rVB	256191	368431	0.70%	0.269%
4	2.968	582	584	589	rVB3	600	447	0.00%	0.000%
5	2.997	589	593	594	rBV3	336	207	0.00%	0.000%
6	3.058	610	612	615	rVB2	416	216	0.00%	0.000%
7	3.077	615	618	619	rBV2	668	296	0.00%	0.000%
8	3.126	630	633	638	rVB	410	295	0.00%	0.000%
9	3.148	638	640	645	rBV	443	301	0.00%	0.000%
10	3.196	653	655	657	rBV	302	197	0.00%	0.000%
11	3.209	657	659	661	rVV2	363	129	0.00%	0.000%
12	3.312	688	691	694	rVV2	444	247	0.00%	0.000%
13	3.396	714	717	721	rVB4	437	344	0.00%	0.000%
14	3.476	738	742	745	rVB2	388	280	0.00%	0.000%
15	3.589	774	777	779	rVB2	345	165	0.00%	0.000%
16	3.608	779	783	786	rBV	316	254	0.00%	0.000%
17	3.666	796	801	806	rVB3	462	392	0.00%	0.000%
18	3.730	817	821	826	rBV2	410	451	0.00%	0.000%
19	3.791	828	840	845	rBV4	3392	5886	0.01%	0.004%
20	3.852	855	859	860	rBV2	254	171	0.00%	0.000%
21	3.933	868	884	886	rBV	55780	95123	0.18%	0.070%
22	4.380	1008	1023	1050	rVB	208407	525852	1.00%	0.384%
23	4.772	1143	1145	1153	rVB4	516	456	0.00%	0.000%
24	4.930	1193	1194	1197	rBV	303	155	0.00%	0.000%
25	5.074	1220	1239	1244	rBV2	531207	1180113	2.25%	0.862%
26	5.643	1402	1416	1439	rBV	409830	814451	1.55%	0.595%
27	5.852	1478	1481	1486	rVB4	282	243	0.00%	0.000%
28	5.904	1493	1497	1499	rBV2	393	285	0.00%	0.000%
29	5.942	1499	1509	1512	rBV8	1578	2799	0.01%	0.002%
30	6.032	1535	1537	1542	rBV3	417	399	0.00%	0.000%
31	6.097	1542	1557	1579	rBV	283924	579607	1.11%	0.424%
32	6.222	1593	1596	1599	rBV3	1109	892	0.00%	0.001%
33	6.257	1604	1607	1613	rBV4	1015	805	0.00%	0.001%
34	6.383	1643	1646	1650	rBV2	475	282	0.00%	0.000%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031620\
 Data File : VV014947.D
 Acq On : 16 Mar 2020 15:42
 Operator : SY/MD
 Sample : L1890-12
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DD2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
 Title : VOC Analysis

35	6.441	1662	1664	1668	rBV	220	156	0.00%	0.000%
36	6.479	1672	1676	1679	rBV2	453	272	0.00%	0.000%
37	6.573	1702	1705	1709	rBV	265	176	0.00%	0.000%
38	6.627	1719	1722	1727	rBV3	674	598	0.00%	0.000%
39	6.650	1727	1729	1731	rVV2	231	132	0.00%	0.000%
40	6.746	1758	1759	1761	rBV	490	150	0.00%	0.000%
41	6.785	1767	1771	1773	rBV2	421	337	0.00%	0.000%
42	6.820	1773	1782	1795	rVB4	4449	9076	0.02%	0.007%
43	6.920	1804	1813	1814	rBV2	553	489	0.00%	0.000%
44	7.010	1829	1841	1865	rVV	164911	302473	0.58%	0.221%
45	7.206	1898	1902	1905	rBV3	406	360	0.00%	0.000%
46	7.338	1929	1943	1961	rBV	679034	1174275	2.24%	0.858%
47	7.550	2003	2009	2014	rBV3	512	708	0.00%	0.001%
48	7.643	2027	2038	2066	rBV	121027	207158	0.40%	0.151%
49	7.836	2095	2098	2100	rBV	339	242	0.00%	0.000%
50	7.865	2104	2107	2108	rBV2	415	253	0.00%	0.000%
51	7.958	2128	2136	2143	rBV4	2463	4251	0.01%	0.003%
52	8.119	2174	2186	2212	rBV	282612	637361	1.22%	0.466%
53	8.441	2283	2286	2287	rBV	400	216	0.00%	0.000%
54	8.646	2346	2350	2352	rBV2	155	142	0.00%	0.000%
55	8.781	2390	2392	2399	rVB2	463	301	0.00%	0.000%
56	8.817	2399	2403	2404	rBV3	373	218	0.00%	0.000%
57	8.910	2408	2432	2474	rBV	30327611	52407786	100.00%	38.293%
58	9.650	2659	2662	2664	rBV	613	377	0.00%	0.000%
59	9.720	2681	2684	2686	rBV2	459	326	0.00%	0.000%
60	9.788	2703	2705	2708	rBV	390	202	0.00%	0.000%
61	9.820	2713	2715	2718	rVB2	425	238	0.00%	0.000%
62	9.878	2729	2733	2737	rBV2	330	365	0.00%	0.000%
63	9.920	2744	2746	2747	rBV	393	183	0.00%	0.000%
64	9.994	2767	2769	2771	rBV	249	129	0.00%	0.000%
65	10.074	2791	2794	2796	rBV2	455	256	0.00%	0.000%
66	10.109	2803	2805	2808	rBV2	502	323	0.00%	0.000%
67	10.129	2809	2811	2813	rBV2	321	157	0.00%	0.000%
68	10.187	2821	2829	2834	rBV3	7172	11009	0.02%	0.008%
69	10.238	2835	2845	2861	rVB	423989	669523	1.28%	0.489%
70	10.347	2876	2879	2881	rBV	481	275	0.00%	0.000%
71	10.399	2886	2895	2904	rBV2	4370	7064	0.01%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031620\
 Data File : VV014947.D
 Acq On : 16 Mar 2020 15:42
 Operator : SY/MD
 Sample : L1890-12
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DD2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
 Title : VOC Analysis

72	10.495	2922	2925	2928	rBV2	363	244	0.00%	0.000%
73	10.566	2940	2947	2952	rBV4	1756	2007	0.00%	0.001%
74	10.678	2978	2982	2984	rBV	436	299	0.00%	0.000%
75	10.698	2986	2988	2991	rVB2	398	218	0.00%	0.000%
76	10.768	3008	3010	3012	rBV	287	147	0.00%	0.000%
77	10.842	3031	3033	3037	rVB	365	192	0.00%	0.000%
78	10.865	3037	3040	3044	rBV3	593	461	0.00%	0.000%
79	10.936	3058	3062	3064	rBV3	998	828	0.00%	0.001%
80	11.003	3077	3083	3086	rBV2	368	402	0.00%	0.000%
81	11.074	3100	3105	3106	rBV2	596	474	0.00%	0.000%
82	11.203	3131	3145	3156	rBV	2587130	3953898	7.54%	2.889%
83	11.296	3157	3174	3198	rVB	15534421	24376430	46.51%	17.811%
84	11.669	3271	3290	3310	rBV	14267893	23250345	44.36%	16.988%
85	12.132	3425	3434	3442	rBV4	7433	12190	0.02%	0.009%
86	12.222	3461	3462	3464	rBV4	442	143	0.00%	0.000%
87	12.334	3494	3497	3498	rBV2	1074	528	0.00%	0.000%
88	12.415	3512	3522	3536	rVB	164649	254483	0.49%	0.186%
89	12.521	3553	3555	3560	rBV3	611	413	0.00%	0.000%
90	12.598	3566	3579	3591	rBV6	58059	144106	0.27%	0.105%
91	12.666	3593	3600	3610	rVB2	33739	49935	0.10%	0.036%
92	12.768	3619	3632	3645	rBV2	94614	146606	0.28%	0.107%
93	13.016	3702	3709	3718	rVB3	12369	19248	0.04%	0.014%
94	13.125	3740	3743	3746	rBV2	512	418	0.00%	0.000%
95	13.190	3761	3763	3768	rBV3	601	498	0.00%	0.000%
96	13.283	3778	3792	3817	rBV	12856674	19490323	37.19%	14.241%
97	13.765	3928	3942	3965	rBV	3273127	4996695	9.53%	3.651%
98	14.527	4174	4179	4188	rBV8	2124	3118	0.01%	0.002%
99	14.842	4261	4277	4288	rVB	111535	225911	0.43%	0.165%
100	15.418	4445	4456	4472	rBV	374423	583437	1.11%	0.426%


Sum of corrected areas: 136859410

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV031620\
Data File : VV014947.D
Acq On : 16 Mar 2020 15:42
Operator : SY/MD
Sample : L1890-12
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DD2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

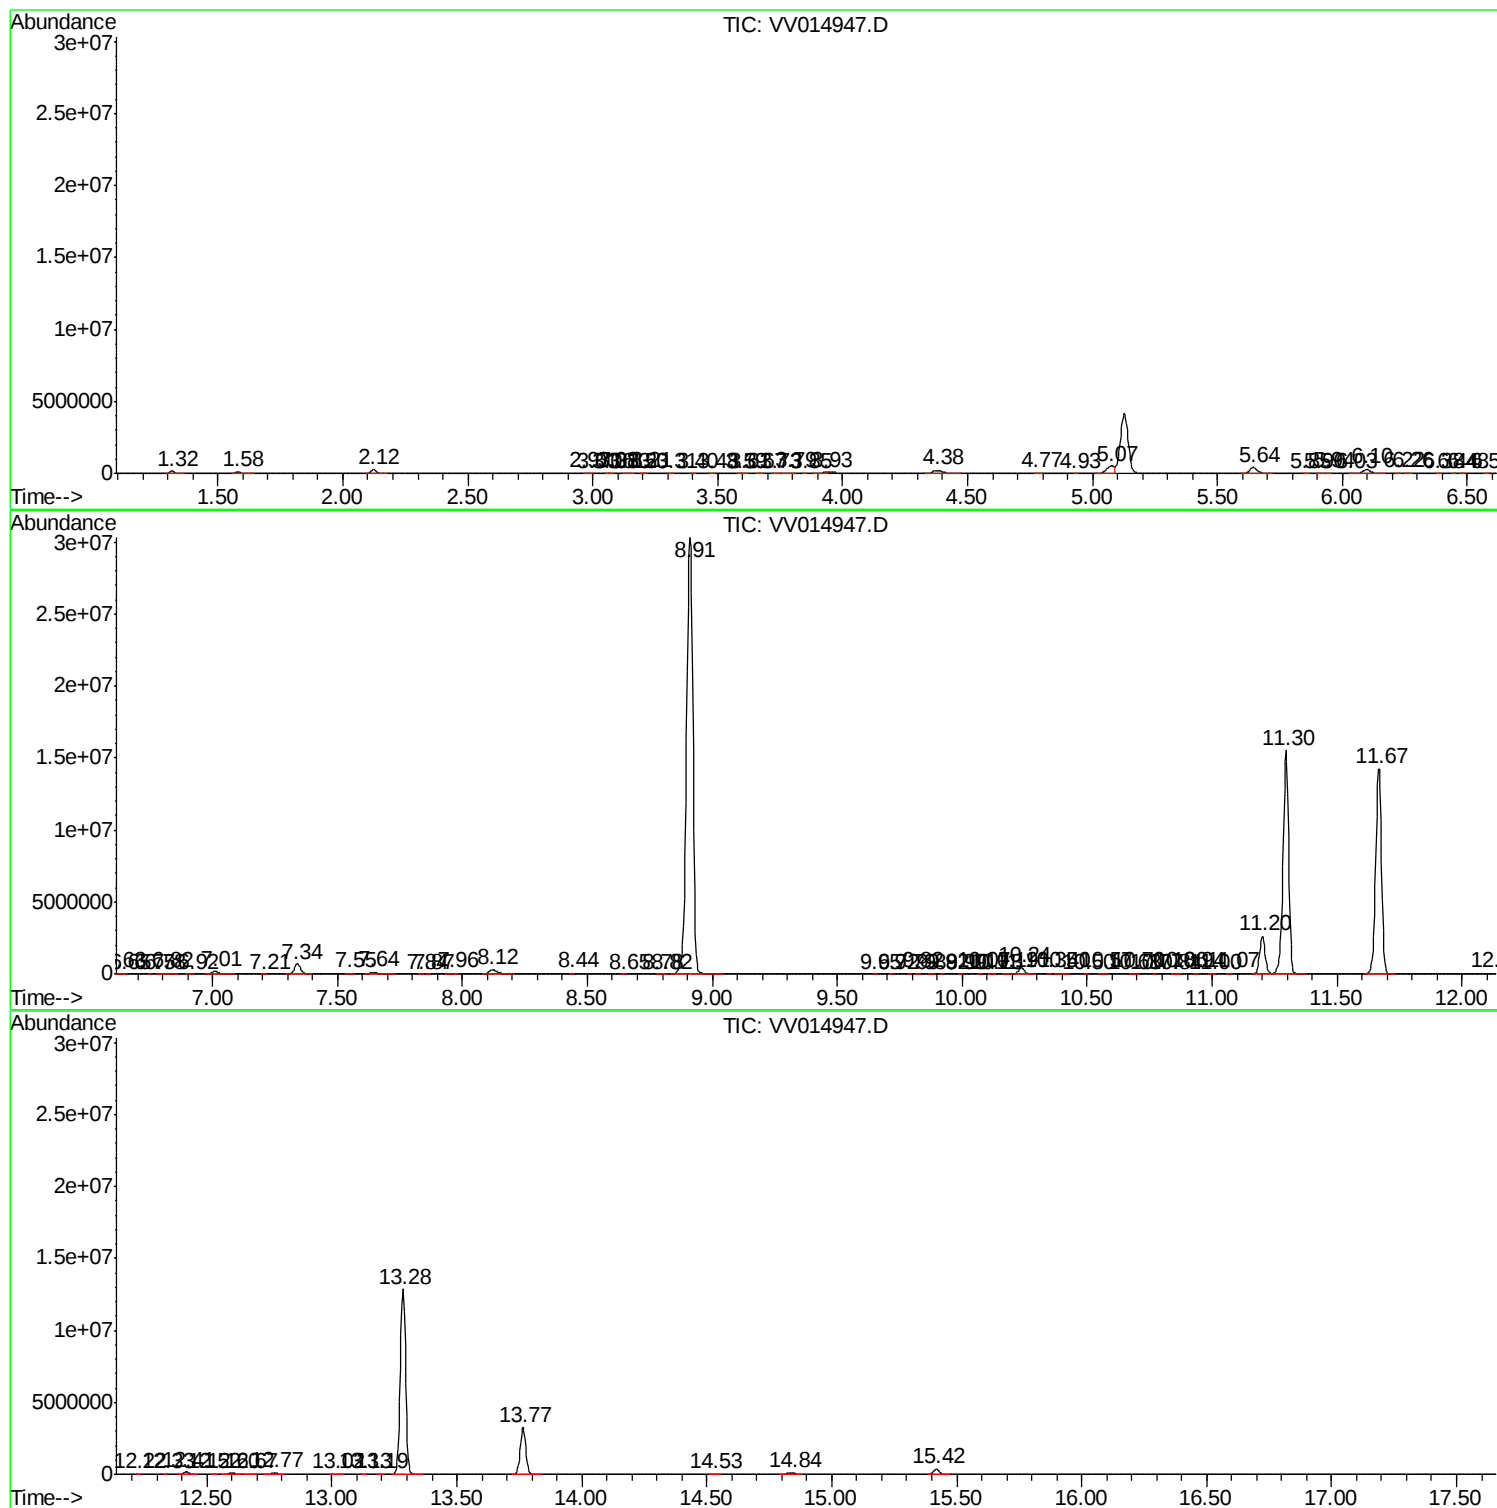

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV031620\
Data File : VV014947.D
Acq On : 16 Mar 2020 15:42
Operator : SY/MD
Sample : L1890-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DD2

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV031620\
Data File : VV014947.D
Acq On : 16 Mar 2020 15:42
Operator : SY/MD
Sample : L1890-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DD2

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc