

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031620\
 Data File : VV014950.D
 Acq On : 16 Mar 2020 16:55
 Operator : SY/MD
 Sample : L1890-15
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DG8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	84	rVB	165439	174895	13.20%	1.715%
2	1.579	145	152	169	rVB	123180	146386	11.05%	1.436%
3	2.119	311	320	339	rVB	254272	368314	27.80%	3.612%
4	3.196	653	655	656	rBV	387	165	0.01%	0.002%
5	3.309	688	690	696	rVB2	512	385	0.03%	0.004%
6	3.335	696	698	700	rBV2	185	61	0.00%	0.001%
7	3.396	715	717	719	rBV2	322	138	0.01%	0.001%
8	3.647	790	795	798	rBV3	328	248	0.02%	0.002%
9	3.733	819	822	824	rBV	143	92	0.01%	0.001%
10	3.801	840	843	845	rBV2	185	139	0.01%	0.001%
11	3.814	845	847	849	rBV	185	94	0.01%	0.001%
12	3.936	873	885	911	rBV2	49325	194381	14.67%	1.906%
13	4.376	1006	1022	1056	rBV	212173	526906	39.77%	5.167%
14	4.634	1097	1102	1104	rBV3	444	294	0.02%	0.003%
15	4.733	1130	1133	1134	rBV2	320	150	0.01%	0.001%
16	4.759	1138	1141	1143	rBV	457	221	0.02%	0.002%
17	4.788	1148	1150	1152	rBV	309	164	0.01%	0.002%
18	4.852	1166	1170	1171	rBV2	199	124	0.01%	0.001%
19	4.962	1202	1204	1208	rVB	359	195	0.01%	0.002%
20	4.987	1210	1212	1216	rVB2	469	263	0.02%	0.003%
21	5.074	1220	1239	1262	rBV2	529796	1324771	100.00%	12.991%
22	5.341	1320	1322	1327	rBV2	457	328	0.02%	0.003%
23	5.389	1334	1337	1339	rBV	513	308	0.02%	0.003%
24	5.438	1351	1352	1353	rVB	380	73	0.01%	0.001%
25	5.489	1366	1368	1370	rBV	224	138	0.01%	0.001%
26	5.643	1401	1416	1436	rBV	395222	788958	59.55%	7.737%
27	5.923	1499	1503	1506	rBV3	1249	1271	0.10%	0.012%
28	5.987	1521	1523	1525	rBV2	358	181	0.01%	0.002%
29	6.016	1530	1532	1533	rVB	265	85	0.01%	0.001%
30	6.026	1533	1535	1538	rBV2	273	206	0.02%	0.002%
31	6.097	1542	1557	1576	rBV	289496	580892	43.85%	5.697%
32	6.290	1616	1617	1619	rBV	257	120	0.01%	0.001%
33	6.331	1628	1630	1631	rBV	261	114	0.01%	0.001%
34	6.447	1663	1666	1670	rBV2	458	338	0.03%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031620\
 Data File : VV014950.D
 Acq On : 16 Mar 2020 16:55
 Operator : SY/MD
 Sample : L1890-15
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DG8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
 Title : VOC Analysis

35	6.508	1682	1685	1687	rBV	413	211	0.02%	0.002%
36	6.576	1701	1706	1707	rBV2	457	419	0.03%	0.004%
37	6.605	1711	1715	1718	rVV2	477	279	0.02%	0.003%
38	6.675	1734	1737	1739	rVB2	361	207	0.02%	0.002%
39	6.849	1787	1791	1794	rBV2	360	355	0.03%	0.003%
40	7.010	1829	1841	1862	rBV	164691	296945	22.41%	2.912%
41	7.203	1899	1901	1903	rBV2	401	185	0.01%	0.002%
42	7.254	1915	1917	1919	rBV2	269	117	0.01%	0.001%
43	7.338	1930	1943	1967	rBV	665375	1152583	87.00%	11.303%
44	7.643	2027	2038	2057	rBV	115731	198551	14.99%	1.947%
45	7.807	2082	2089	2092	rBV2	700	682	0.05%	0.007%
46	7.836	2093	2098	2099	rBV2	372	267	0.02%	0.003%
47	7.878	2109	2111	2112	rBV	384	109	0.01%	0.001%
48	7.917	2120	2123	2125	rVB2	498	260	0.02%	0.003%
49	7.968	2131	2139	2146	rBV4	2289	4085	0.31%	0.040%
50	8.068	2168	2170	2171	rBV	353	124	0.01%	0.001%
51	8.122	2175	2187	2226	rVV	286819	657255	49.61%	6.445%
52	8.399	2272	2273	2275	rBV	412	154	0.01%	0.002%
53	8.428	2279	2282	2287	rVB4	990	660	0.05%	0.006%
54	8.447	2287	2288	2289	rBV4	236	77	0.01%	0.001%
55	8.695	2364	2365	2367	rVB	337	121	0.01%	0.001%
56	8.711	2367	2370	2371	rBV2	298	166	0.01%	0.002%
57	8.810	2400	2401	2404	rBV	271	152	0.01%	0.001%
58	8.875	2408	2421	2449	rVV	607930	1014067	76.55%	9.944%
59	9.087	2485	2487	2490	rVB	636	284	0.02%	0.003%
60	9.135	2497	2502	2506	rBV3	477	538	0.04%	0.005%
61	9.154	2506	2508	2510	rBV3	422	219	0.02%	0.002%
62	9.280	2545	2547	2550	rBV	363	159	0.01%	0.002%
63	9.351	2568	2569	2570	rBV	137	41	0.00%	0.000%
64	9.418	2588	2590	2592	rBV2	220	103	0.01%	0.001%
65	9.566	2633	2636	2642	rBV2	723	638	0.05%	0.006%
66	9.846	2721	2723	2724	rVB	239	51	0.00%	0.001%
67	9.871	2730	2731	2733	rBV	230	88	0.01%	0.001%
68	9.949	2754	2755	2757	rVB	408	80	0.01%	0.001%
69	9.965	2758	2760	2763	rVB	467	160	0.01%	0.002%
70	10.019	2774	2777	2781	rBV2	488	439	0.03%	0.004%
71	10.119	2806	2808	2810	rBB	236	75	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031620\
 Data File : VV014950.D
 Acq On : 16 Mar 2020 16:55
 Operator : SY/MD
 Sample : L1890-15
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DG8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
 Title : VOC Analysis

72	10.132	2810	2812	2814	rVB2	447	177	0.01%	0.002%
73	10.145	2814	2816	2819	rBV	429	256	0.02%	0.003%
74	10.238	2833	2845	2866	rVB	421581	667079	50.35%	6.542%
75	10.405	2890	2897	2905	rVB4	2977	4862	0.37%	0.048%
76	10.476	2913	2919	2923	rBV	475	451	0.03%	0.004%
77	10.502	2925	2927	2930	rVB2	442	233	0.02%	0.002%
78	10.553	2941	2943	2945	rBV2	324	123	0.01%	0.001%
79	10.595	2954	2956	2958	rBV	354	136	0.01%	0.001%
80	10.817	3024	3025	3029	rVB2	374	177	0.01%	0.002%
81	10.871	3040	3042	3045	rBV2	564	383	0.03%	0.004%
82	10.913	3052	3055	3057	rBV	379	249	0.02%	0.002%
83	10.977	3072	3075	3076	rBV	627	323	0.02%	0.003%
84	11.084	3106	3108	3110	rBV2	388	187	0.01%	0.002%
85	11.122	3117	3120	3123	rBV2	562	392	0.03%	0.004%
86	11.199	3139	3144	3153	rBV5	2488	3326	0.25%	0.033%
87	11.270	3154	3166	3187	rVV	609828	967379	73.02%	9.487%
88	11.505	3236	3239	3240	rBV	282	141	0.01%	0.001%
89	11.543	3249	3251	3253	rBV	587	279	0.02%	0.003%
90	11.646	3269	3283	3301	rBV	678225	1077104	81.30%	10.563%
91	12.100	3421	3424	3427	rBV2	347	231	0.02%	0.002%
92	12.257	3471	3473	3475	rBV	554	272	0.02%	0.003%
93	12.315	3487	3491	3492	rBV2	346	209	0.02%	0.002%
94	13.071	3723	3726	3727	rBV	366	193	0.01%	0.002%
95	13.283	3784	3792	3808	rVB2	19798	30864	2.33%	0.303%


Sum of corrected areas: 10197330

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV031620\
Data File : VV014950.D
Acq On : 16 Mar 2020 16:55
Operator : SY/MD
Sample : L1890-15
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DG8

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

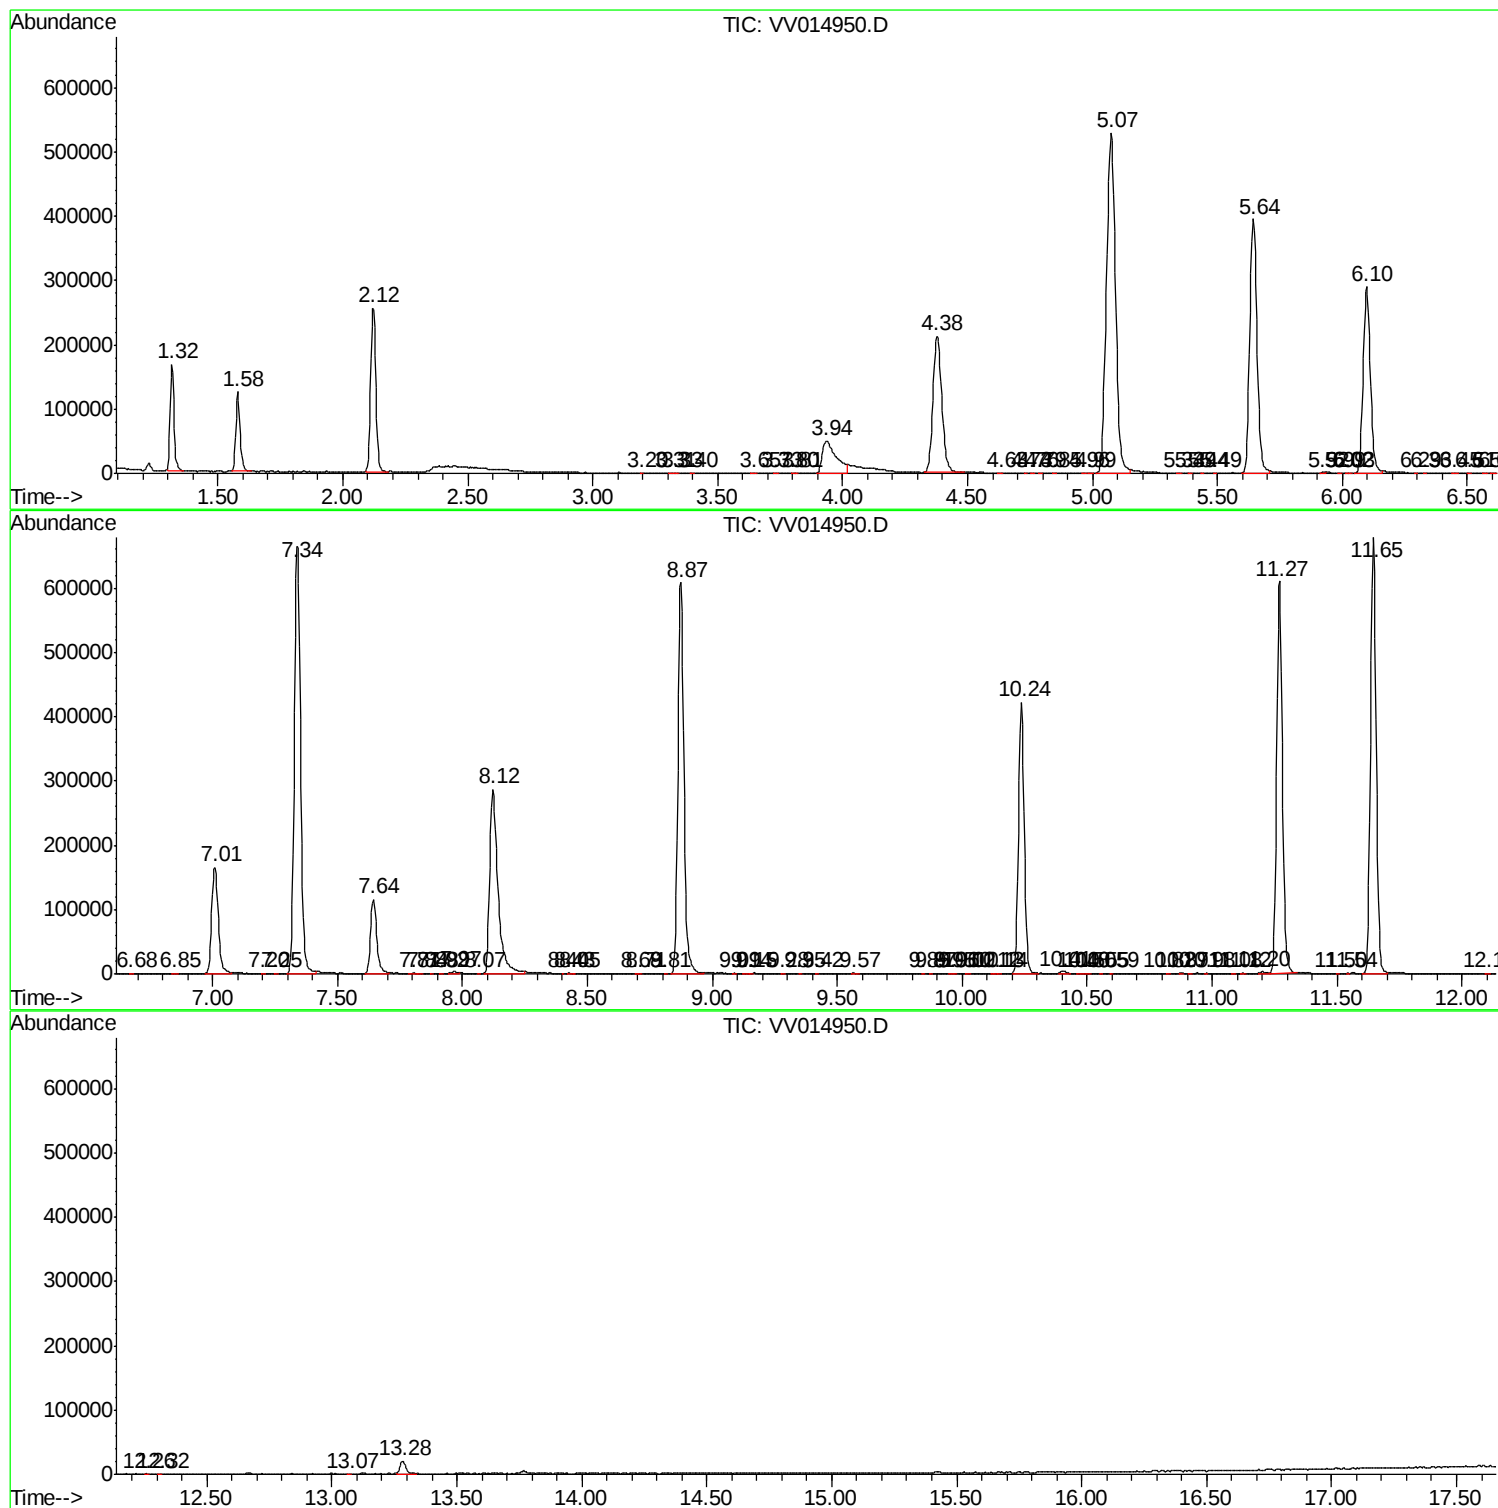

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV031620\
Data File : VV014950.D
Acq On : 16 Mar 2020 16:55
Operator : SY/MD
Sample : L1890-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DG8

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV031620\
Data File : VV014950.D
Acq On : 16 Mar 2020 16:55
Operator : SY/MD
Sample : L1890-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DG8

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc