

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031620\
 Data File : VV014958.D
 Acq On : 16 Mar 2020 20:08
 Operator : SY/MD
 Sample : L1940-12
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DA6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	85	rVB	159690	166386	9.85%	1.420%
2	1.579	144	152	167	rBV	116743	145646	8.63%	1.243%
3	2.123	311	321	337	rBV	243782	348233	20.62%	2.972%
4	2.823	537	539	540	rVB	458	152	0.01%	0.001%
5	2.901	557	563	564	rBV2	404	376	0.02%	0.003%
6	2.933	570	573	577	rBV2	538	386	0.02%	0.003%
7	2.978	584	587	588	rBV2	408	196	0.01%	0.002%
8	3.132	633	635	636	rBV	325	138	0.01%	0.001%
9	3.206	653	658	660	rBV2	352	326	0.02%	0.003%
10	3.277	677	680	682	rVB2	277	166	0.01%	0.001%
11	3.325	693	695	698	rBV	291	212	0.01%	0.002%
12	3.405	718	720	726	rVB2	225	180	0.01%	0.002%
13	3.463	733	738	740	rBV2	317	290	0.02%	0.002%
14	3.528	756	758	761	rVB2	560	265	0.02%	0.002%
15	3.547	761	764	768	rBV2	359	363	0.02%	0.003%
16	3.698	808	811	817	rVB2	413	320	0.02%	0.003%
17	3.791	835	840	842	rBV2	331	269	0.02%	0.002%
18	3.885	867	869	872	rBV2	300	184	0.01%	0.002%
19	3.933	872	884	909	rBV2	48126	185183	10.97%	1.581%
20	4.376	1008	1022	1050	rVB2	202418	499493	29.58%	4.264%
21	4.563	1078	1080	1083	rBV3	690	468	0.03%	0.004%
22	4.820	1155	1160	1162	rVB2	399	244	0.01%	0.002%
23	4.843	1162	1167	1168	rBV2	442	344	0.02%	0.003%
24	4.971	1203	1207	1209	rBV2	295	168	0.01%	0.001%
25	4.984	1209	1211	1214	rVB2	443	203	0.01%	0.002%
26	5.003	1214	1217	1220	rBV3	544	375	0.02%	0.003%
27	5.074	1220	1239	1278	rBV2	498746	1323102	78.36%	11.294%
28	5.396	1337	1339	1341	rBV	428	144	0.01%	0.001%
29	5.412	1341	1344	1346	rBV2	405	229	0.01%	0.002%
30	5.460	1356	1359	1362	rVB2	400	233	0.01%	0.002%
31	5.479	1362	1365	1366	rBV	283	164	0.01%	0.001%
32	5.515	1372	1376	1379	rBV3	418	308	0.02%	0.003%
33	5.550	1382	1387	1390	rVB2	446	385	0.02%	0.003%
34	5.566	1390	1392	1395	rBV2	482	352	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031620\
 Data File : VV014958.D
 Acq On : 16 Mar 2020 20:08
 Operator : SY/MD
 Sample : L1940-12
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DA6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
 Title : VOC Analysis

35	5.643	1402	1416	1440	rBV	393964	779817	46.19%	6.656%
36	5.872	1486	1487	1491	rVB2	418	181	0.01%	0.002%
37	5.910	1497	1499	1500	rBV2	614	284	0.02%	0.002%
38	5.991	1522	1524	1527	rVB2	334	142	0.01%	0.001%
39	6.097	1540	1557	1584	rBV	276905	566263	33.54%	4.833%
40	6.302	1619	1621	1623	rBV2	366	221	0.01%	0.002%
41	6.344	1632	1634	1637	rVB	339	160	0.01%	0.001%
42	6.364	1637	1640	1642	rBV3	403	227	0.01%	0.002%
43	6.415	1651	1656	1660	rBV2	270	269	0.02%	0.002%
44	6.466	1669	1672	1675	rBV	302	201	0.01%	0.002%
45	6.611	1714	1717	1719	rBV	343	194	0.01%	0.002%
46	6.653	1728	1730	1735	rBV	277	210	0.01%	0.002%
47	6.862	1792	1795	1797	rVB2	293	188	0.01%	0.002%
48	6.900	1805	1807	1809	rBV	308	140	0.01%	0.001%
49	7.010	1826	1841	1861	rBV	158352	285152	16.89%	2.434%
50	7.167	1886	1890	1891	rBV2	1152	567	0.03%	0.005%
51	7.196	1897	1899	1904	rVB2	418	272	0.02%	0.002%
52	7.222	1905	1907	1910	rVB2	429	215	0.01%	0.002%
53	7.267	1919	1921	1922	rBV	516	159	0.01%	0.001%
54	7.338	1930	1943	1971	rBV	634849	1109329	65.70%	9.469%
55	7.643	2025	2038	2065	rBV	110738	193092	11.44%	1.648%
56	7.872	2104	2109	2110	rBV3	390	270	0.02%	0.002%
57	7.900	2116	2118	2121	rVB	840	406	0.02%	0.003%
58	7.920	2121	2124	2127	rBV	298	238	0.01%	0.002%
59	7.952	2131	2134	2135	rBV2	855	494	0.03%	0.004%
60	8.064	2166	2169	2175	rVB2	330	296	0.02%	0.003%
61	8.122	2175	2187	2225	rBV	270716	622770	36.88%	5.316%
62	8.553	2319	2321	2323	rBV2	431	182	0.01%	0.002%
63	8.823	2403	2405	2407	rBV2	256	167	0.01%	0.001%
64	8.875	2408	2421	2453	rVV2	604775	1306404	77.37%	11.151%
65	9.273	2541	2545	2547	rBV2	316	224	0.01%	0.002%
66	9.434	2593	2595	2598	rBV2	251	157	0.01%	0.001%
67	9.463	2602	2604	2609	rVB	294	169	0.01%	0.001%
68	9.495	2609	2614	2615	rBV	352	263	0.02%	0.002%
69	9.547	2628	2630	2631	rBV	418	168	0.01%	0.001%
70	9.624	2652	2654	2660	rVB2	306	271	0.02%	0.002%
71	9.769	2697	2699	2704	rVB2	444	229	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031620\
 Data File : VV014958.D
 Acq On : 16 Mar 2020 20:08
 Operator : SY/MD
 Sample : L1940-12
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DA6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
 Title : VOC Analysis

72	9.801	2704	2709	2713	rBV2	293	342	0.02%	0.003%
73	9.900	2738	2740	2745	rVB2	267	148	0.01%	0.001%
74	9.945	2752	2754	2758	rBV3	376	174	0.01%	0.001%
75	10.048	2784	2786	2790	rBV	512	437	0.03%	0.004%
76	10.238	2833	2845	2863	rBV	402542	634079	37.55%	5.412%
77	10.360	2879	2883	2885	rBV2	304	203	0.01%	0.002%
78	10.408	2891	2898	2906	rVB3	1506	2536	0.15%	0.022%
79	10.563	2942	2946	2951	rVB2	510	454	0.03%	0.004%
80	10.585	2951	2953	2955	rBV	260	139	0.01%	0.001%
81	10.650	2970	2973	2976	rBV2	363	240	0.01%	0.002%
82	10.952	3065	3067	3073	rVV4	396	198	0.01%	0.002%
83	10.977	3073	3075	3080	rVB2	377	230	0.01%	0.002%
84	11.048	3093	3097	3099	rBV2	351	215	0.01%	0.002%
85	11.090	3108	3110	3113	rBV	309	225	0.01%	0.002%
86	11.203	3134	3145	3155	rBV2	54805	86481	5.12%	0.738%
87	11.273	3155	3167	3169	rBV	672486	938893	55.61%	8.014%
88	11.650	3267	3284	3310	rBV2	758486	1688437	100.00%	14.412%
89	11.817	3333	3336	3338	rBV2	491	293	0.02%	0.003%
90	11.855	3346	3348	3350	rBV	370	139	0.01%	0.001%
91	11.887	3356	3358	3360	rBV2	514	201	0.01%	0.002%
92	11.913	3364	3366	3369	rBV2	290	187	0.01%	0.002%
93	11.968	3381	3383	3386	rBV3	550	356	0.02%	0.003%
94	12.093	3420	3422	3425	rBV	575	316	0.02%	0.003%
95	12.145	3434	3438	3439	rBV2	330	178	0.01%	0.002%
96	12.260	3472	3474	3476	rBV	381	196	0.01%	0.002%
97	12.418	3514	3523	3533	rBV3	8495	13523	0.80%	0.115%
98	12.772	3625	3633	3642	rVB7	5836	8520	0.50%	0.073%
99	13.283	3780	3792	3812	rBV	414077	640118	37.91%	5.464%
100	13.765	3932	3942	3956	rVB	99085	152457	9.03%	1.301%


Sum of corrected areas: 11715389

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV031620\
Data File : VV014958.D
Acq On : 16 Mar 2020 20:08
Operator : SY/MD
Sample : L1940-12
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DA6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

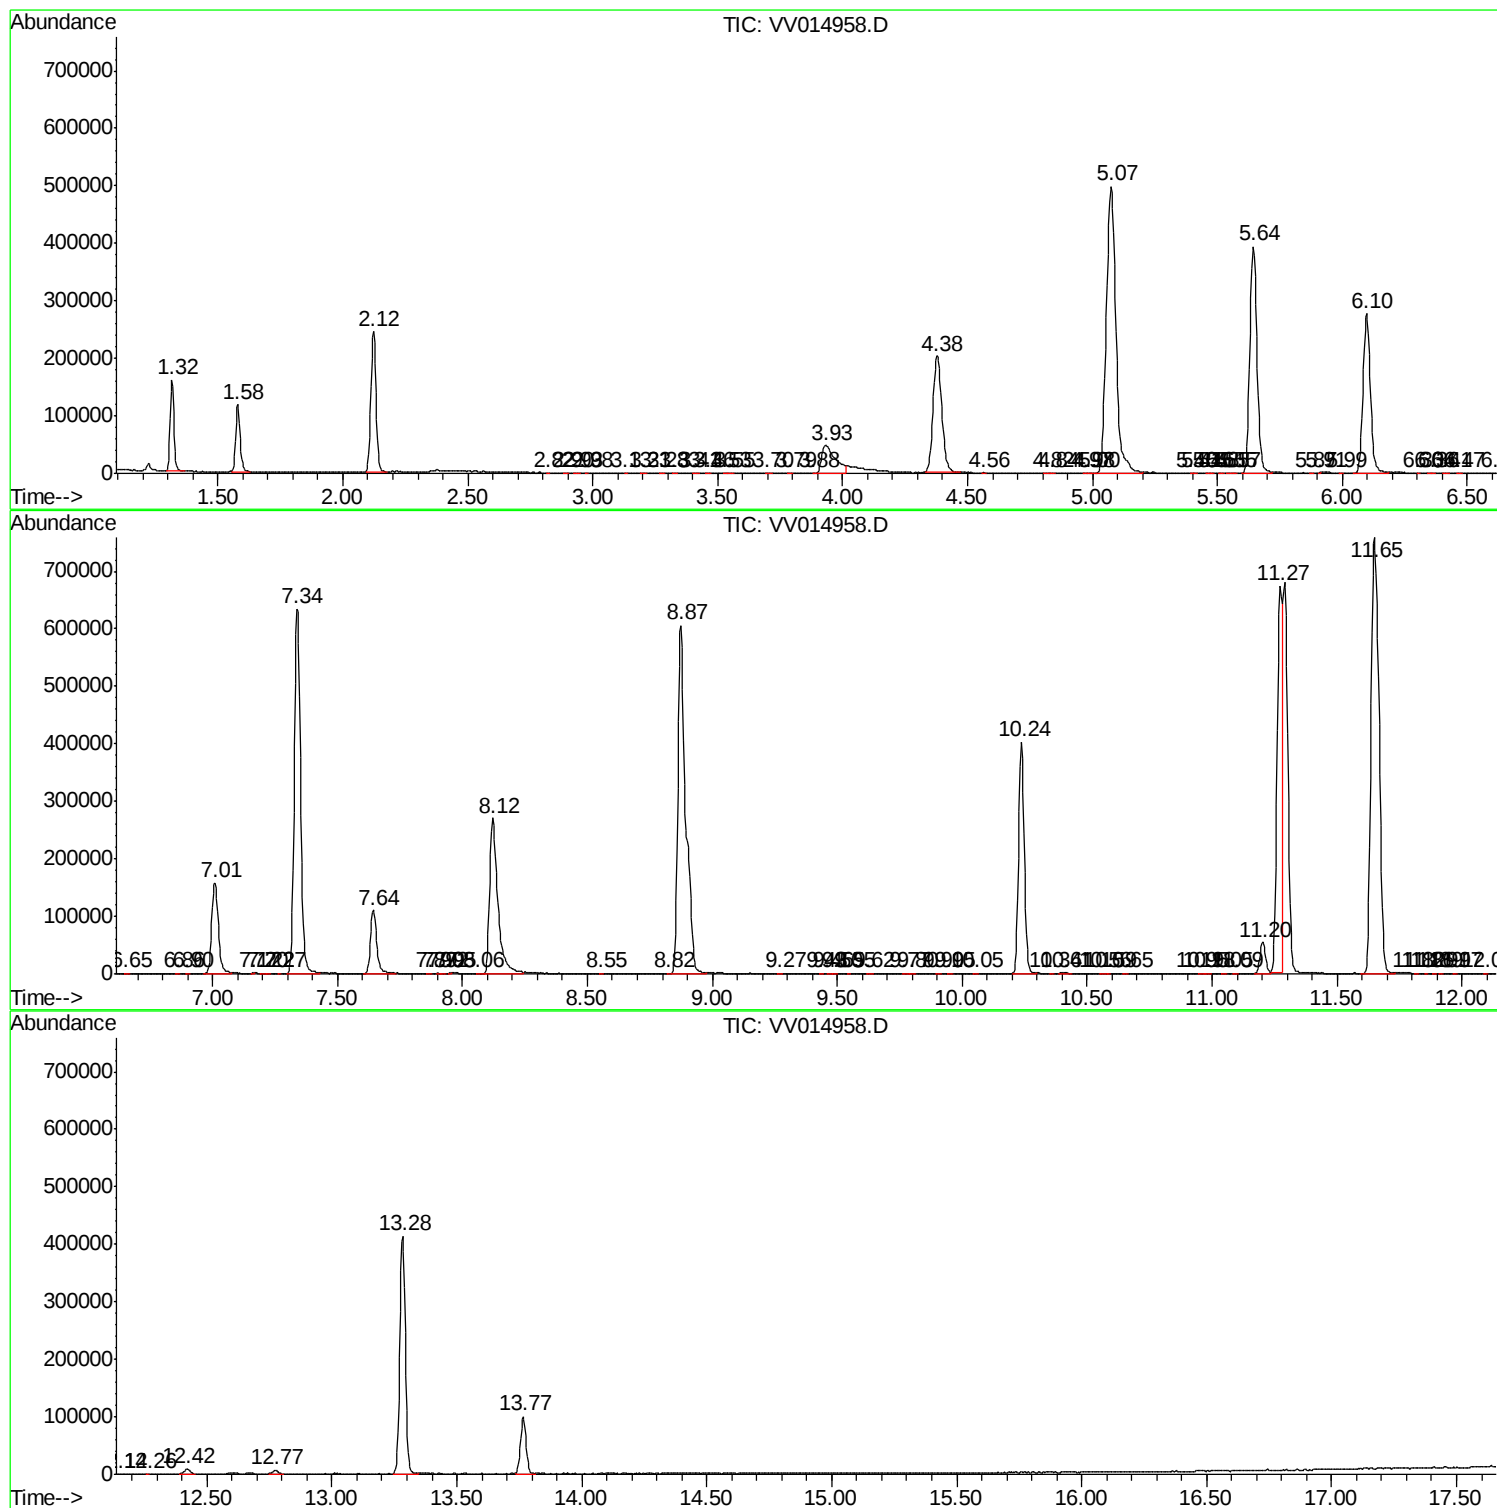

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV031620\
Data File : VV014958.D
Acq On : 16 Mar 2020 20:08
Operator : SY/MD
Sample : L1940-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DA6

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV031620\
Data File : VV014958.D
Acq On : 16 Mar 2020 20:08
Operator : SY/MD
Sample : L1940-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DA6

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc