

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031620\
 Data File : VV014959.D
 Acq On : 16 Mar 2020 20:32
 Operator : SY/MD
 Sample : L1940-13
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DA7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	86	rVB	152628	160566	12.68%	1.674%
2	1.579	144	152	165	rVB	114701	138945	10.98%	1.449%
3	2.119	311	320	336	rVB	235358	336007	26.54%	3.504%
4	2.840	541	544	546	rBV2	600	361	0.03%	0.004%
5	2.959	578	581	586	rBV3	430	361	0.03%	0.004%
6	2.984	586	589	590	rBV2	342	200	0.02%	0.002%
7	3.039	601	606	607	rBV	330	254	0.02%	0.003%
8	3.168	643	646	649	rBV2	249	156	0.01%	0.002%
9	3.354	698	704	705	rBV2	224	258	0.02%	0.003%
10	3.386	712	714	715	rBV2	194	77	0.01%	0.001%
11	3.512	751	753	755	rVB	214	66	0.01%	0.001%
12	3.579	770	774	775	rBV2	325	191	0.02%	0.002%
13	3.589	775	777	778	rBV	299	84	0.01%	0.001%
14	3.727	817	820	823	rBV2	551	328	0.03%	0.003%
15	3.933	873	884	918	rBV2	46775	195997	15.48%	2.044%
16	4.376	1006	1022	1049	rBV2	194696	483437	38.19%	5.041%
17	4.711	1124	1126	1133	rBV4	276	256	0.02%	0.003%
18	4.785	1146	1149	1150	rBV	315	160	0.01%	0.002%
19	4.827	1161	1162	1163	rBV	170	36	0.00%	0.000%
20	4.852	1168	1170	1173	rVB2	336	169	0.01%	0.002%
21	4.868	1173	1175	1177	rBV	258	98	0.01%	0.001%
22	4.881	1177	1179	1180	rBV	198	85	0.01%	0.001%
23	5.000	1213	1216	1220	rBV3	559	331	0.03%	0.003%
24	5.074	1221	1239	1276	rBV2	484937	1265941	100.00%	13.201%
25	5.373	1329	1332	1335	rBV2	379	272	0.02%	0.003%
26	5.470	1356	1362	1364	rBV3	388	303	0.02%	0.003%
27	5.573	1392	1394	1396	rBV	300	174	0.01%	0.002%
28	5.640	1402	1415	1442	rBV	375331	752431	59.44%	7.846%
29	5.846	1477	1479	1483	rVB2	409	187	0.01%	0.002%
30	5.888	1490	1492	1493	rBV2	478	200	0.02%	0.002%
31	6.097	1542	1557	1579	rBV	270661	543875	42.96%	5.672%
32	6.274	1610	1612	1617	rVB3	926	545	0.04%	0.006%
33	6.364	1637	1640	1642	rBV	473	259	0.02%	0.003%
34	6.386	1644	1647	1653	rVB2	375	342	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031620\
 Data File : VV014959.D
 Acq On : 16 Mar 2020 20:32
 Operator : SY/MD
 Sample : L1940-13
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DA7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
 Title : VOC Analysis

35	6.534	1688	1693	1696	rBV4	415	404	0.03%	0.004%
36	6.579	1705	1707	1710	rBV	190	102	0.01%	0.001%
37	6.598	1711	1713	1717	rVV2	345	198	0.02%	0.002%
38	6.666	1731	1734	1735	rBV	375	182	0.01%	0.002%
39	6.682	1735	1739	1741	rVB2	892	588	0.05%	0.006%
40	6.695	1741	1743	1745	rBV	153	61	0.00%	0.001%
41	6.727	1750	1753	1755	rBV3	313	171	0.01%	0.002%
42	6.753	1758	1761	1764	rBV3	459	262	0.02%	0.003%
43	6.884	1799	1802	1804	rVB2	296	120	0.01%	0.001%
44	6.904	1804	1808	1810	rBV2	355	274	0.02%	0.003%
45	7.010	1826	1841	1862	rBV	149202	272856	21.55%	2.845%
46	7.338	1930	1943	1969	rBV	607148	1058335	83.60%	11.037%
47	7.521	1996	2000	2002	rBV2	565	434	0.03%	0.005%
48	7.643	2027	2038	2060	rBV2	102818	178867	14.13%	1.865%
49	7.794	2083	2085	2086	rBV	410	190	0.02%	0.002%
50	7.820	2091	2093	2096	rVV3	398	255	0.02%	0.003%
51	7.846	2098	2101	2105	rVB3	432	307	0.02%	0.003%
52	7.875	2105	2110	2112	rBV	653	417	0.03%	0.004%
53	7.965	2128	2138	2145	rBV4	2708	4592	0.36%	0.048%
54	8.048	2160	2164	2165	rBV4	175	119	0.01%	0.001%
55	8.122	2175	2187	2226	rBV	264379	604623	47.76%	6.305%
56	8.318	2246	2248	2251	rBV3	1014	594	0.05%	0.006%
57	8.466	2292	2294	2295	rBV3	311	128	0.01%	0.001%
58	8.634	2343	2346	2351	rBV2	369	225	0.02%	0.002%
59	8.672	2355	2358	2361	rBV2	451	226	0.02%	0.002%
60	8.733	2375	2377	2381	rBV2	308	197	0.02%	0.002%
61	8.875	2408	2421	2447	rBV	574419	1026371	81.08%	10.703%
62	9.019	2465	2466	2467	rBV	425	125	0.01%	0.001%
63	9.158	2507	2509	2512	rBV3	637	331	0.03%	0.003%
64	9.312	2555	2557	2560	rBV2	223	137	0.01%	0.001%
65	9.325	2560	2561	2565	rVB	394	166	0.01%	0.002%
66	9.460	2600	2603	2604	rBV	208	99	0.01%	0.001%
67	9.476	2606	2608	2612	rVB2	324	189	0.01%	0.002%
68	9.653	2662	2663	2668	rVB2	312	214	0.02%	0.002%
69	9.701	2675	2678	2680	rBV	273	183	0.01%	0.002%
70	9.788	2704	2705	2706	rVB	215	41	0.00%	0.000%
71	9.839	2719	2721	2722	rBV	261	100	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031620\
 Data File : VV014959.D
 Acq On : 16 Mar 2020 20:32
 Operator : SY/MD
 Sample : L1940-13
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DA7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
 Title : VOC Analysis

72	9.904	2738	2741	2743	rBV	234	134	0.01%	0.001%
73	10.016	2774	2776	2777	rBV	301	108	0.01%	0.001%
74	10.026	2777	2779	2780	rBV	179	58	0.00%	0.001%
75	10.238	2832	2845	2862	rBV	396557	618791	48.88%	6.453%
76	10.408	2889	2898	2907	rVB3	3087	4844	0.38%	0.051%
77	10.515	2928	2931	2933	rBV	194	126	0.01%	0.001%
78	10.560	2942	2945	2950	rVB3	685	506	0.04%	0.005%
79	10.929	3058	3060	3066	rBV3	338	367	0.03%	0.004%
80	10.987	3076	3078	3083	rVB2	313	216	0.02%	0.002%
81	11.096	3110	3112	3114	rBV	295	138	0.01%	0.001%
82	11.206	3138	3146	3153	rBV5	2497	3661	0.29%	0.038%
83	11.270	3154	3166	3195	rVV	565184	926927	73.22%	9.666%
84	11.646	3270	3283	3305	rBV	613921	981021	77.49%	10.230%
85	11.823	3335	3338	3342	rBV3	590	400	0.03%	0.004%
86	12.662	3597	3599	3603	rBV4	493	378	0.03%	0.004%
87	13.283	3784	3792	3804	rVB5	9628	15625	1.23%	0.163%
88	13.363	3815	3817	3818	rBV	390	158	0.01%	0.002%
89	13.916	3986	3989	3991	rBV	521	305	0.02%	0.003%


Sum of corrected areas: 9589398

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV031620\
Data File : VV014959.D
Acq On : 16 Mar 2020 20:32
Operator : SY/MD
Sample : L1940-13
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DA7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

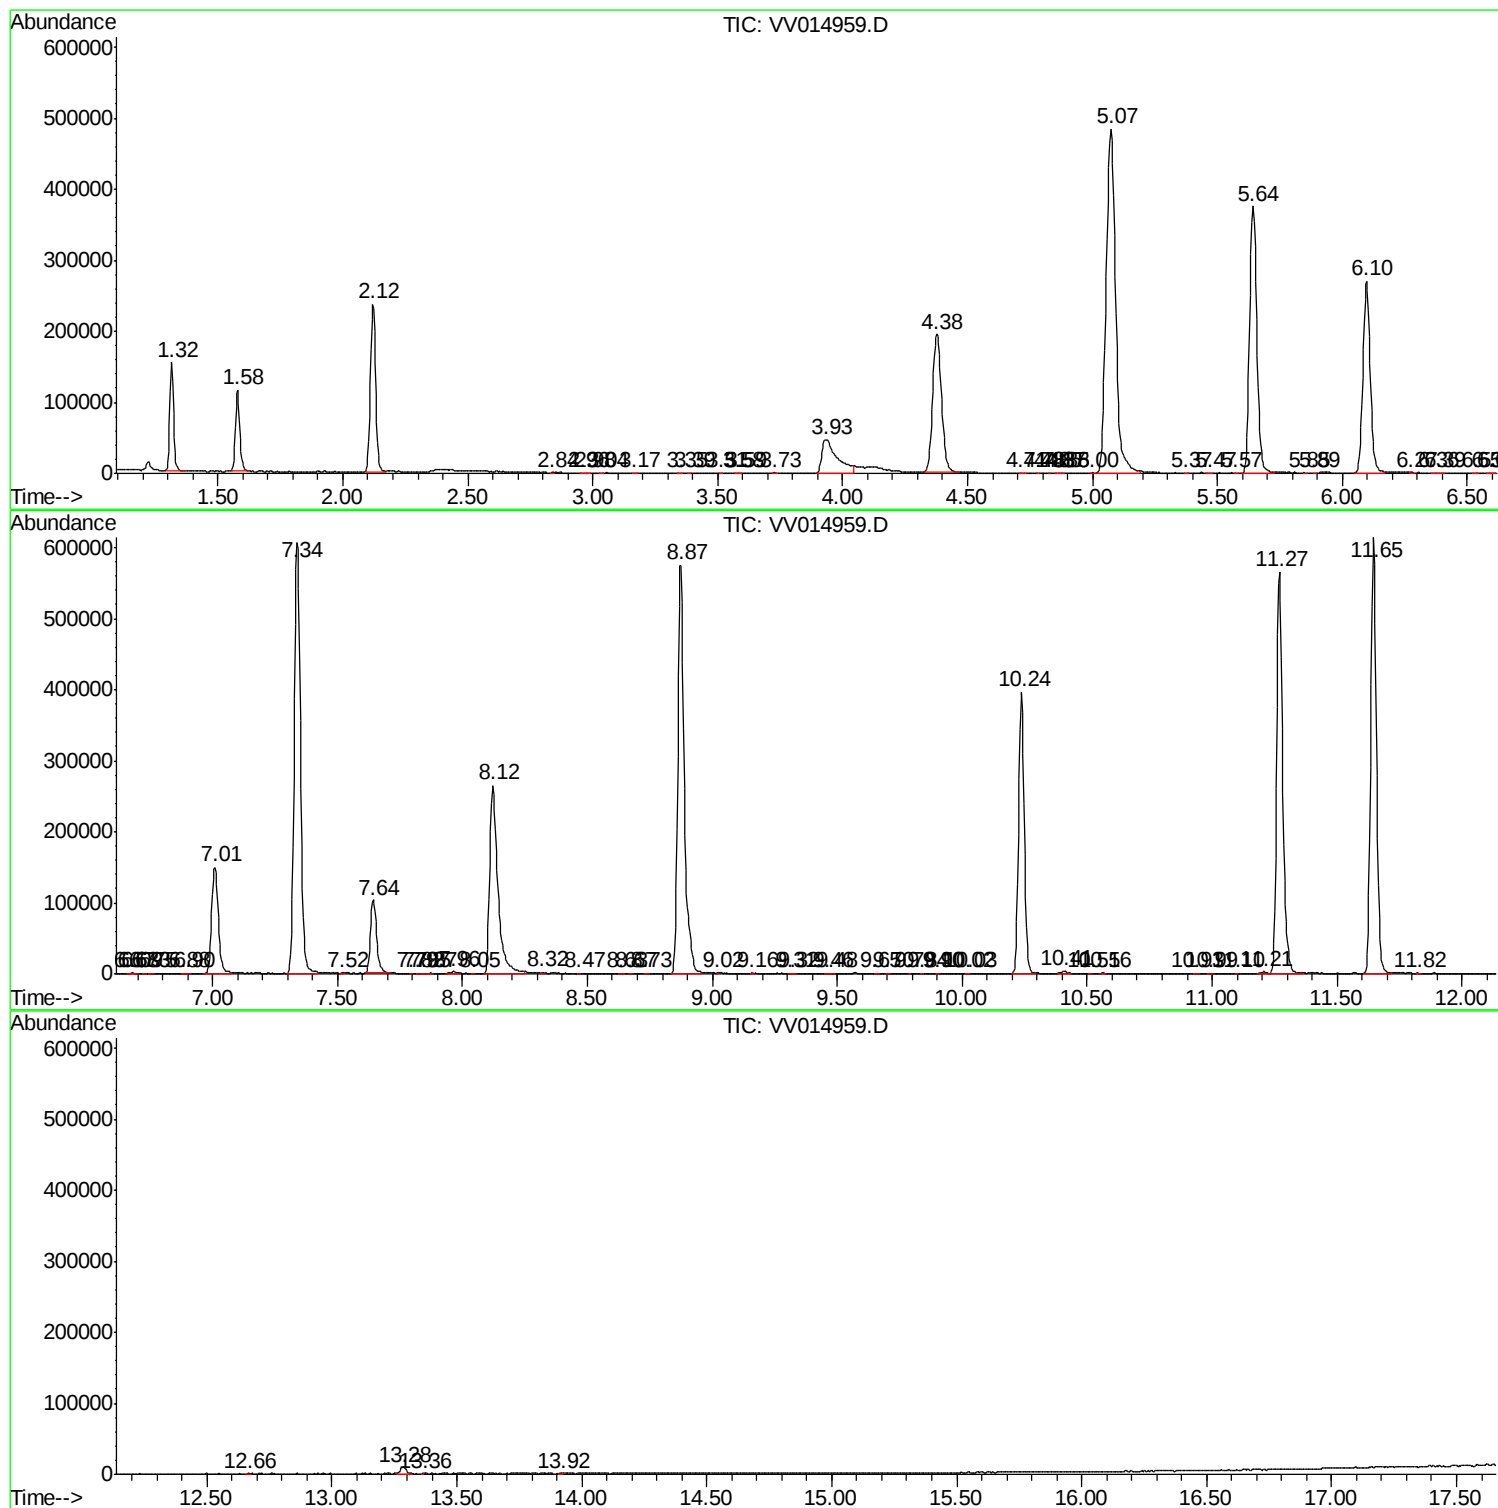

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV031620\
Data File : VV014959.D
Acq On : 16 Mar 2020 20:32
Operator : SY/MD
Sample : L1940-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DA7

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV031620\
Data File : VV014959.D
Acq On : 16 Mar 2020 20:32
Operator : SY/MD
Sample : L1940-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DA7

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc