

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031620\
 Data File : VV014960.D
 Acq On : 16 Mar 2020 20:56
 Operator : SY/MD
 Sample : L1940-15
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DB0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.222	37	41	49	rVB2	18856	17983	1.36%	0.176%
2	1.316	63	70	82	rBV	158440	163915	12.39%	1.605%
3	1.579	145	152	166	rVB	118222	142187	10.75%	1.393%
4	2.119	312	320	338	rVB	244911	355831	26.89%	3.485%
5	2.959	579	581	584	rBV3	631	337	0.03%	0.003%
6	3.148	638	640	642	rBV	264	103	0.01%	0.001%
7	3.203	655	657	661	rBV3	694	450	0.03%	0.004%
8	3.290	682	684	685	rBV	157	51	0.00%	0.000%
9	3.360	704	706	710	rVB2	346	213	0.02%	0.002%
10	3.467	737	739	742	rBV2	335	169	0.01%	0.002%
11	3.524	755	757	759	rBV	297	125	0.01%	0.001%
12	3.553	764	766	769	rVB3	452	219	0.02%	0.002%
13	3.569	769	771	778	rBV2	192	174	0.01%	0.002%
14	3.605	779	782	784	rBV	310	156	0.01%	0.002%
15	3.631	787	790	794	rBV	402	276	0.02%	0.003%
16	3.933	872	884	905	rBV2	47798	175078	13.23%	1.715%
17	4.377	1005	1022	1051	rBV	212167	525081	39.68%	5.143%
18	4.820	1156	1160	1163	rBV2	358	296	0.02%	0.003%
19	4.885	1179	1180	1184	rBV2	355	241	0.02%	0.002%
20	4.958	1201	1203	1205	rBV	312	130	0.01%	0.001%
21	5.074	1220	1239	1275	rBV2	510359	1323176	100.00%	12.959%
22	5.380	1331	1334	1336	rBV2	750	446	0.03%	0.004%
23	5.643	1402	1416	1436	rBV	396287	790939	59.78%	7.747%
24	5.926	1500	1504	1506	rBV3	722	650	0.05%	0.006%
25	5.971	1515	1518	1519	rBV2	581	358	0.03%	0.004%
26	5.997	1523	1526	1529	rBV3	447	324	0.02%	0.003%
27	6.097	1542	1557	1580	rBV	279161	574929	43.45%	5.631%
28	6.457	1667	1669	1670	rBV	190	61	0.00%	0.001%
29	6.585	1707	1709	1712	rVB2	459	235	0.02%	0.002%
30	6.618	1716	1719	1722	rVB2	564	309	0.02%	0.003%
31	6.650	1722	1729	1732	rBV4	630	692	0.05%	0.007%
32	6.878	1798	1800	1803	rBV2	320	174	0.01%	0.002%
33	6.917	1811	1812	1815	rVB2	224	85	0.01%	0.001%
34	7.010	1829	1841	1867	rBV	155942	284614	21.51%	2.788%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031620\
 Data File : VV014960.D
 Acq On : 16 Mar 2020 20:56
 Operator : SY/MD
 Sample : L1940-15
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DB0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
 Title : VOC Analysis

35	7.155	1880	1886	1887	rBV2	1545	1419	0.11%	0.014%
36	7.286	1926	1927	1929	rBV	238	106	0.01%	0.001%
37	7.338	1930	1943	1964	rBV	638888	1121422	84.75%	10.983%
38	7.643	2027	2038	2060	rBV	108819	186807	14.12%	1.830%
39	7.872	2107	2109	2110	rBV	269	69	0.01%	0.001%
40	7.923	2123	2125	2126	rBV	299	131	0.01%	0.001%
41	8.122	2175	2187	2218	rBV	277590	635040	47.99%	6.220%
42	8.537	2314	2316	2317	rBV	302	89	0.01%	0.001%
43	8.566	2323	2325	2326	rBV	449	193	0.01%	0.002%
44	8.695	2361	2365	2368	rBV3	392	256	0.02%	0.003%
45	8.772	2386	2389	2391	rVB3	462	228	0.02%	0.002%
46	8.788	2391	2394	2397	rBV2	332	261	0.02%	0.003%
47	8.875	2408	2421	2448	rBV	611682	1086148	82.09%	10.638%
48	9.080	2483	2485	2486	rBV2	473	191	0.01%	0.002%
49	9.151	2505	2507	2508	rBV2	327	99	0.01%	0.001%
50	9.312	2555	2557	2560	rBV2	291	167	0.01%	0.002%
51	9.524	2621	2623	2629	rVB	393	189	0.01%	0.002%
52	9.556	2630	2633	2636	rBV3	569	417	0.03%	0.004%
53	9.788	2703	2705	2710	rBV2	617	560	0.04%	0.005%
54	9.945	2751	2754	2755	rBV	592	282	0.02%	0.003%
55	10.238	2833	2845	2865	rBV	414583	654216	49.44%	6.407%
56	10.408	2890	2898	2909	rVB4	2888	4606	0.35%	0.045%
57	10.489	2922	2923	2924	rBV4	303	65	0.00%	0.001%
58	10.682	2981	2983	2984	rBV	331	125	0.01%	0.001%
59	10.727	2995	2997	3000	rBV2	315	162	0.01%	0.002%
60	10.743	3000	3002	3004	rBV	340	181	0.01%	0.002%
61	10.900	3049	3051	3055	rVB2	466	237	0.02%	0.002%
62	11.116	3116	3118	3119	rBV	448	166	0.01%	0.002%
63	11.270	3154	3166	3188	rBV	621617	1053789	79.64%	10.321%
64	11.486	3231	3233	3235	rVB2	803	301	0.02%	0.003%
65	11.646	3271	3283	3303	rBV	661557	1076516	81.36%	10.543%
66	11.920	3364	3368	3370	rBV2	416	230	0.02%	0.002%
67	12.492	3544	3546	3549	rBV	268	172	0.01%	0.002%
68	12.669	3593	3601	3608	rVB4	2861	3724	0.28%	0.036%
69	12.736	3620	3622	3627	rBV2	401	356	0.03%	0.003%
70	13.286	3784	3793	3805	rVB3	13493	21307	1.61%	0.209%

LSC Area Percent Report

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031620\
Data File : VV014960.D
Acq On : 16 Mar 2020 20:56
Operator : SY/MD
Sample : L1940-15
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DB0

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Title : VOC Analysis


Sum of corrected areas: 10210234

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV031620\
Data File : VV014960.D
Acq On : 16 Mar 2020 20:56
Operator : SY/MD
Sample : L1940-15
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DB0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

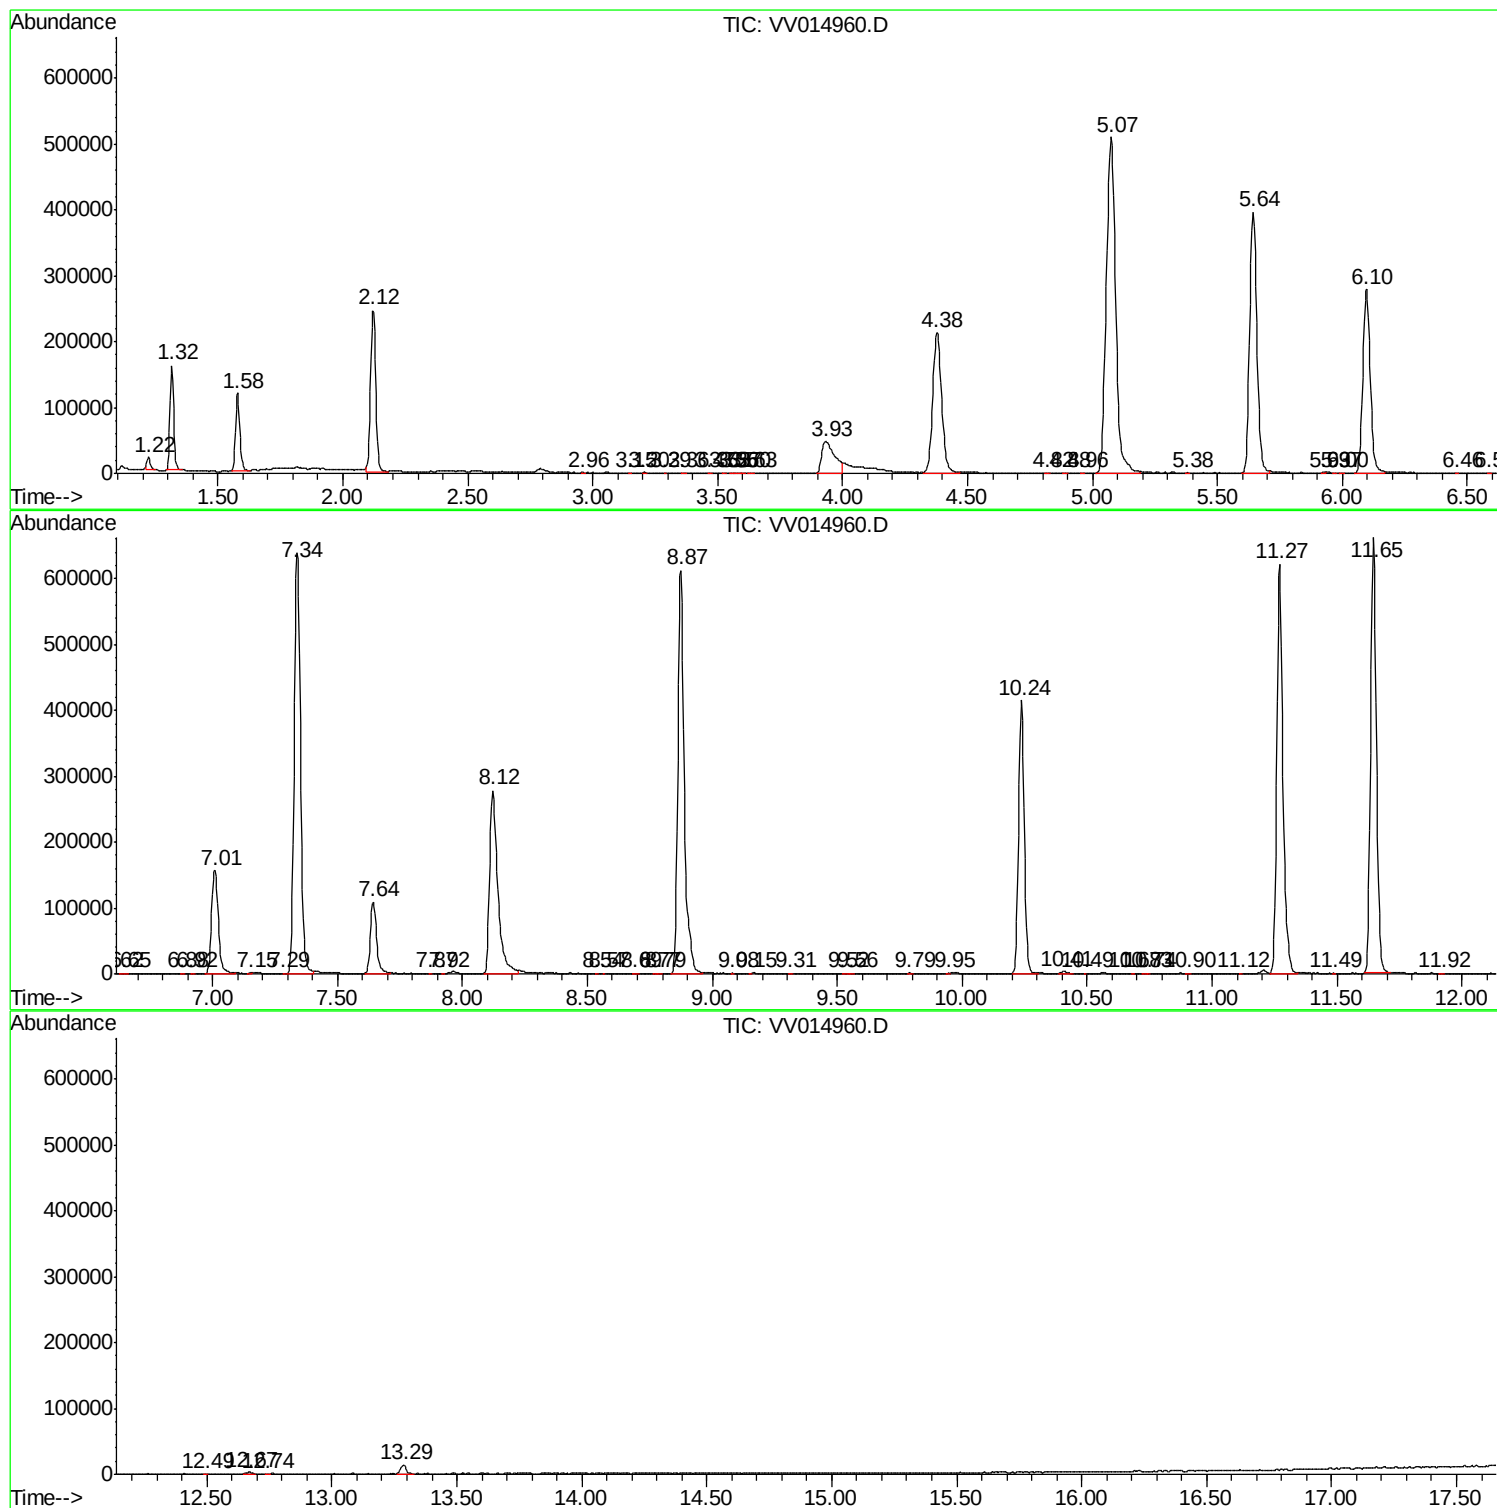

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV031620\
Data File : VV014960.D
Acq On : 16 Mar 2020 20:56
Operator : SY/MD
Sample : L1940-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DB0

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV031620\
Data File : VV014960.D
Acq On : 16 Mar 2020 20:56
Operator : SY/MD
Sample : L1940-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DB0

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc