


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV031620\
 Data File : VV014933.D
 Acq On : 16 Mar 2020 09:03
 Operator : SY/MD
 Sample : BFB64
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB64

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
 Title : VOC Analysis
 Last Update : Wed Mar 18 07:43:00 2020

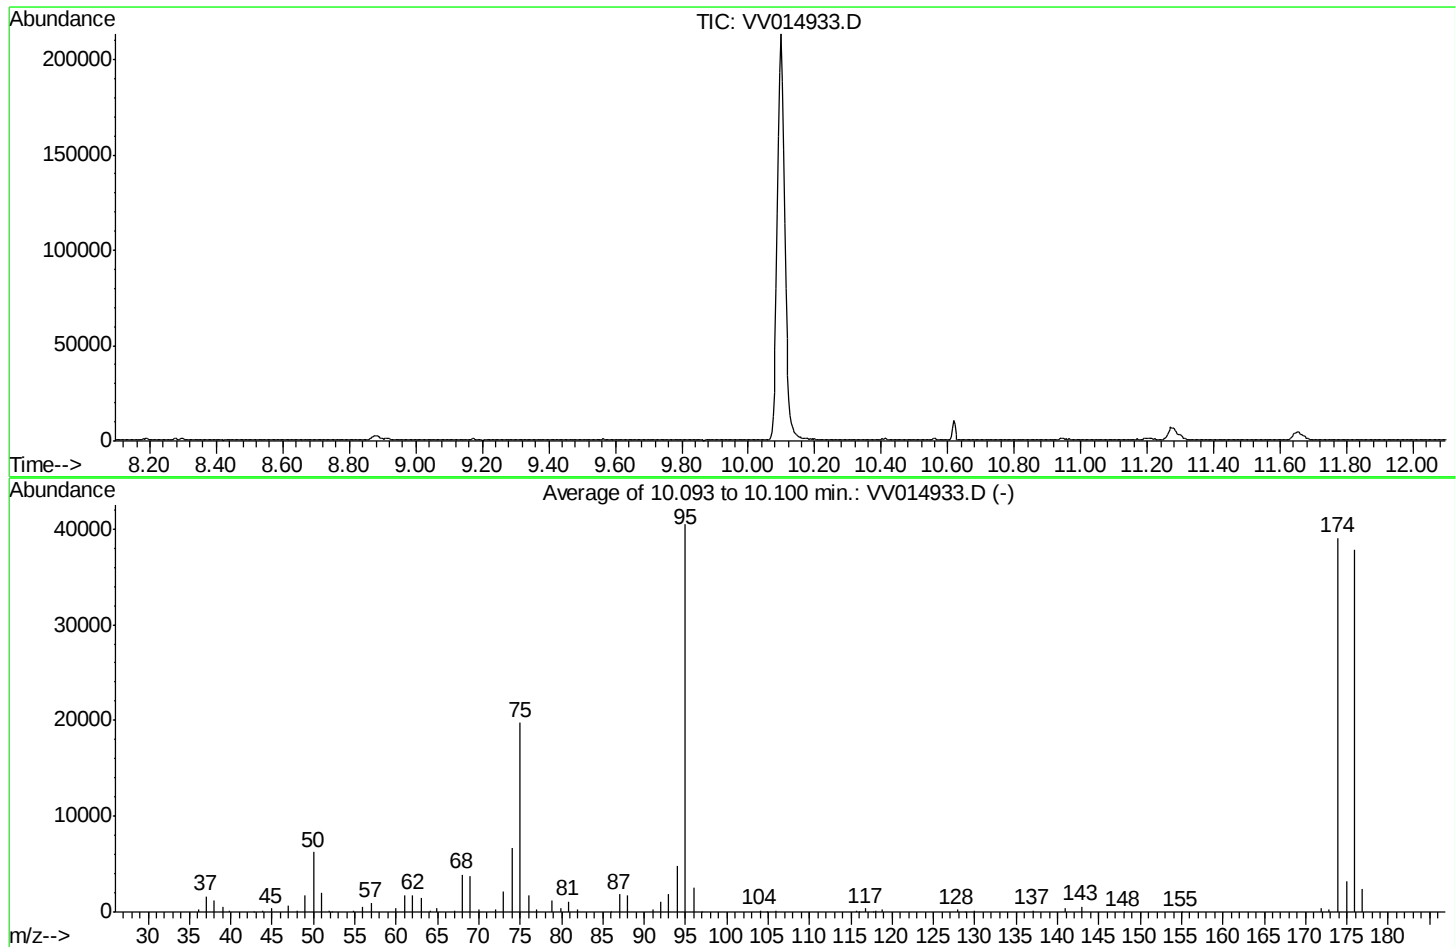

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2789

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.5	6273	PASS
75	95	30	80	48.8	19746	PASS
95	95	100	100	100.0	40474	PASS
96	95	5	9	6.2	2508	PASS
173	174	0.00	2	0.8	320	PASS
174	95	50	120	96.5	39045	PASS
175	174	5	9	8.1	3149	PASS
176	174	95	101	97.0	37874	PASS
177	176	5	9	6.5	2461	PASS

m/z	Abundance
36.00	334.0
37.00	1650.0
38.00	1282.0
39.00	614.0
39.90	253.0
43.90	439.0
44.90	338.0
47.00	580.0
48.00	146.0
49.00	1446.0
50.00	6118.0
51.00	1863.0
51.90	129.0
54.90	134.0
55.90	616.0
57.00	850.0
59.90	397.0
61.00	1658.0
62.00	1541.0
63.00	1476.0
64.10	107.0
65.00	351.0
67.00	140.0
68.00	3499.0
69.00	3563.0
70.00	248.0
71.90	319.0
73.00	1963.0
74.00	5940.0
75.00	19520.0
76.00	1647.0
76.90	296.0
78.90	1041.0
79.90	391.0
80.90	1044.0
82.10	308.0
87.00	1767.0
87.90	1534.0
91.00	249.0
92.00	1068.0
93.00	1757.0
94.00	4547.0
95.00	38248.0
96.00	2394.0
104.00	144.0
104.80	106.0
105.90	116.0
115.70	159.0
116.80	360.0
118.00	130.0
118.80	348.0
128.10	209.0
129.80	125.0
137.10	147.0
140.90	392.0
142.90	486.0
171.90	329.0
172.80	286.0
173.90	35912.0
174.90	3073.0
175.90	35208.0
176.90	2254.0

Instrument :
MSVOA_V
ClientSampleId :
BFB64

m/z	Abundance
36.00	272.0
37.00	1769.0
38.00	1272.0
39.00	624.0
39.90	300.0
43.90	441.0
44.90	381.0
46.90	650.0
48.00	205.0
49.00	1901.0
50.00	6372.0
51.00	2022.0
51.90	111.0
54.90	143.0
55.90	623.0
57.00	1061.0
59.90	449.0
61.00	1791.0
62.00	1844.0
63.00	1514.0
64.10	136.0
65.00	375.0
67.00	164.0
68.00	4057.0
69.00	3922.0
70.10	331.0
72.00	334.0
73.00	2218.0
74.00	6940.0
75.00	20248.0
76.00	1741.0
76.90	264.0
78.90	1235.0
79.90	401.0
80.80	1151.0
82.00	257.0
87.00	1914.0
87.90	1864.0
91.00	251.0
92.00	1152.0
93.00	1990.0
94.00	5085.0
95.00	41880.0
96.00	2608.0
104.00	163.0
105.90	139.0
115.80	150.0
116.80	379.0
117.70	127.0
118.10	118.0
118.80	321.0
127.90	256.0
129.90	140.0
137.10	176.0
140.80	462.0
142.90	624.0
154.90	101.0
172.00	395.0
172.80	333.0
173.90	40432.0
174.90	3314.0
175.90	39016.0
176.90	2505.0

Instrument :
MSVOA_V
ClientSampleId :
BFB64

m/z	Abundance
36.10	261.0
37.00	1598.0
38.00	1225.0
39.00	540.0
39.90	336.0
42.70	108.0
43.90	369.0
44.90	386.0
46.90	600.0
48.00	235.0
49.00	1963.0
50.00	6329.0
51.00	1988.0
52.20	116.0
54.90	121.0
55.90	565.0
57.00	1053.0
59.90	434.0
61.00	1676.0
62.00	2005.0
63.00	1475.0
64.10	167.0
64.90	365.0
67.10	158.0
68.00	4121.0
69.00	3776.0
70.10	364.0
72.00	326.0
73.00	2092.0
74.00	6992.0
75.00	19472.0
76.00	1688.0
77.00	224.0
78.90	1168.0
79.90	396.0
80.80	1191.0
81.90	234.0
85.90	106.0
87.00	1891.0
88.00	1954.0
91.00	179.0
92.00	1076.0
93.00	1940.0
94.00	5012.0
95.00	41296.0
96.00	2522.0
97.00	122.0
104.00	156.0
105.90	119.0
116.00	137.0
116.80	358.0
118.90	258.0
127.80	282.0
128.80	131.0
129.90	157.0
137.00	145.0
140.80	502.0
142.90	648.0
148.00	103.0
155.00	114.0
172.00	386.0
172.80	342.0
173.90	40792.0
174.90	3061.0
175.90	39400.0
176.90	2626.0

Instrument :
MSVOA_V
ClientSampleId :
BFB64

Scan 2789 (10.058 min): VV014933.D
BFB64

m/z	Abundance
39.90	172.0
43.80	229.0

Instrument :
MSVOA_V
ClientSampleId :
BFB64