

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW031621\
 Data File : VW020635.D
 Acq On : 16 Mar 2021 17:01
 Operator : SY/MD
 Sample : M1675-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BD5

Quant Time: Mar 17 01:52:30 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM031321WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Mar 17 01:47:28 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	431443	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	425953	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.255	152	184161	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	120159	34.53	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	69.06%		
7) Chloroethane-d5	1.571	69	106527	38.26	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	76.52%		
11) 1,1-Dichloroethene-d2	2.111	63	188052	28.43	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	56.86%#		
21) 2-Butanone-d5	3.889	46	251434	112.57	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	112.57%		
24) Chloroform-d	4.352	84	260242	43.02	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	86.04%		
26) 1,2-Dichloroethane-d4	5.034	65	184383	46.20	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	92.40%		
32) Benzene-d6	5.053	84	516565	43.89	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	87.78%		
36) 1,2-Dichloropropane-d6	6.075	67	176531	46.88	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	93.76%		
41) Toluene-d8	7.320	98	431155	41.22	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	82.44%		
43) trans-1,3-Dichloroprop...	7.625	79	73203	41.60	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	83.20%		
47) 2-Hexanone-d5	8.091	63	143292	101.71	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	101.71%		
57) 1,1,2,2-Tetrachloroeth...	10.220	84	223048	47.40	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	94.80%		
64) 1,2-Dichlorobenzene-d4	11.631	152	177992	49.88	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	99.76%		
Target Compounds						Qvalue
25) Chloroform	4.375	83	13699	2.21	ug/L	86
27) 1,2-Dichloroethane	5.056	62	3510	0.72	ug/L	99
48) 2-Hexanone	8.153	43	9788	2.48	ug/L #	49


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031621\
Data File : VV020635.D
Acq On : 16 Mar 2021 17:01
Operator : SY/MD
Sample : M1675-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BD5

Quant Time: Mar 17 01:52:30 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM031321WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Mar 17 01:47:28 2021
Response via : Initial Calibration




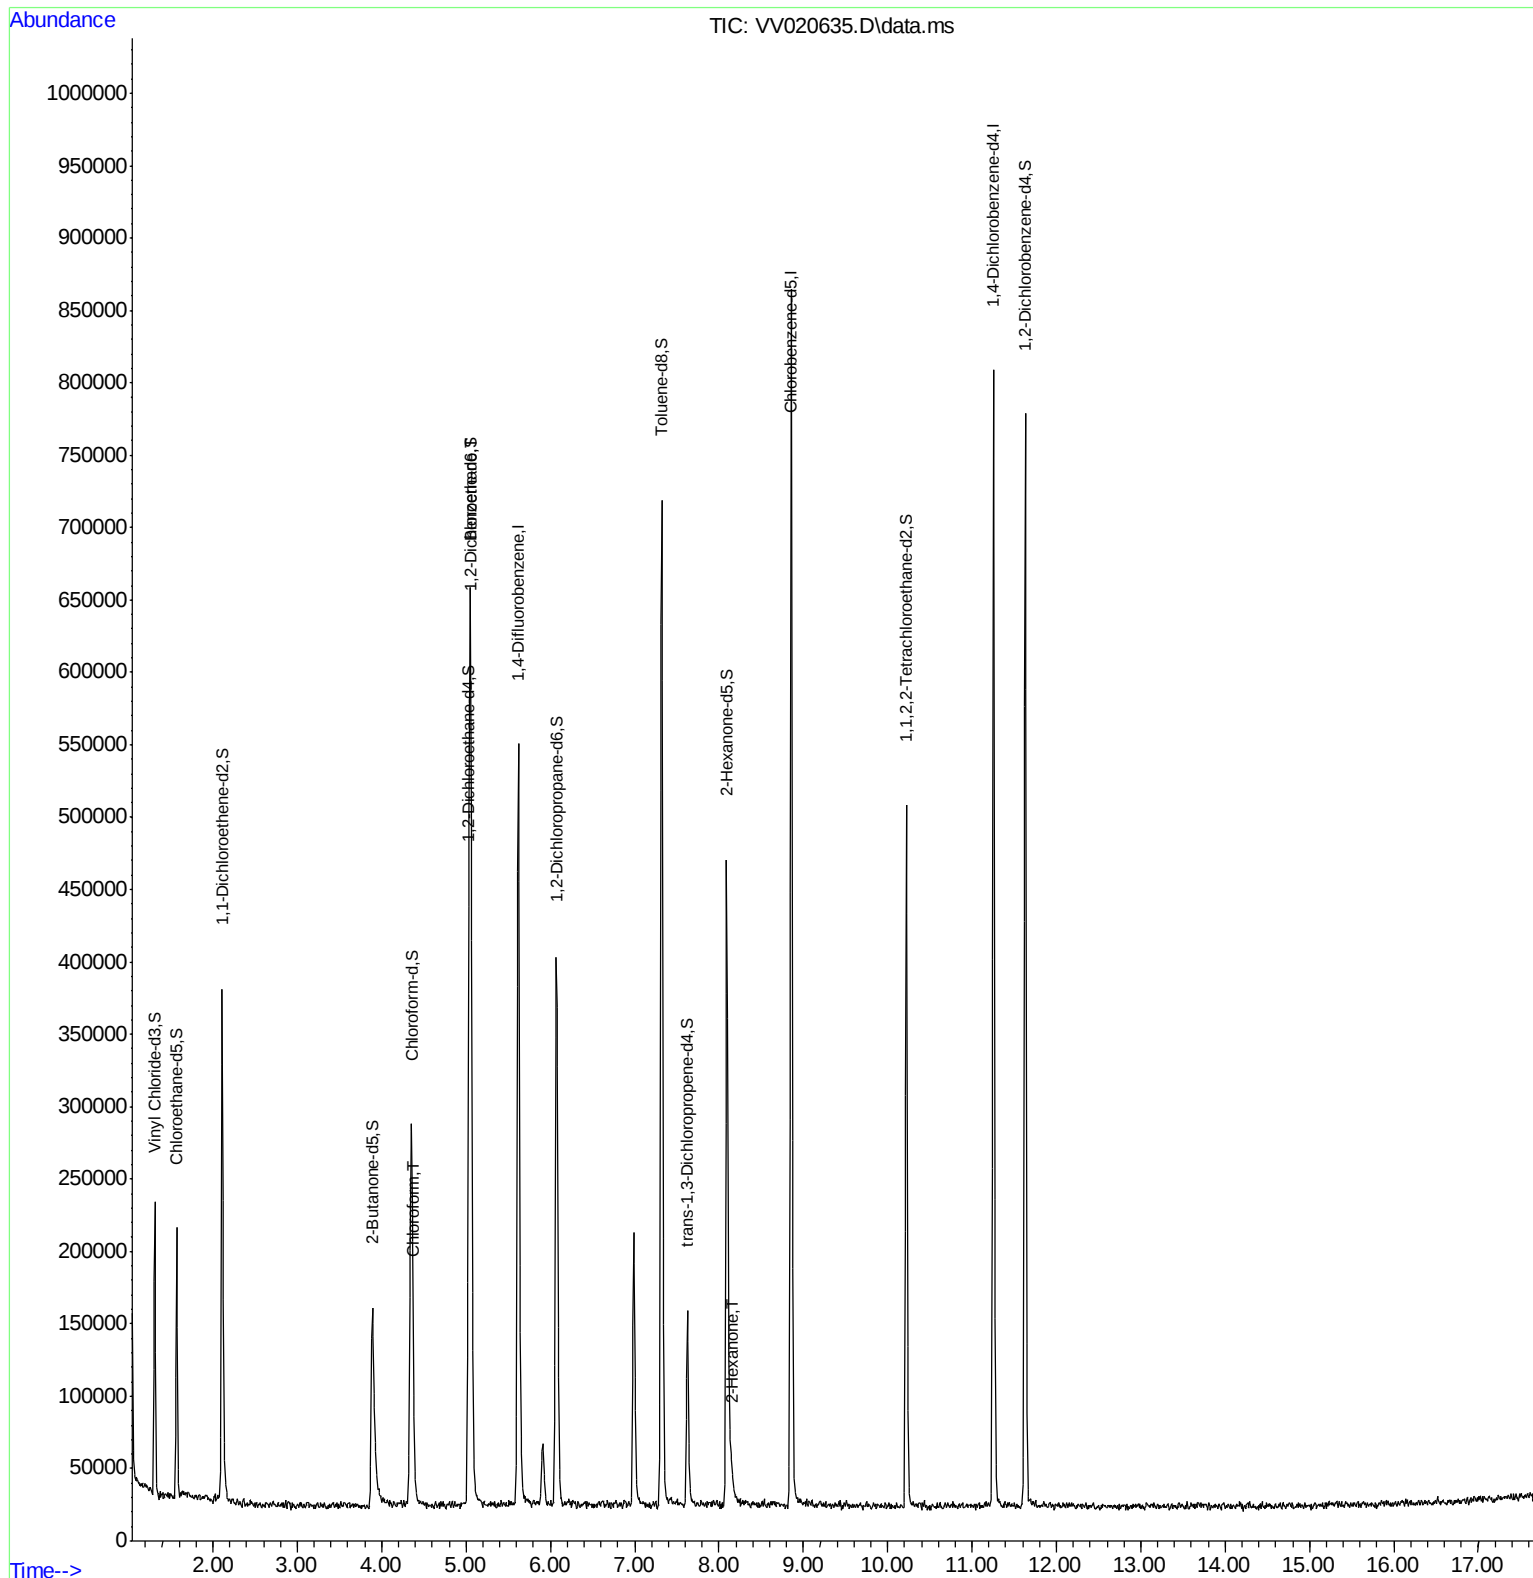


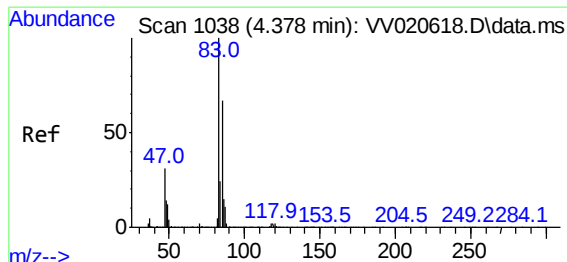

#25
Chloroform
Concen: 2.21 ug/L
RT: 4.375 min Scan# 1037
Delta R.T. -0.003 min
Lab File: VV020635.D
Acq: 16 Mar 2021 17:01




Instrument :
MSVOA_V
ClientSampleId :
C0BD5


Tgt Ion: 83 Resp: 13699
Ion Ratio Lower Upper
83 100
85 74.0 44.2 82.2

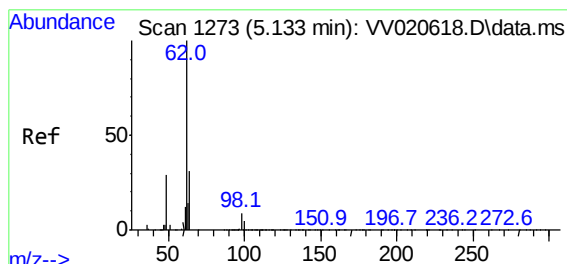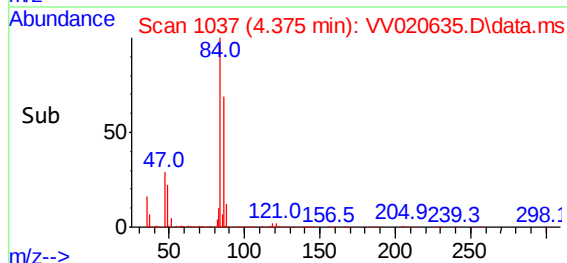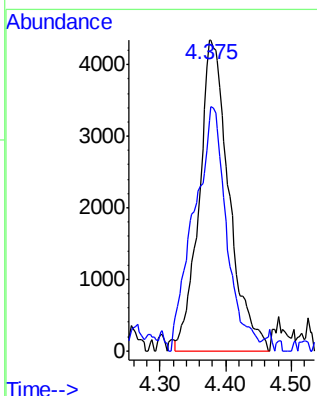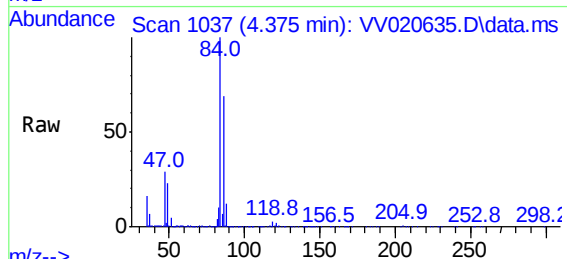

#27
1,2-Dichloroethane
Concen: 0.72 ug/L
RT: 5.056 min Scan# 1249
Delta R.T. -0.077 min
Lab File: VV020635.D
Acq: 16 Mar 2021 17:01


Tgt Ion: 62 Resp: 3510
Ion Ratio Lower Upper
62 100
98 8.9 6.9 10.3

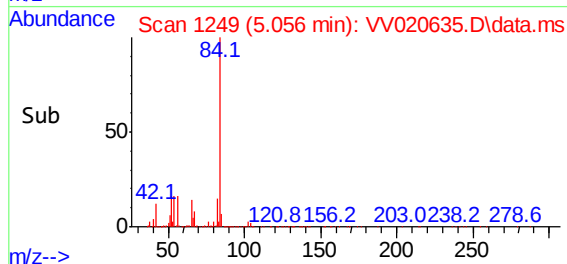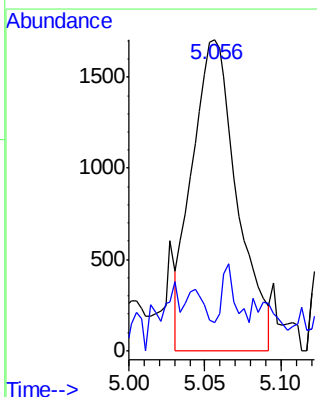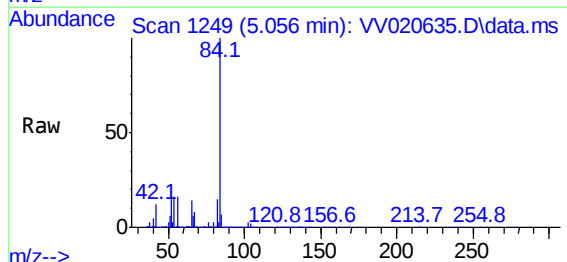

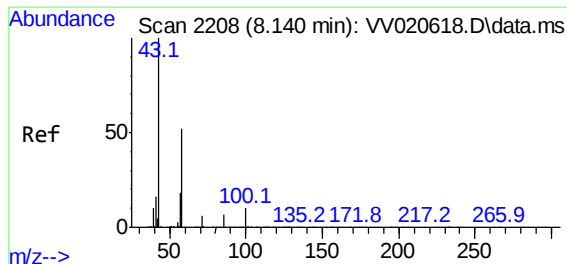

#48
 2-Hexanone
 Concen: 2.48 ug/L
 RT: 8.153 min Scan# 2212
 Delta R.T. 0.013 min
 Lab File: VV020635.D
 Acq: 16 Mar 2021 17:01

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BD5

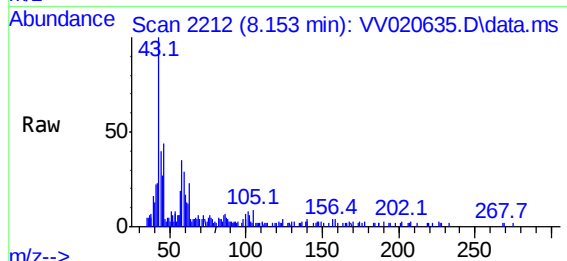

Tgt Ion: 43 Resp: 9788

Ion	Ratio	Lower	Upper
43	100		
58	5.2	41.8	62.6#
57	6.2	15.0	22.4#
100	4.2	8.9	13.3#

