

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031621\
 Data File : VV020619.D
 Acq On : 16 Mar 2021 10:41
 Operator : SY/MD
 Sample : VV0316WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK70

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM031321WMA.M

Title : VOC Analysis

Signal : TIC: VV020619.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	97	rVB	277310	274611	15.37%	1.999%
2	1.568	158	164	173	rBV	222547	235884	13.20%	1.717%
3	2.108	323	332	354	rVB	425415	659865	36.93%	4.803%
4	2.741	522	529	530	rBV7	4588	4497	0.25%	0.033%
5	3.008	610	612	614	rBV3	3597	2046	0.11%	0.015%
6	3.060	626	628	631	rBV4	3282	2324	0.13%	0.017%
7	3.301	699	703	706	rBV5	3574	3360	0.19%	0.024%
8	3.654	811	813	817	rBV5	5528	3438	0.19%	0.025%
9	3.889	876	886	914	rBV2	126978	365670	20.47%	2.662%
10	4.349	1017	1029	1050	rVB2	290975	688207	38.52%	5.010%
11	4.728	1144	1147	1148	rBV3	2787	1797	0.10%	0.013%
12	4.841	1181	1182	1184	rBV2	2784	1596	0.09%	0.012%
13	4.886	1194	1196	1198	rBV3	2702	1571	0.09%	0.011%
14	4.905	1198	1202	1205	rVV6	4323	4162	0.23%	0.030%
15	5.050	1231	1247	1267	rBV2	701778	1786722	100.00%	13.006%
16	5.400	1353	1356	1359	rVB5	5694	3142	0.18%	0.023%
17	5.423	1361	1363	1365	rBV3	5219	3101	0.17%	0.023%
18	5.500	1385	1387	1388	rBV2	3746	1738	0.10%	0.013%
19	5.619	1412	1424	1445	rBV	578271	1138243	63.71%	8.286%
20	6.027	1545	1551	1553	rBV6	4784	5515	0.31%	0.040%
21	6.072	1553	1565	1585	rVV2	413101	836469	46.82%	6.089%
22	6.359	1650	1654	1655	rBV4	3229	2238	0.13%	0.016%
23	6.728	1767	1769	1772	rVB4	4142	1663	0.09%	0.012%
24	6.989	1841	1850	1870	rBV	214556	375224	21.00%	2.731%
25	7.230	1922	1925	1928	rBV5	4383	3773	0.21%	0.027%
26	7.320	1941	1953	1969	rBV	810684	1386465	77.60%	10.093%
27	7.625	2039	2048	2067	rBV	154438	265949	14.88%	1.936%
28	7.834	2108	2113	2116	rBV7	4493	5182	0.29%	0.038%
29	7.879	2125	2127	2132	rVB6	5219	3607	0.20%	0.026%
30	7.905	2132	2135	2137	rBV4	3689	2004	0.11%	0.015%
31	8.092	2184	2193	2221	rBV2	414642	815082	45.62%	5.933%
32	8.857	2421	2431	2447	rBV	884475	1420892	79.53%	10.343%
33	9.561	2647	2650	2652	rBV4	3108	1908	0.11%	0.014%
34	9.683	2686	2688	2690	rBV3	3565	1467	0.08%	0.011%
35	9.696	2690	2692	2697	rVB5	4818	3545	0.20%	0.026%
36	9.899	2751	2755	2757	rBV5	6290	5771	0.32%	0.042%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031621\
 Data File : VV020619.D
 Acq On : 16 Mar 2021 10:41
 Operator : SY/MD
 Sample : VV0316WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK70

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM031321WMA.M

Title : VOC Analysis

37	10.220	2846	2855	2871	rVB	470916	737274	41.26%	5.367%
38	10.503	2938	2943	2944	rBV5	4605	3440	0.19%	0.025%
39	10.760	3020	3023	3024	rBV3	2984	1946	0.11%	0.014%
40	10.905	3066	3068	3069	rBV2	2382	1214	0.07%	0.009%
41	11.255	3166	3177	3190	rBV	876317	1337780	74.87%	9.738%
42	11.561	3270	3272	3274	rBV3	3058	1754	0.10%	0.013%
43	11.628	3283	3293	3310	rVB	816807	1267102	70.92%	9.224%
44	11.718	3319	3321	3323	rBV3	3866	1599	0.09%	0.012%
45	11.799	3344	3346	3347	rBV2	2885	1401	0.08%	0.010%
46	11.892	3373	3375	3380	rVB6	3801	2716	0.15%	0.020%
47	12.120	3443	3446	3451	rVB7	4557	3099	0.17%	0.023%
48	12.149	3451	3455	3456	rBV4	3943	3015	0.17%	0.022%
49	12.374	3523	3525	3526	rBV2	3814	1551	0.09%	0.011%
50	12.551	3576	3580	3581	rBV4	3683	2614	0.15%	0.019%
51	12.706	3626	3628	3631	rVB4	2157	820	0.05%	0.006%
52	12.770	3643	3648	3650	rBV6	5217	4184	0.23%	0.030%
53	12.979	3711	3713	3716	rBV4	3847	2706	0.15%	0.020%
54	13.059	3736	3738	3743	rBV5	3291	2472	0.14%	0.018%
55	13.143	3762	3764	3766	rBV3	3518	1485	0.08%	0.011%
56	13.397	3837	3843	3847	rBV9	4983	5926	0.33%	0.043%
57	13.490	3870	3872	3875	rVB4	5322	2469	0.14%	0.018%
58	13.673	3927	3929	3930	rBV2	2677	1393	0.08%	0.010%
59	13.709	3938	3940	3943	rBV4	2985	1787	0.10%	0.013%
60	13.924	4006	4007	4008	rBV	3120	954	0.05%	0.007%
61	14.033	4036	4041	4045	rBV6	3625	4794	0.27%	0.035%
62	14.140	4072	4074	4077	rBV4	2877	1492	0.08%	0.011%
63	14.387	4147	4151	4152	rBV4	3095	1770	0.10%	0.013%
64	14.545	4197	4200	4202	rBV4	4923	3413	0.19%	0.025%
65	14.696	4244	4247	4250	rVB5	3558	2471	0.14%	0.018%
66	14.844	4290	4293	4298	rVB7	4618	3672	0.21%	0.027%
67	15.043	4353	4355	4358	rBV4	3745	2443	0.14%	0.018%
68	15.172	4393	4395	4397	rBV3	2157	1078	0.06%	0.008%
69	15.223	4409	4411	4415	rBV5	3817	3019	0.17%	0.022%
70	15.403	4465	4467	4468	rBV2	3990	1713	0.10%	0.012%
71	16.361	4763	4765	4767	rBV3	3292	1908	0.11%	0.014%




Sum of corrected areas: 13737202

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031621\
Data File : VV020619.D
Acq On : 16 Mar 2021 10:41
Operator : SY/MD
Sample : VV0316WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
VBLK70

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM031321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

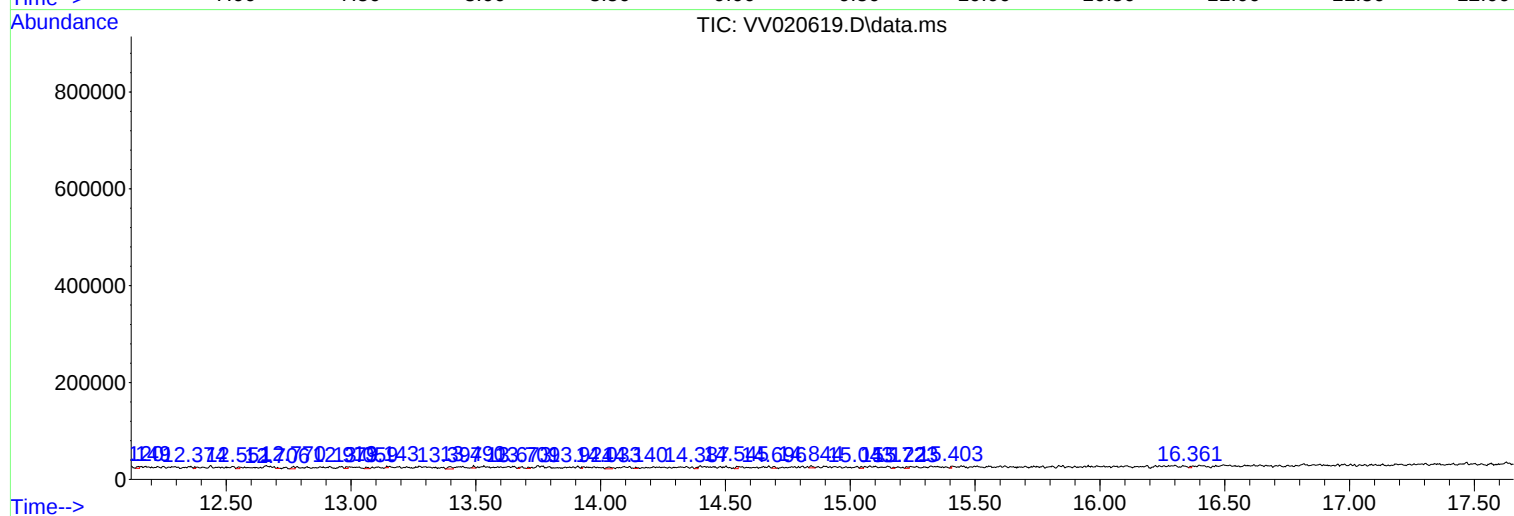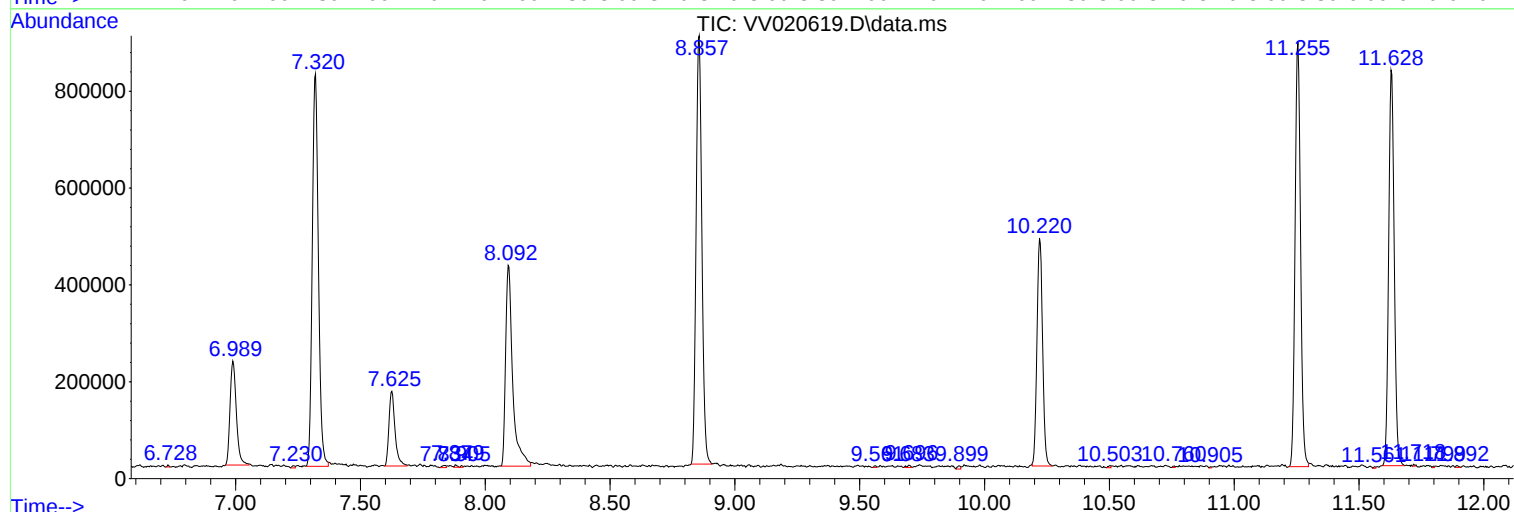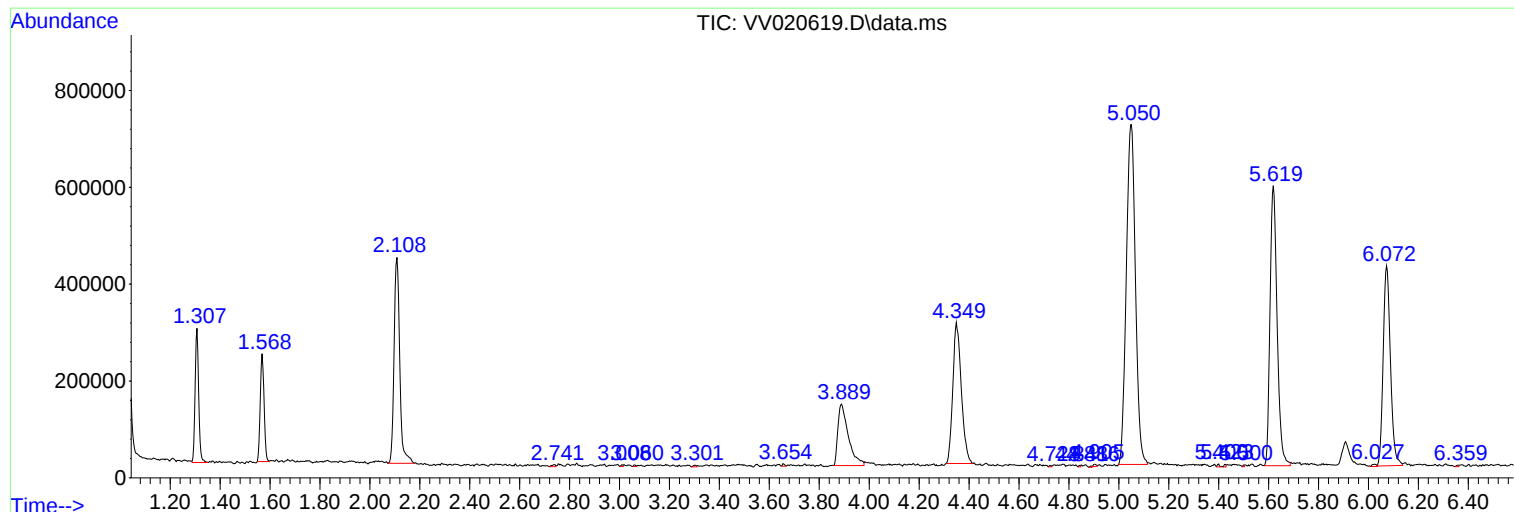

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031621\
Data File : VV020619.D
Acq On : 16 Mar 2021 10:41
Operator : SY/MD
Sample : VV0316WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK70

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM031321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031621\
Data File : VV020619.D
Acq On : 16 Mar 2021 10:41
Operator : SY/MD
Sample : VV0316WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK70

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM031321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
