

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031621\
 Data File : VV020636.D
 Acq On : 16 Mar 2021 17:24
 Operator : SY/MD
 Sample : M1675-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BE8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM031321WMA.M

Title : VOC Analysis

Signal : TIC: VV020636.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	78	83	97	rVB	199066	206444	11.46%	1.396%
2	1.571	158	165	175	rBV	190305	216325	12.00%	1.463%
3	2.111	324	333	353	rVB2	384150	625657	34.72%	4.232%
4	2.455	437	440	443	rBV5	3801	3033	0.17%	0.021%
5	2.523	459	461	463	rBV2	3740	2072	0.11%	0.014%
6	2.716	519	521	525	rVB5	3791	2189	0.12%	0.015%
7	2.773	534	539	543	rVB7	5489	4412	0.24%	0.030%
8	2.999	606	609	614	rVB7	4680	3748	0.21%	0.025%
9	3.034	618	620	622	rBV3	3046	1794	0.10%	0.012%
10	3.089	633	637	639	rBV5	3438	2545	0.14%	0.017%
11	3.182	658	666	668	rBV9	5408	8163	0.45%	0.055%
12	3.317	706	708	712	rBV5	2463	1928	0.11%	0.013%
13	3.500	757	765	767	rBV8	2697	3252	0.18%	0.022%
14	3.564	779	785	790	rBV9	4260	5616	0.31%	0.038%
15	3.590	790	793	797	rVB5	3701	2363	0.13%	0.016%
16	3.896	877	888	918	rBV2	131818	450733	25.01%	3.049%
17	4.201	977	983	986	rBV8	4880	5632	0.31%	0.038%
18	4.352	1014	1030	1052	rBV2	272779	682031	37.85%	4.613%
19	4.529	1081	1085	1086	rBV4	6210	4383	0.24%	0.030%
20	4.687	1132	1134	1137	rBV4	3014	1665	0.09%	0.011%
21	4.719	1142	1144	1147	rBV4	3089	1566	0.09%	0.011%
22	5.050	1231	1247	1267	rBV2	642798	1627888	90.34%	11.010%
23	5.535	1395	1398	1400	rBV4	2884	1561	0.09%	0.011%
24	5.619	1413	1424	1446	rBV	532008	1052157	58.39%	7.116%
25	5.915	1504	1516	1541	rVB2	891224	1801970	100.00%	12.188%
26	6.072	1554	1565	1587	rVB	386553	778930	43.23%	5.268%
27	6.252	1618	1621	1623	rBV4	4817	3433	0.19%	0.023%
28	6.641	1739	1742	1747	rBV7	4445	3923	0.22%	0.027%
29	6.989	1840	1850	1869	rBV2	193275	353465	19.62%	2.391%
30	7.320	1942	1953	1971	rBV	713269	1203251	66.77%	8.138%
31	7.625	2039	2048	2065	rBV	137666	231928	12.87%	1.569%
32	7.905	2133	2135	2138	rBV3	3391	2090	0.12%	0.014%
33	8.027	2169	2173	2174	rBV3	3720	3003	0.17%	0.020%
34	8.092	2184	2193	2219	rBV2	429849	839073	46.56%	5.675%
35	8.452	2303	2305	2308	rBV3	3944	1632	0.09%	0.011%
36	8.651	2365	2367	2370	rBV4	3459	2263	0.13%	0.015%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031621\
 Data File : VV020636.D
 Acq On : 16 Mar 2021 17:24
 Operator : SY/MD
 Sample : M1675-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BE8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM031321WMA.M
 Title : VOC Analysis

37	8.773	2403	2405	2408	rBV3	3793	2284	0.13%	0.015%
38	8.857	2420	2431	2444	rBV	833271	1342593	74.51%	9.081%
39	9.191	2531	2535	2539	rBV7	6070	5280	0.29%	0.036%
40	9.262	2552	2557	2560	rBV6	4680	4619	0.26%	0.031%
41	9.374	2590	2592	2595	rBV4	3151	2489	0.14%	0.017%
42	9.555	2645	2648	2650	rBV4	3519	2270	0.13%	0.015%
43	9.577	2653	2655	2661	rVB7	3300	2629	0.15%	0.018%
44	9.651	2675	2678	2680	rBV4	3095	1969	0.11%	0.013%
45	9.908	2755	2758	2761	rBV4	5317	4548	0.25%	0.031%
46	10.001	2783	2787	2788	rVB3	3240	1859	0.10%	0.013%
47	10.053	2799	2803	2807	rBV6	2946	2914	0.16%	0.020%
48	10.075	2808	2810	2813	rVB4	3940	2059	0.11%	0.014%
49	10.098	2813	2817	2823	rBV9	2459	3109	0.17%	0.021%
50	10.182	2839	2843	2844	rBV4	6533	4308	0.24%	0.029%
51	10.220	2845	2855	2872	rVB	468295	742919	41.23%	5.025%
52	10.365	2893	2900	2903	rBV8	5202	7469	0.41%	0.051%
53	10.590	2968	2970	2974	rVB5	3492	2203	0.12%	0.015%
54	10.686	2993	3000	3002	rBV7	5017	6280	0.35%	0.042%
55	10.847	3047	3050	3053	rBV5	3664	2710	0.15%	0.018%
56	10.940	3077	3079	3082	rBV4	3361	2004	0.11%	0.014%
57	11.117	3133	3134	3137	rBV3	3619	1991	0.11%	0.013%
58	11.255	3166	3177	3194	rBV	797825	1207635	67.02%	8.168%
59	11.522	3258	3260	3263	rBV3	4912	3278	0.18%	0.022%
60	11.590	3278	3281	3282	rBV3	3226	1578	0.09%	0.011%
61	11.632	3283	3294	3309	rVB	752266	1176644	65.30%	7.958%
62	11.786	3338	3342	3344	rBV5	2510	2245	0.12%	0.015%
63	11.960	3391	3396	3400	rBV7	5256	4720	0.26%	0.032%
64	12.040	3418	3421	3424	rBV5	2924	1735	0.10%	0.012%
65	12.066	3426	3429	3433	rVB6	3934	3278	0.18%	0.022%
66	12.088	3433	3436	3437	rBV3	3005	1593	0.09%	0.011%
67	12.136	3447	3451	3453	rBV5	3093	2009	0.11%	0.014%
68	12.255	3484	3488	3491	rBV5	4271	3294	0.18%	0.022%
69	12.278	3492	3495	3497	rVV4	3257	1837	0.10%	0.012%
70	12.304	3500	3503	3505	rBV4	3048	2177	0.12%	0.015%
71	12.352	3515	3518	3521	rVB5	4065	2658	0.15%	0.018%
72	12.384	3521	3528	3532	rBV9	4273	5583	0.31%	0.038%
73	12.490	3557	3561	3563	rBV5	2899	2779	0.15%	0.019%
74	12.686	3619	3622	3624	rBV4	3554	2558	0.14%	0.017%
75	12.853	3672	3674	3679	rBV6	4941	4491	0.25%	0.030%
76	12.911	3690	3692	3696	rBV5	3453	2322	0.13%	0.016%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031621\
 Data File : VV020636.D
 Acq On : 16 Mar 2021 17:24
 Operator : SY/MD
 Sample : M1675-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BE8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM031321WMA.M

Title : VOC Analysis

77	13.021	3722	3726	3728	rBV5	3037	2647	0.15%	0.018%
78	13.117	3752	3756	3757	rBV4	3987	2173	0.12%	0.015%
79	13.181	3773	3776	3777	rBV3	3274	1959	0.11%	0.013%
80	13.236	3788	3793	3795	rBV6	4053	3666	0.20%	0.025%
81	13.265	3800	3802	3806	rVB5	4461	2195	0.12%	0.015%
82	13.339	3823	3825	3828	rVB4	4712	2048	0.11%	0.014%
83	13.480	3866	3869	3870	rBV2	3757	1630	0.09%	0.011%
84	13.606	3905	3908	3909	rBV3	2722	1755	0.10%	0.012%
85	13.667	3924	3927	3931	rVB5	3140	2192	0.12%	0.015%
86	13.722	3942	3944	3947	rBV4	2815	2061	0.11%	0.014%
87	13.976	4019	4023	4025	rBV5	2698	2435	0.14%	0.016%
88	14.021	4034	4037	4040	rBV5	2341	1646	0.09%	0.011%
89	14.651	4229	4233	4234	rBV4	4466	2959	0.16%	0.020%
90	14.902	4306	4311	4313	rBV5	3372	2804	0.16%	0.019%
91	14.979	4333	4335	4339	rBV5	3676	2942	0.16%	0.020%
92	15.004	4341	4343	4345	rBV3	3664	1871	0.10%	0.013%
93	15.056	4355	4359	4361	rBV4	3929	2524	0.14%	0.017%
94	15.107	4372	4375	4378	rBV5	3549	2907	0.16%	0.020%
95	15.143	4384	4386	4388	rBV3	4352	2139	0.12%	0.014%
96	15.188	4395	4400	4403	rBV5	4872	4948	0.27%	0.033%
97	15.374	4455	4458	4459	rBV2	2964	1535	0.09%	0.010%
98	15.558	4513	4515	4517	rBV3	3505	2290	0.13%	0.015%
99	15.660	4543	4547	4550	rBV5	4493	3496	0.19%	0.024%
100	16.747	4880	4885	4887	rBV6	5511	5417	0.30%	0.037%




Sum of corrected areas: 14785277

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031621\
Data File : VV020636.D
Acq On : 16 Mar 2021 17:24
Operator : SY/MD
Sample : M1675-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
C0BE8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM031321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

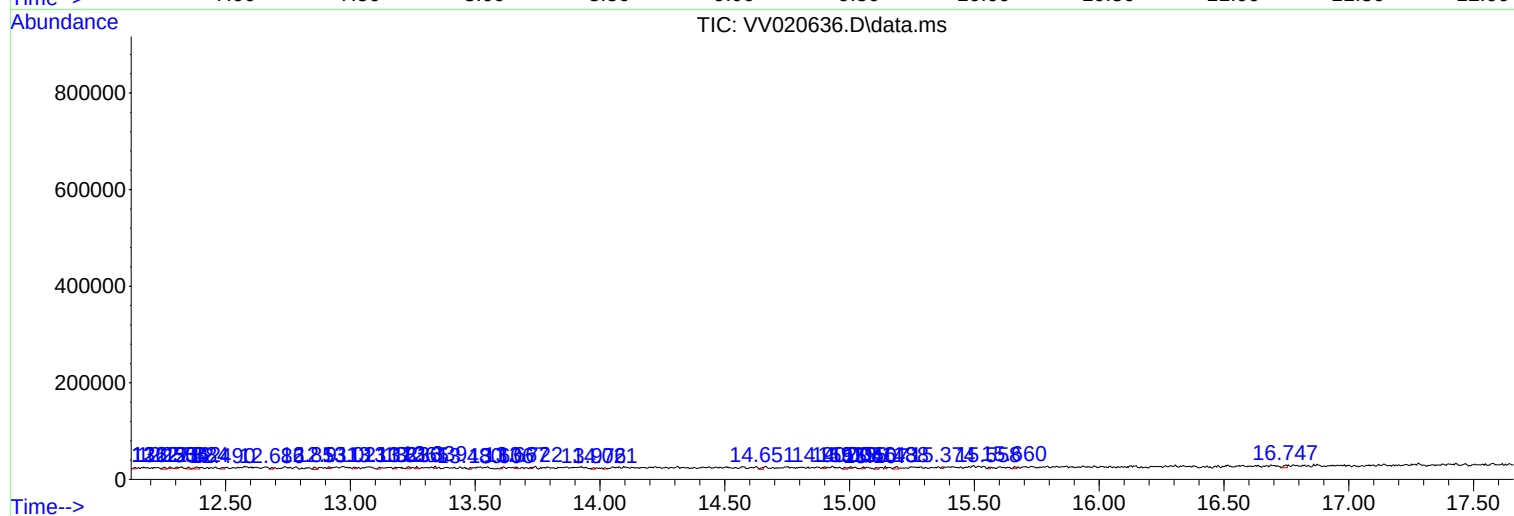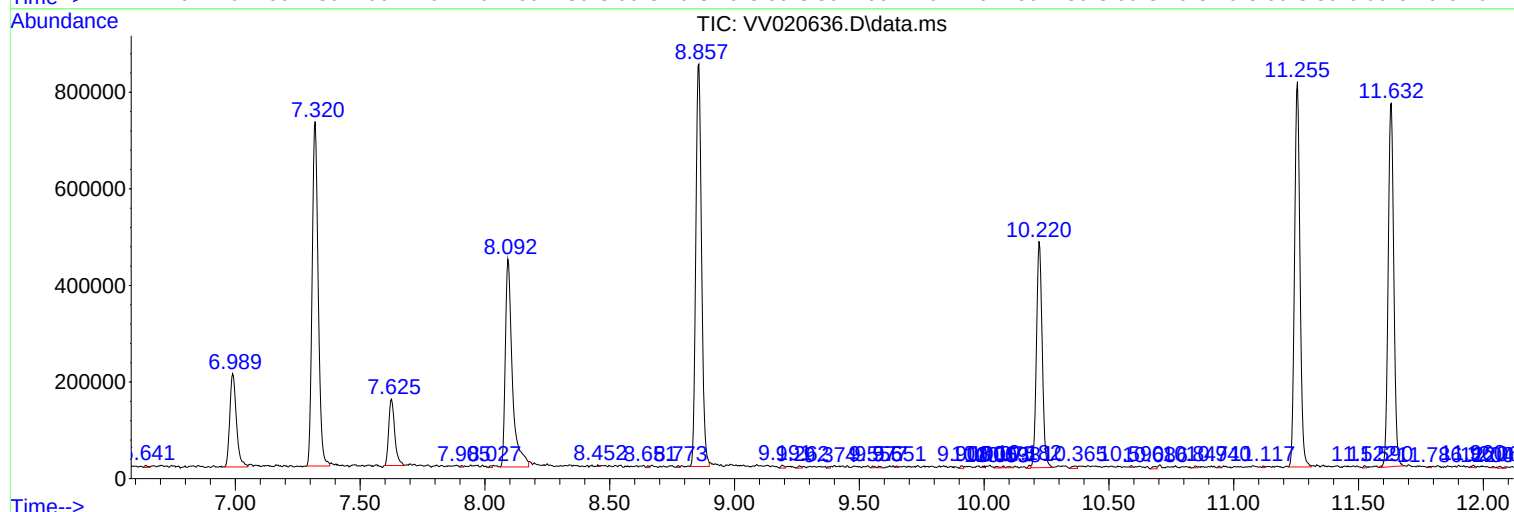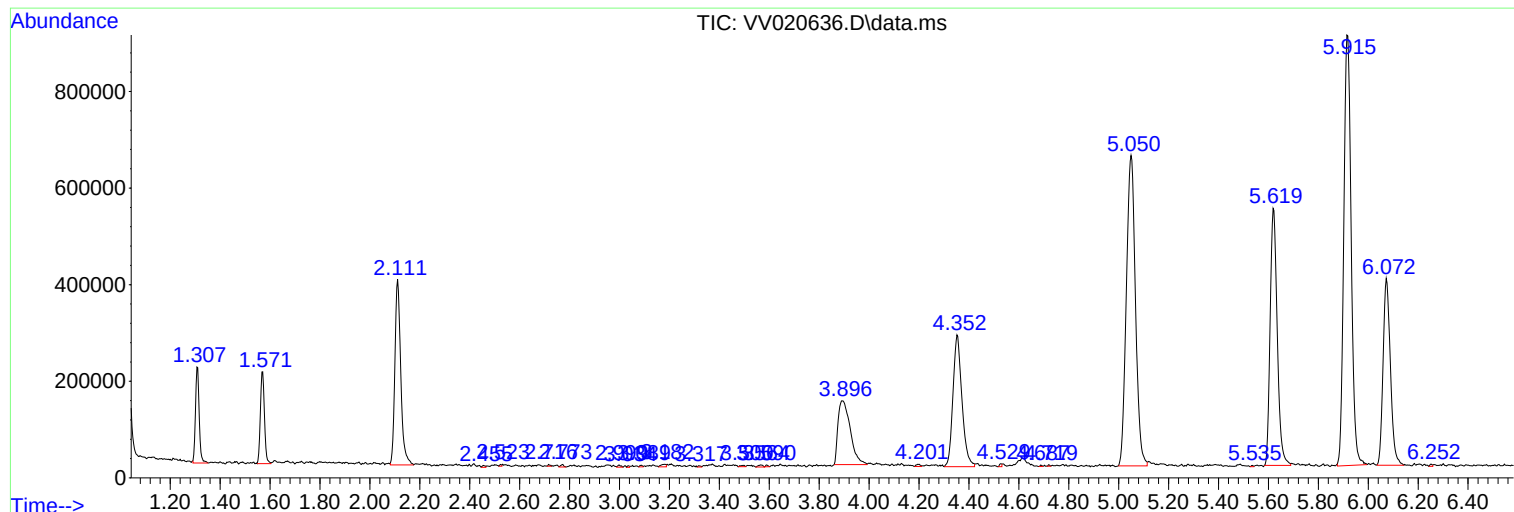

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031621\
Data File : VV020636.D
Acq On : 16 Mar 2021 17:24
Operator : SY/MD
Sample : M1675-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BE8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM031321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031621\
Data File : VV020636.D
Acq On : 16 Mar 2021 17:24
Operator : SY/MD
Sample : M1675-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BE8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM031321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
