




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031623\
 Data File : VV030220.D
 Acq On : 16 Mar 2023 13:23
 Operator : SY/MD
 Sample : 01884-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CB927

Manual IntegrationsAPPROVED

Quant Time: Mar 17 05:48:00 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Mar 17 05:46:57 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 03/17/2023
 Supervised By :Mahesh Dadoda 03/17/2023

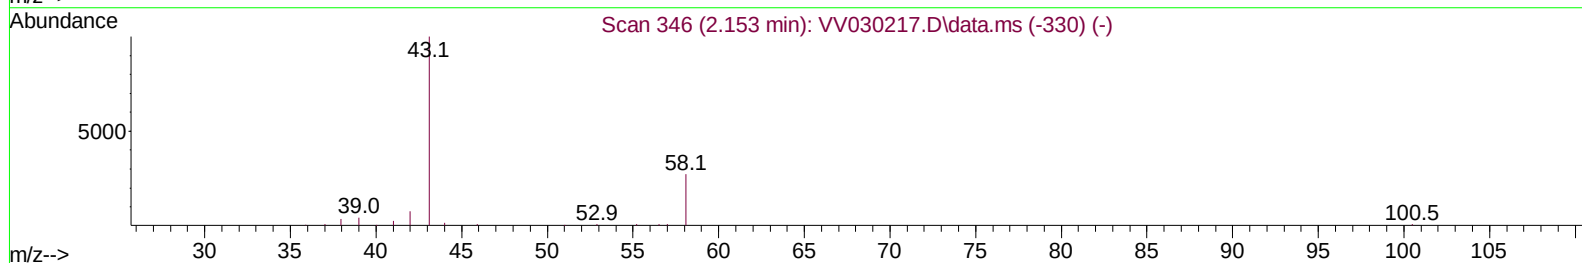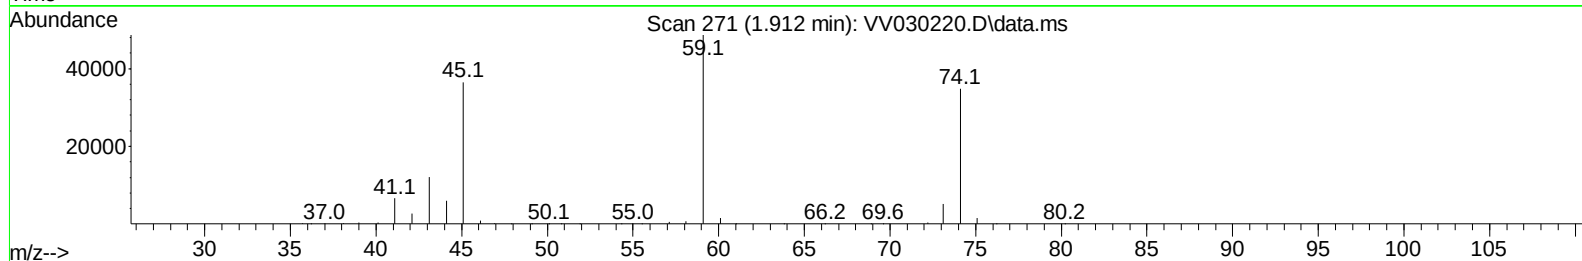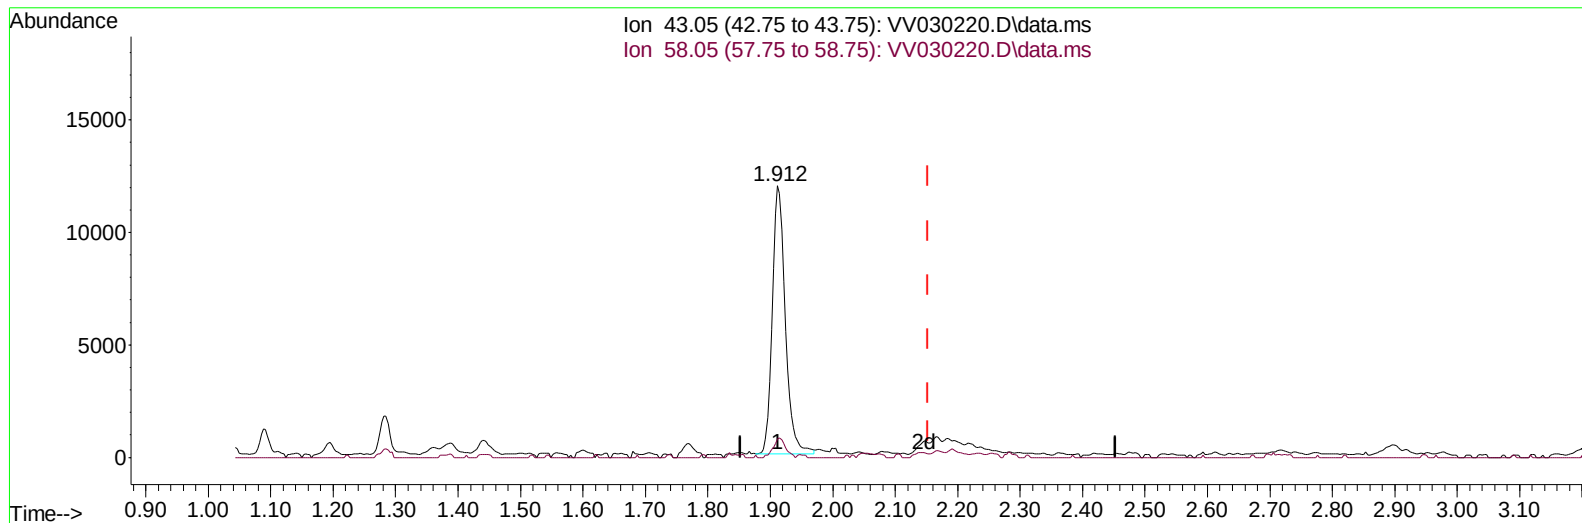

TIC: VV030220.D\data.ms

(13) Acetone (T)

1.912min (-0.241) 15.81 ug/L

response 17204

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	14.70	6.86
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031623\
 Data File : VV030220.D
 Acq On : 16 Mar 2023 13:23
 Operator : SY/MD
 Sample : 01884-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CB927

Manual IntegrationsAPPROVED

Quant Time: Mar 17 05:48:00 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Mar 17 05:46:57 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 03/17/2023
 Supervised By :Mahesh Dadoda 03/17/2023

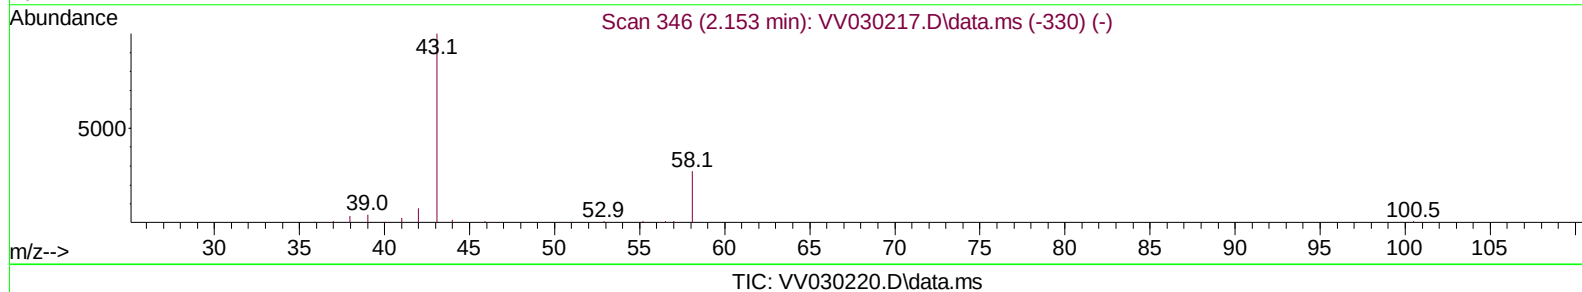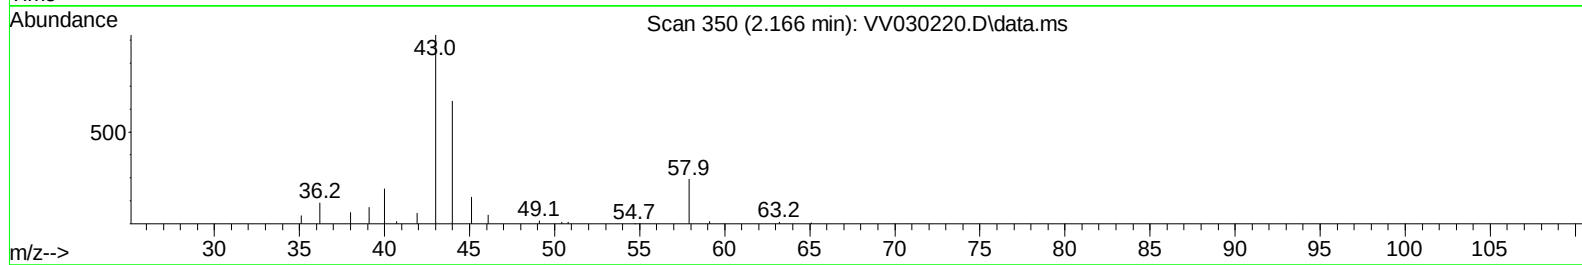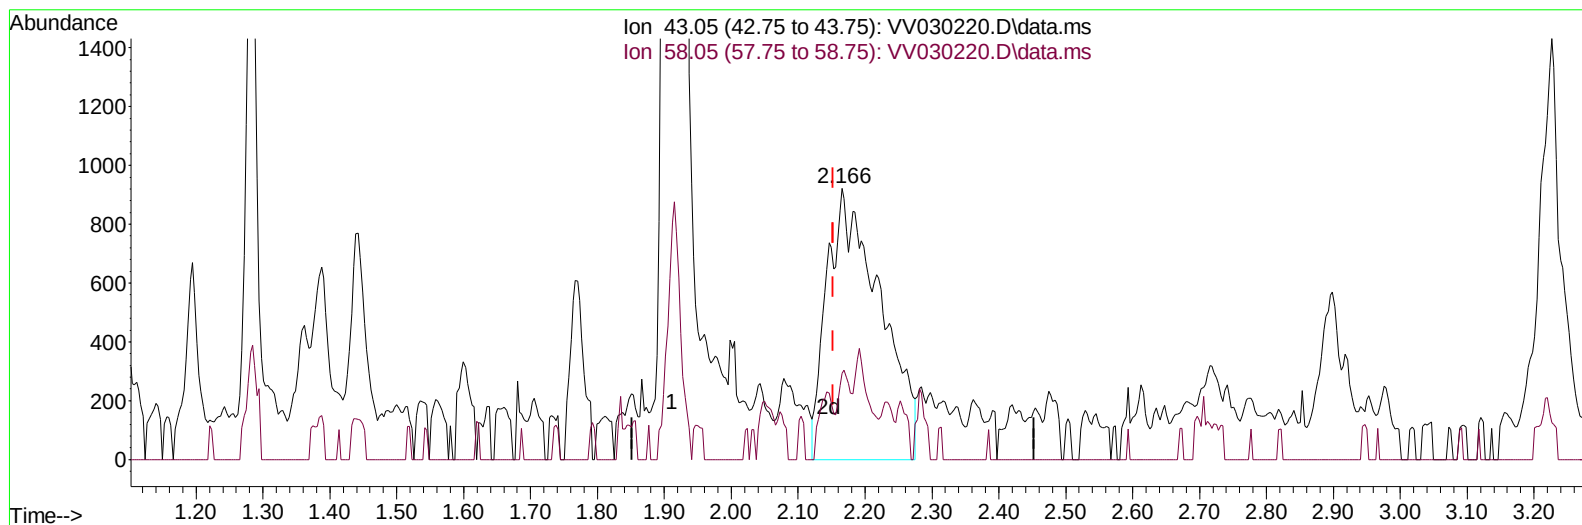

(13) Acetone (T)

2.166min (+ 0.013) 4.66 ug/L m

response 5069

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	14.70	23.30
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031623\
 Data File : VV030220.D
 Acq On : 16 Mar 2023 13:23
 Operator : SY/MD
 Sample : 01884-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CB927

Manual IntegrationsAPPROVED

Quant Time: Mar 17 05:48:00 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Mar 17 05:46:57 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 03/17/2023
 Supervised By :Mahesh Dadoda 03/17/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.545	114		123451	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.792	117		119571	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152		71515	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.281	65		34399	4.306	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	86.200%	
7) Chloroethane-d5	1.535	69		31776	4.238	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	84.800%	
11) 1,1-Dichloroethene-d2	2.063	63		55556	3.383	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	67.600%	
20) 2-Butanone-d5	3.838	46		66626	45.240	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	90.480%	
24) Chloroform-d	4.259	84		73302	4.492	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.800%	
26) 1,2-Dichloroethane-d4	4.956	65		35247	5.291	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	105.800%	
32) Benzene-d6	4.969	84		131500	4.087	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	81.800%	
36) 1,2-Dichloropropane-d6	5.998	67		41819	4.320	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	86.400%	
41) Toluene-d8	7.252	98		119386	3.915	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	78.200%	
43) trans-1,3-Dichloroprop...	7.561	79		14380	4.342	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	86.800%	
46) 2-Hexanone-d5	8.037	63		60078	43.851	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	87.700%	
56) 1,1,2,2-Tetrachloroeth...	10.162	84		31878	4.629	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	92.600%	
66) 1,2-Dichlorobenzene-d4	11.570	152		51234	4.234	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	84.600%	
Target Compounds							
						Qvalue	
13) Acetone	2.166	43		5069m	4.657	ug/L	
22) cis-1,2-Dichloroethene	3.828	96		1321	0.152	ug/L	91
30) Cyclohexane	4.593	56		3118	0.257	ug/L	97
33) Benzene	5.027	78		5989	0.183	ug/L	100
35) Methylcyclohexane	6.056	83		3457	0.250	ug/L #	78
42) Toluene	7.329	91		10407	0.294	ug/L	98
51) Chlorobenzene	8.821	112		362141	15.182	ug/L	98
52) Ethylbenzene	8.960	91		2167	0.056	ug/L	94
53) m,p-Xylene	9.082	106		2515	0.170	ug/L	96
54) o-Xylene	9.490	106		2287	0.162	ug/L	88
60) Isopropylbenzene	9.876	105		47086	1.144	ug/L	98
64) 1,3-Dichlorobenzene	11.130	146		1610	0.075	ug/L #	91
65) 1,4-Dichlorobenzene	11.217	146		47032	2.176	ug/L	95
67) 1,2-Dichlorobenzene	11.590	146		4539	0.240	ug/L #	83

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031623\
Data File : VV030220.D
Acq On : 16 Mar 2023 13:23
Operator : SY/MD
Sample : 01884-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CB927

Manual IntegrationsAPPROVED

Quant Time: Mar 17 05:48:00 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Mar 17 05:46:57 2023
Response via : Initial Calibration

Reviewed By :Krupa Patel 03/17/2023
Supervised By :Mahesh Dadoda 03/17/2023

