

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW031623\
 Data File : VW030222.D
 Acq On : 16 Mar 2023 14:57
 Operator : SY/MD
 Sample : 01947-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CB941

Quant Time: Mar 17 05:48:35 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Mar 17 05:46:57 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.539	114	152101	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.792	117	145832	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	76206	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.282	65	37228	3.783	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	75.600%
7) Chloroethane-d5	1.536	69	33424	3.618	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	72.400%
11) 1,1-Dichloroethene-d2	2.063	63	58150	2.874	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	57.400%#
20) 2-Butanone-d5	3.812	46	75756	41.750	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	83.500%
24) Chloroform-d	4.256	84	73876	3.675	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	73.400%
26) 1,2-Dichloroethane-d4	4.950	65	36380	4.433	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.600%
32) Benzene-d6	4.966	84	136493	3.478	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	69.600%#
36) 1,2-Dichloropropane-d6	5.995	67	42086	3.565	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	71.400%
41) Toluene-d8	7.249	98	120219	3.232	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	64.600%#
43) trans-1,3-Dichloroprop...	7.561	79	15278	3.783	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	75.600%
46) 2-Hexanone-d5	8.034	63	57768	34.572	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	69.140%
56) 1,1,2,2-Tetrachloroeth...	10.162	84	29321	3.491	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	69.800%
66) 1,2-Dichlorobenzene-d4	11.570	152	44950	3.486	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	69.800%#
Target Compounds					Qvalue	
13) Acetone	2.146	43	4265	3.180	ug/L	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031623\
Data File : VV030222.D
Acq On : 16 Mar 2023 14:57
Operator : SY/MD
Sample : 01947-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CB941

Quant Time: Mar 17 05:48:35 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Mar 17 05:46:57 2023
Response via : Initial Calibration

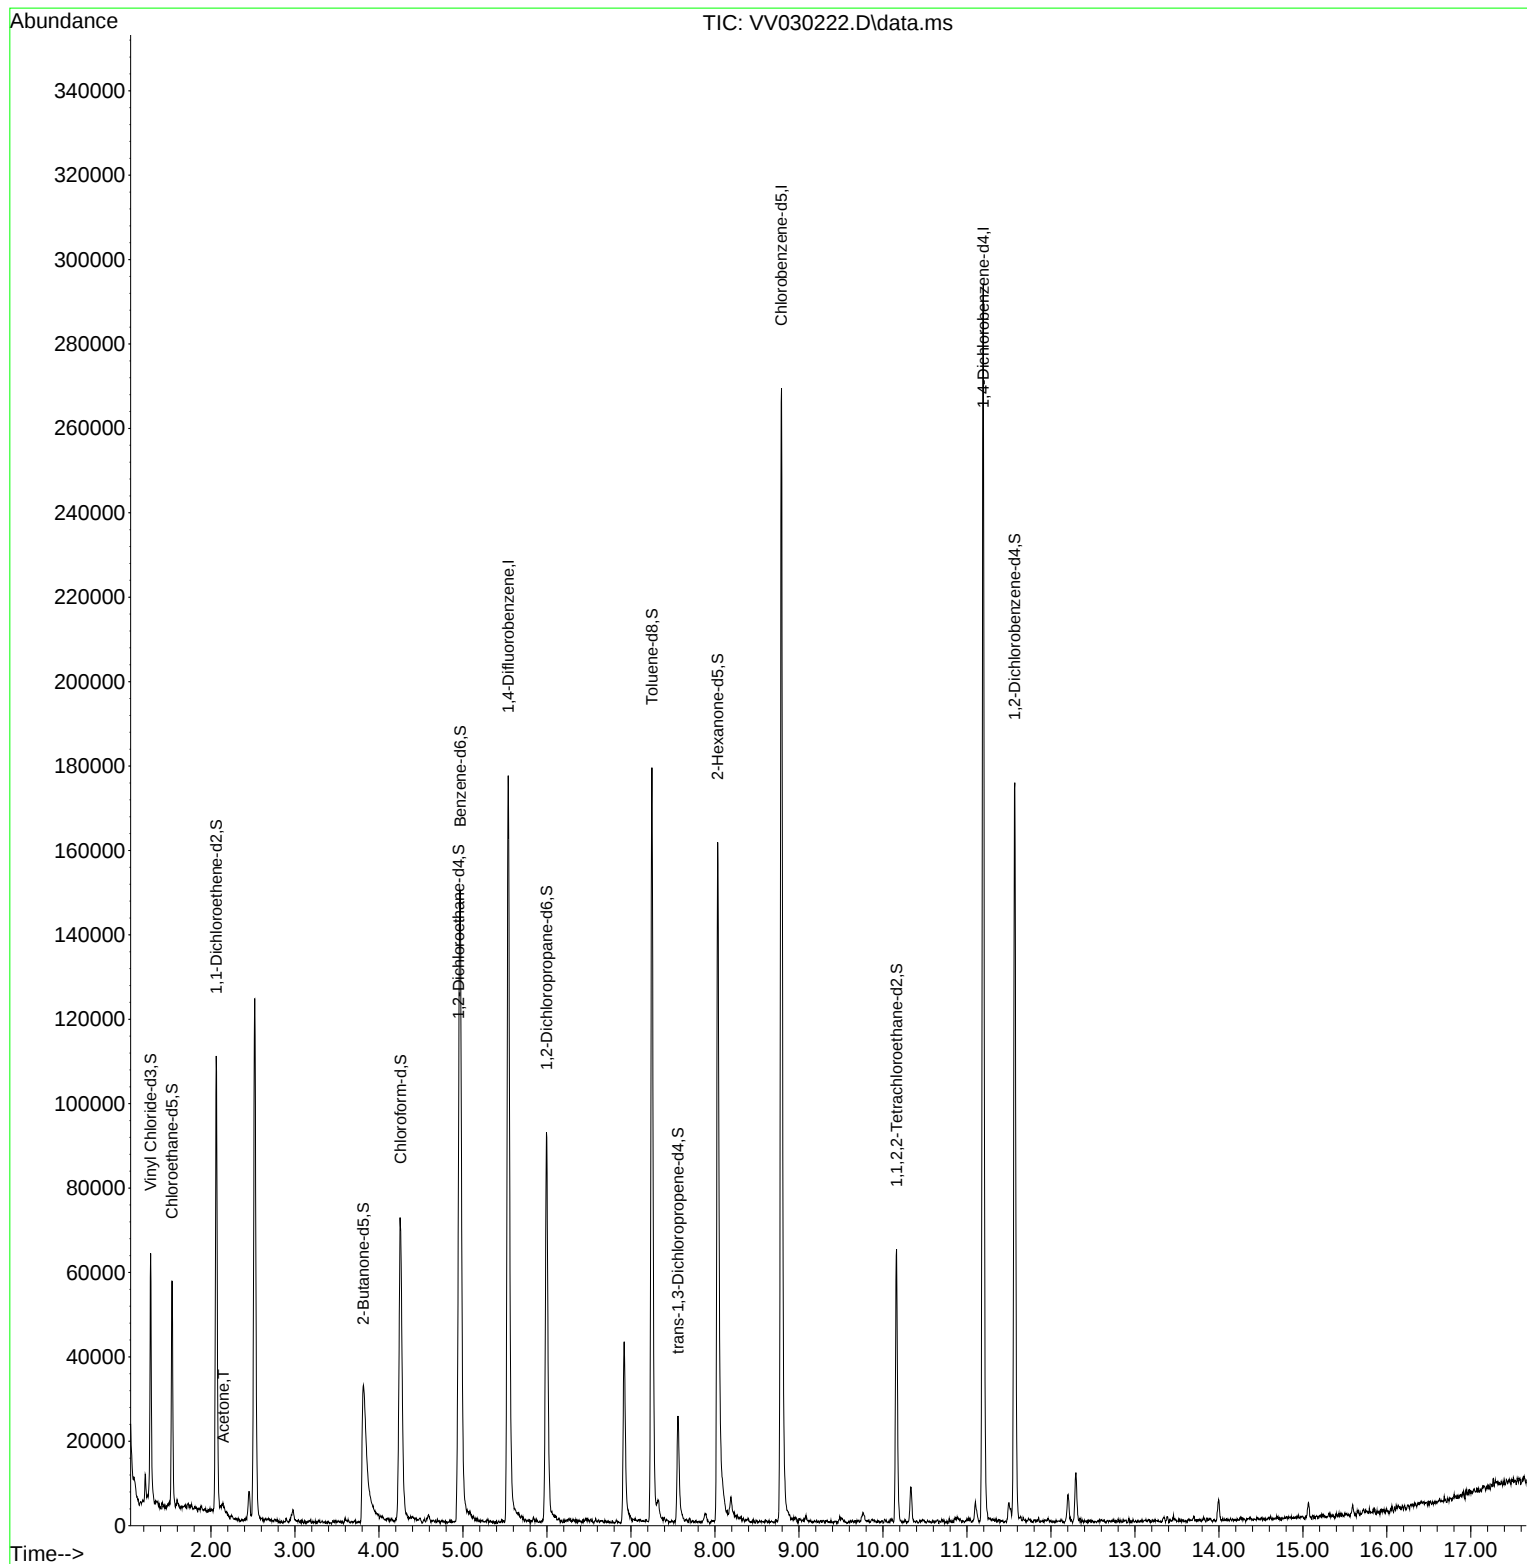

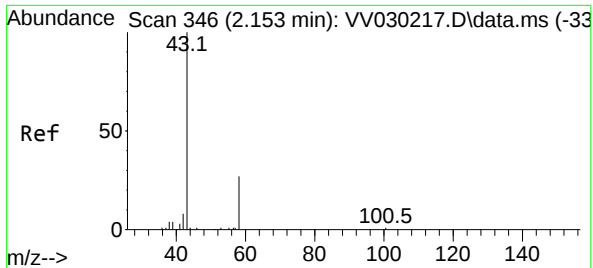

#13
 Acetone
 Concen: 3.180 ug/L
 RT: 2.146 min Scan# 34
 Delta R.T. -0.006 min
 Lab File: VV030222.D
 Acq: 16 Mar 2023 14:57

Instrument :
 MSVOA_V
 ClientSampleId :
 CB941

Tgt Ion: 43 Resp: 4265
 Ion Ratio Lower Upper
 43 100
 58 19.2 0.0 29.4

