

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031623\
 Data File : VV030218.D
 Acq On : 16 Mar 2023 12:29
 Operator : SY/MD
 Sample : VV0316WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK313

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV030218.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.220	51	56	62	rBV2	3705	4988	1.25%	0.147%
2	1.282	69	75	87	rVB	60199	61471	15.38%	1.814%
3	1.536	146	154	167	rVB	55772	64948	16.25%	1.917%
4	2.066	307	319	335	rBV	114571	165338	41.36%	4.880%
5	2.452	430	439	450	rBV5	4932	9478	2.37%	0.280%
6	3.834	855	869	908	rBV2	27187	136407	34.12%	4.026%
7	4.262	986	1002	1020	rBV2	73935	183314	45.86%	5.410%
8	4.969	1206	1222	1247	rBV2	153939	399764	100.00%	11.798%
9	5.542	1389	1400	1422	rBV	128312	274670	68.71%	8.106%
10	5.998	1528	1542	1561	rBV	92197	199563	49.92%	5.890%
11	6.924	1818	1830	1851	rBV	40929	84494	21.14%	2.494%
12	7.252	1920	1932	1949	rBV	181770	323495	80.92%	9.547%
13	7.561	2017	2028	2042	rBV	27079	51272	12.83%	1.513%
14	8.037	2166	2176	2202	rBV	166770	339896	85.02%	10.031%
15	8.792	2400	2411	2435	rBV	199702	339688	84.97%	10.025%
16	10.162	2827	2837	2852	rBV	67920	108791	27.21%	3.211%
17	10.333	2882	2890	2900	rVB6	3121	5098	1.28%	0.150%
18	11.194	3147	3158	3176	rBV	208080	334129	83.58%	9.861%
19	11.571	3263	3275	3296	rBV	178102	285941	71.53%	8.439%
20	12.204	3459	3472	3479	rBV2	5883	9789	2.45%	0.289%
21	13.995	4020	4029	4037	rBV2	3923	5783	1.45%	0.171%




Sum of corrected areas: 3388317

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031623\
Data File : VV030218.D
Acq On : 16 Mar 2023 12:29
Operator : SY/MD
Sample : VV0316WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK313

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

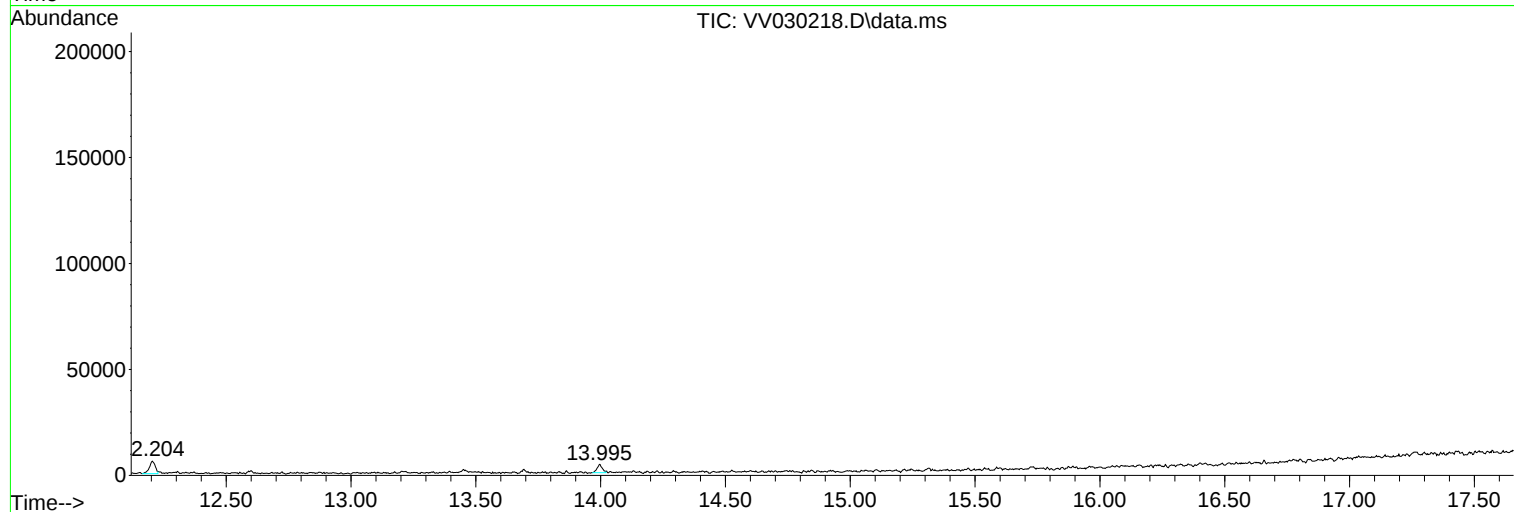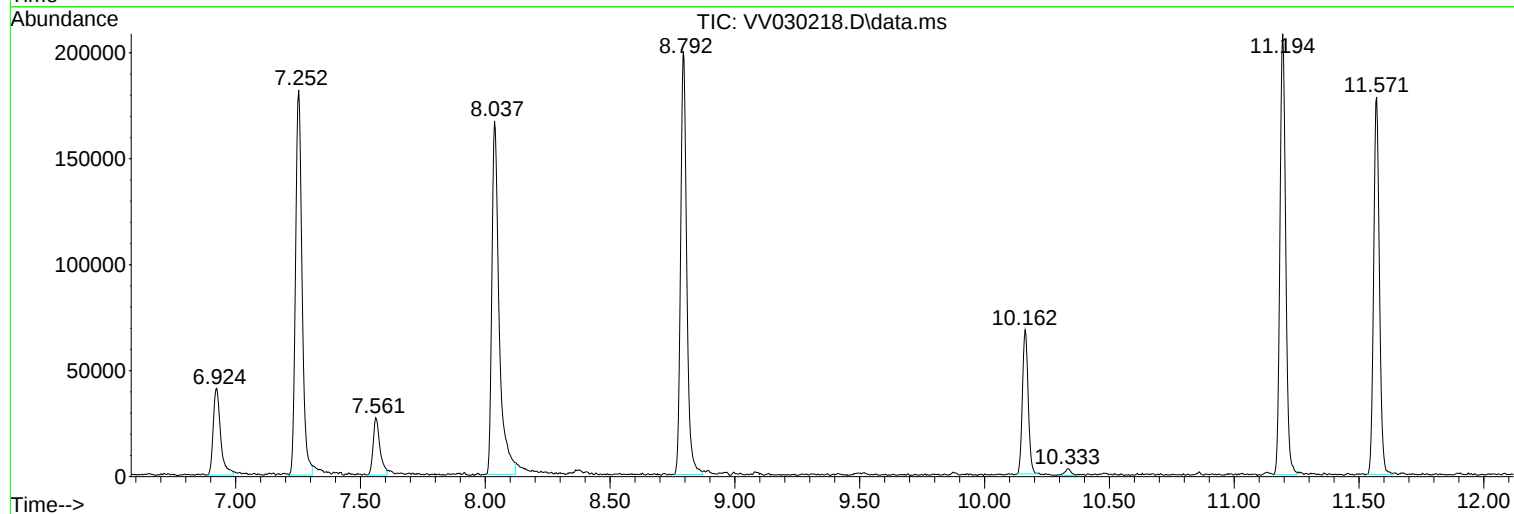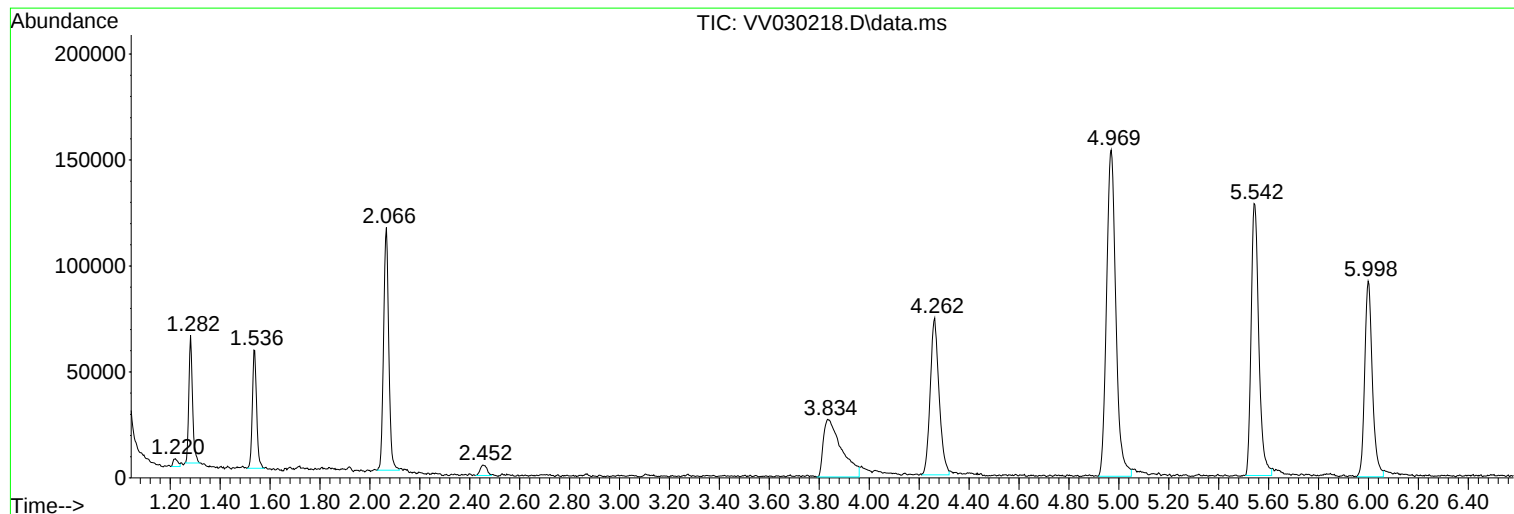

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031623\
Data File : VV030218.D
Acq On : 16 Mar 2023 12:29
Operator : SY/MD
Sample : VV0316WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK313

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031623\
Data File : VV030218.D
Acq On : 16 Mar 2023 12:29
Operator : SY/MD
Sample : VV0316WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK313

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------