

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031623\
 Data File : VV030219.D
 Acq On : 16 Mar 2023 12:58
 Operator : SY/MD
 Sample : 01884-08DL 4X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CB916DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV030219.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.114	19	23	32	rVB	15673	17303	3.30%	0.410%
2	1.191	43	47	52	rBV2	7795	6513	1.24%	0.154%
3	1.281	68	75	90	rVB	66523	73289	13.96%	1.735%
4	1.535	147	154	168	rVB	57968	68887	13.12%	1.631%
5	1.912	265	271	285	rVB	11079	16962	3.23%	0.401%
6	2.063	308	318	334	rBV	113281	167658	31.94%	3.968%
7	2.455	428	440	455	rVB2	15992	27976	5.33%	0.662%
8	3.834	854	869	898	rBV3	31812	145823	27.78%	3.452%
9	4.259	985	1001	1033	rVB	72873	192173	36.61%	4.549%
10	4.966	1201	1221	1253	rBV3	158769	430205	81.96%	10.183%
11	5.542	1388	1400	1419	rBV	135080	280770	53.49%	6.646%
12	5.998	1528	1542	1563	rBV2	94984	202538	38.59%	4.794%
13	6.921	1816	1829	1844	rBV	42681	85460	16.28%	2.023%
14	7.252	1919	1932	1949	rBV	185462	333120	63.46%	7.885%
15	7.561	2018	2028	2046	rBV3	27240	52419	9.99%	1.241%
16	8.037	2165	2176	2204	rBV	172127	351889	67.04%	8.329%
17	8.792	2400	2411	2414	rBV	220914	302607	57.65%	7.163%
18	8.821	2415	2420	2448	rVB	318614	524907	100.00%	12.424%
19	10.162	2826	2837	2851	rBV2	68924	112967	21.52%	2.674%
20	10.336	2881	2891	2899	rBV3	7538	11224	2.14%	0.266%
21	10.812	3031	3039	3046	rBV4	4297	5905	1.12%	0.140%
22	10.998	3090	3097	3107	rBV2	7914	11416	2.17%	0.270%
23	11.194	3147	3158	3180	rBV2	236160	436181	83.10%	10.324%
24	11.570	3264	3275	3294	rVB	194453	324576	61.83%	7.683%
25	12.201	3462	3471	3478	rBV5	4882	9234	1.76%	0.219%
26	12.246	3479	3485	3491	rVB4	4426	5990	1.14%	0.142%
27	12.612	3587	3599	3600	rBV7	6810	8096	1.54%	0.192%
28	13.992	4020	4028	4036	rBV2	5214	7319	1.39%	0.173%
29	16.262	4727	4734	4744	rVB4	7269	11445	2.18%	0.271%




Sum of corrected areas: 4224852

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031623\
Data File : VV030219.D
Acq On : 16 Mar 2023 12:58
Operator : SY/MD
Sample : 01884-08DL 4X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CB916DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

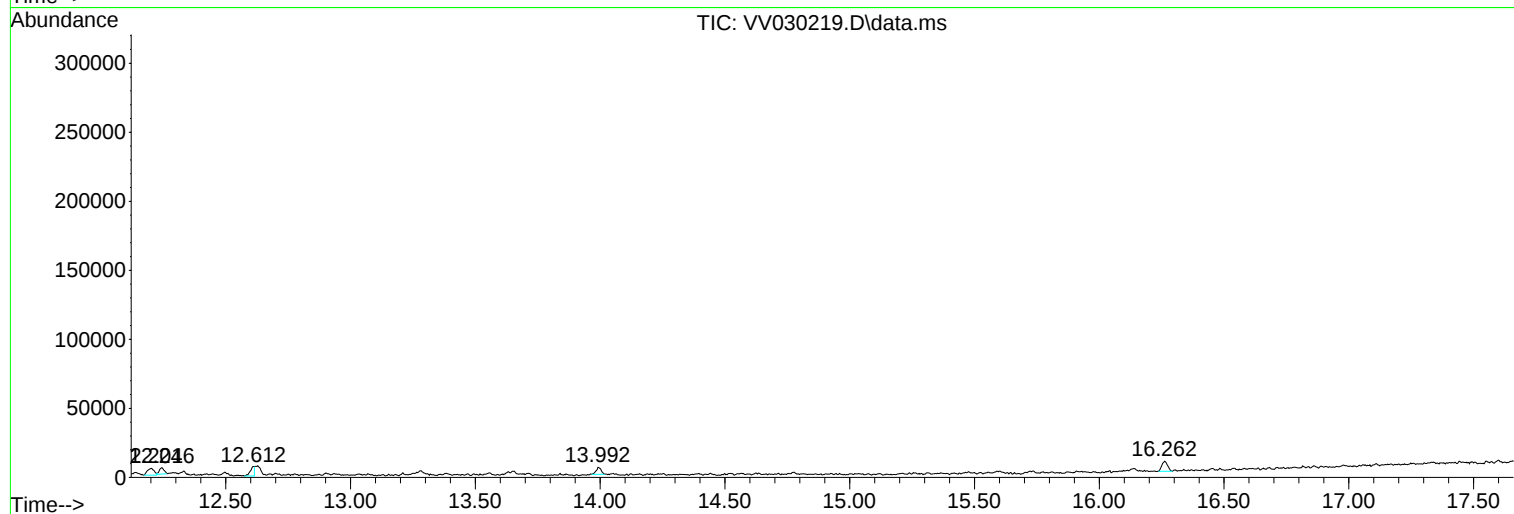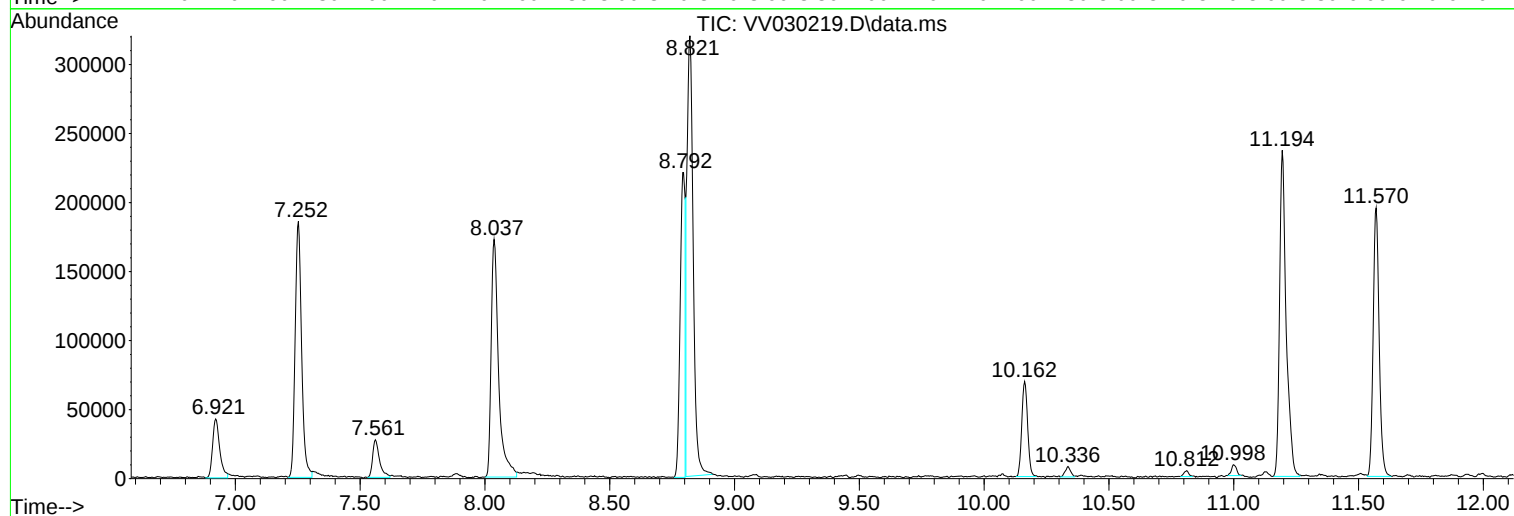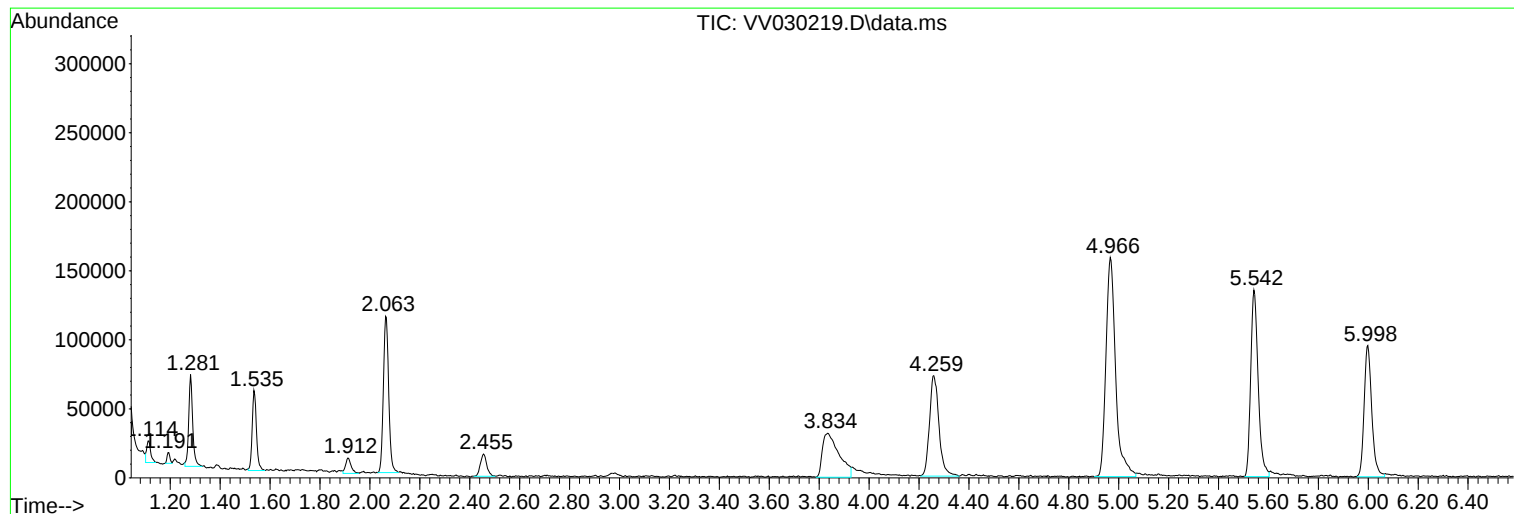

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031623\
Data File : VV030219.D
Acq On : 16 Mar 2023 12:58
Operator : SY/MD
Sample : 01884-08DL 4X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CB916DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031623\
Data File : VV030219.D
Acq On : 16 Mar 2023 12:58
Operator : SY/MD
Sample : 01884-08DL 4X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CB916DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc