

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031623\
 Data File : VV030221.D
 Acq On : 16 Mar 2023 13:55
 Operator : SY/MD
 Sample : 01884-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV030221.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.217	51	55	63	rBV4	4029	5155	1.26%	0.145%
2	1.281	68	75	88	rVB	59637	65027	15.89%	1.823%
3	1.535	146	154	164	rBV	55582	65211	15.93%	1.828%
4	2.063	308	318	335	rBV	107842	162124	39.61%	4.545%
5	2.452	431	439	451	rBV4	8669	14514	3.55%	0.407%
6	3.815	850	863	902	rBV2	38328	147734	36.09%	4.141%
7	4.259	986	1001	1020	rBV	71930	181950	44.45%	5.101%
8	4.966	1200	1221	1244	rBV3	156620	409295	100.00%	11.474%
9	5.542	1386	1400	1420	rBV2	147621	307884	75.22%	8.631%
10	5.998	1527	1542	1563	rBV	95071	205296	50.16%	5.755%
11	6.921	1818	1829	1853	rBV2	43203	85304	20.84%	2.391%
12	7.252	1920	1932	1949	rBV	183996	332013	81.12%	9.307%
13	7.561	2018	2028	2043	rBV	26801	51133	12.49%	1.433%
14	8.034	2165	2175	2209	rBV	172275	339210	82.88%	9.509%
15	8.792	2395	2411	2432	rBV	229768	388940	95.03%	10.903%
16	10.162	2826	2837	2850	rBV	65214	106725	26.08%	2.992%
17	10.332	2883	2890	2901	rVB4	3755	5886	1.44%	0.165%
18	11.194	3146	3158	3177	rBV	241993	381215	93.14%	10.687%
19	11.570	3263	3275	3293	rBV	186931	295902	72.30%	8.295%
20	12.204	3463	3472	3480	rBV2	6303	9861	2.41%	0.276%
21	16.432	4779	4787	4796	rBV9	3470	6810	1.66%	0.191%




Sum of corrected areas: 3567189

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031623\
Data File : VV030221.D
Acq On : 16 Mar 2023 13:55
Operator : SY/MD
Sample : 01884-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

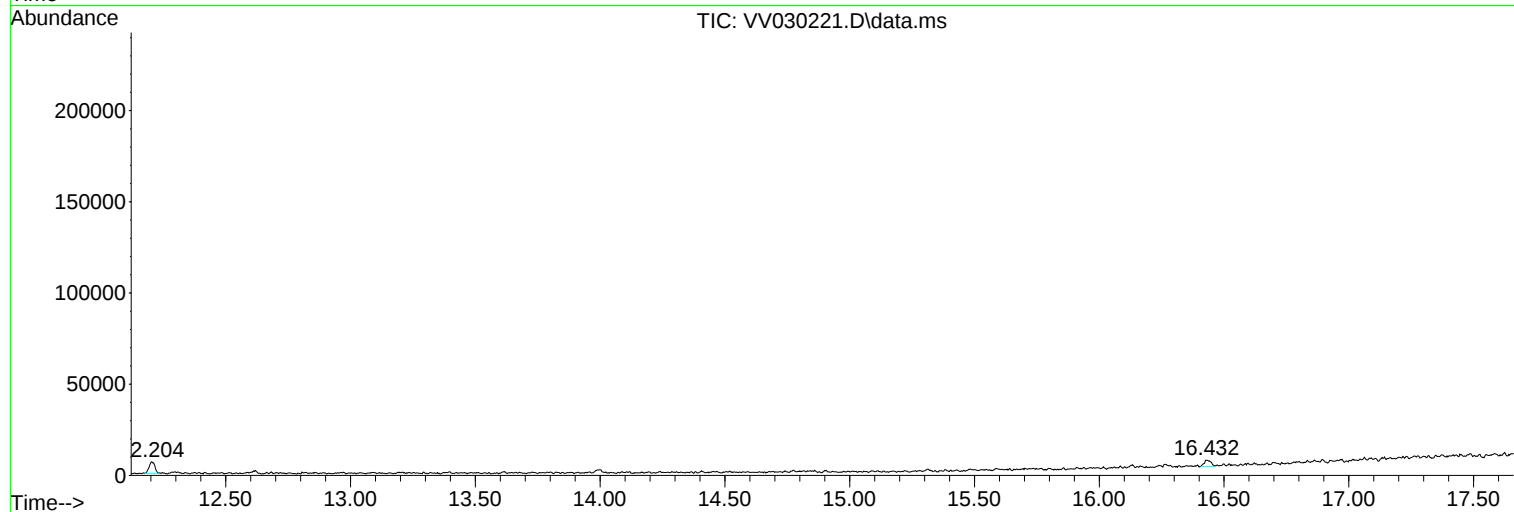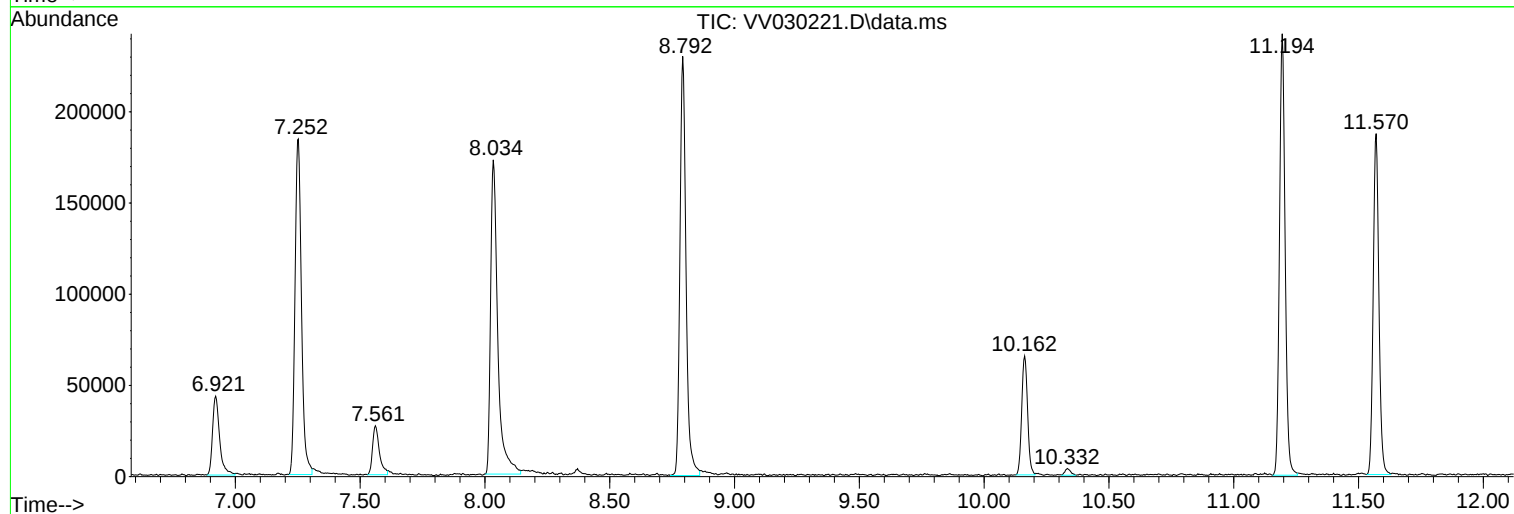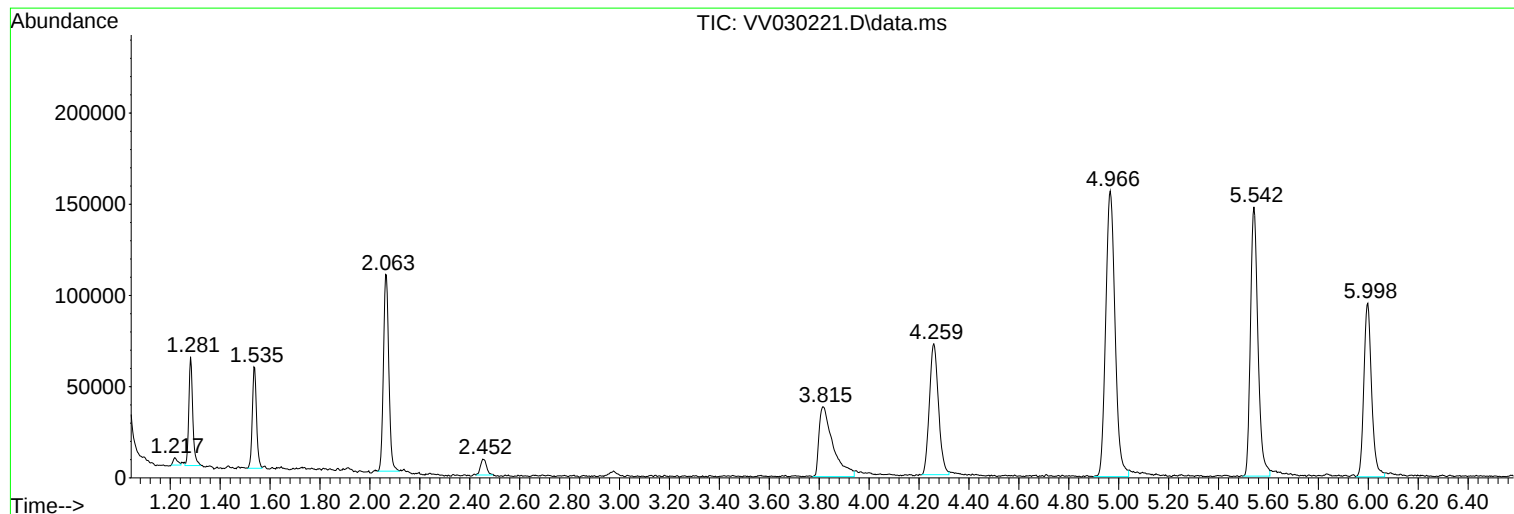

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031623\
Data File : VV030221.D
Acq On : 16 Mar 2023 13:55
Operator : SY/MD
Sample : 01884-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031623\
Data File : VV030221.D
Acq On : 16 Mar 2023 13:55
Operator : SY/MD
Sample : 01884-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc