
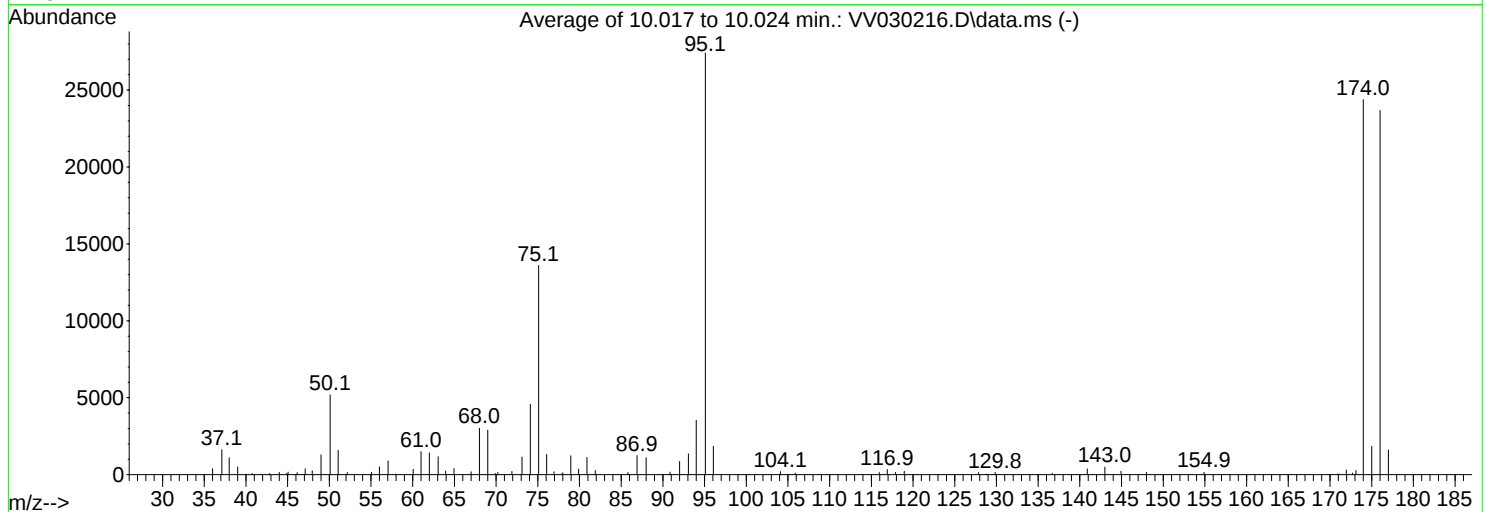


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031623\
Data File : VV030216.D
Acq On : 16 Mar 2023 11:08
Operator : SY/MD
Sample : BFB233
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB233

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Mar 17 22:49:08 2023

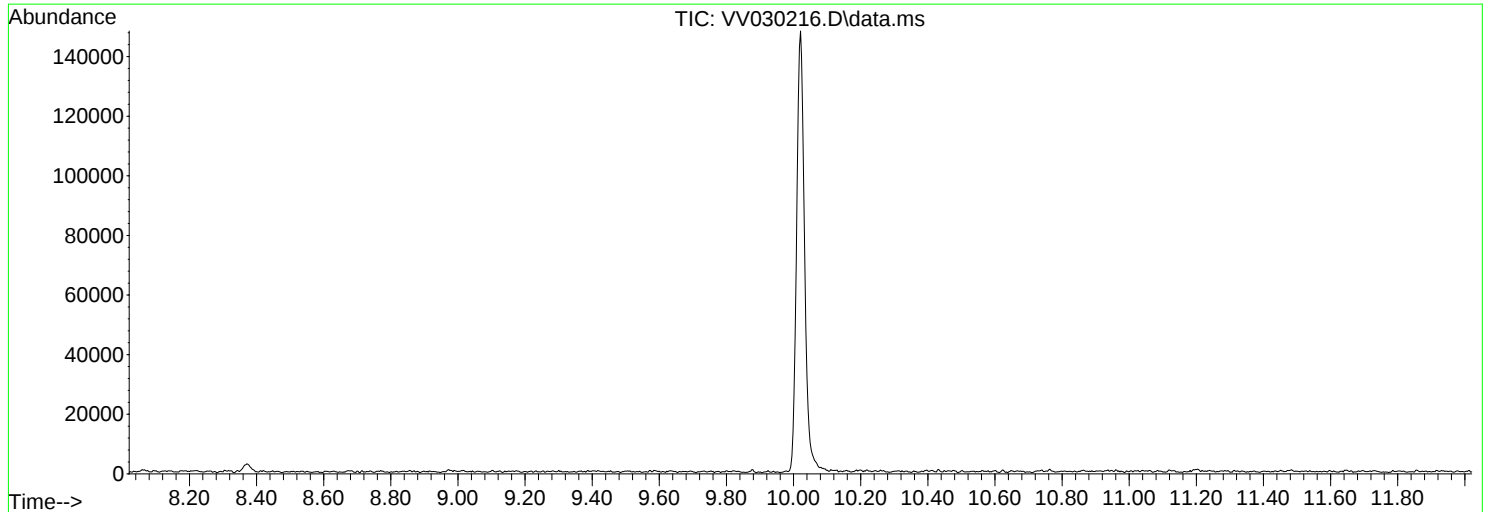

AutoFind: Scans 2792, 2793, 2794; Background Corrected with Scan 2780

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.9	5191	PASS
75	95	30	80	49.6	13599	PASS
95	95	100	100	100.0	27419	PASS
96	95	5	9	6.7	1838	PASS
173	174	0.00	2	1.1	275	PASS
174	95	50	120	88.9	24376	PASS
175	174	5	9	7.5	1839	PASS
176	174	95	105	97.1	23677	PASS
177	176	5	10	6.8	1602	PASS

m/z	Abundance
36.60	118.0
38.20	161.0
39.00	126.0
40.00	178.0
42.20	112.0
44.00	266.0

Instrument :
MSVOA_V
ClientSampleId :
BFB233

m/z	Abundance
36.00	297.0
37.10	1650.0
38.00	1249.0
39.00	557.0
40.00	227.0
40.80	110.0
41.90	101.0
42.80	124.0
44.00	412.0
44.90	247.0
46.10	156.0
47.10	412.0
48.00	201.0
49.00	1371.0
50.10	5246.0
51.00	1697.0
52.20	141.0
53.00	108.0
55.00	144.0
56.00	510.0
57.10	899.0
57.90	120.0
60.00	358.0
61.00	1435.0
62.00	1337.0
63.10	1127.0
64.00	265.0
65.00	372.0
67.00	206.0
68.00	2973.0
69.00	2945.0
69.90	205.0
71.90	222.0
73.10	1121.0
74.10	4587.0
75.10	13537.0
76.10	1359.0
76.90	189.0
77.80	124.0
79.00	1213.0
79.90	408.0
80.90	1152.0
81.90	272.0
85.80	142.0
86.90	1224.0
88.00	1100.0
90.80	157.0
92.00	858.0
93.10	1332.0
94.00	3599.0
95.10	27224.0
96.00	1903.0
104.10	188.0
105.80	108.0
115.90	137.0
116.90	332.0
117.90	148.0
118.90	212.0
127.80	138.0
129.90	122.0
140.90	405.0
143.00	493.0
144.90	215.0
148.00	118.0
154.90	152.0
170.90	110.0
172.00	304.0
172.70	310.0
174.00	23792.0
175.00	1801.0
176.00	23576.0
177.00	1544.0

Instrument :
MSVOA_V
ClientSampleId :
BFB233

m/z	Abundance
36.00	394.0
37.10	1655.0
38.00	1280.0
39.00	659.0
40.00	221.0
40.70	113.0
42.80	104.0
44.00	437.0
45.10	256.0
46.20	144.0
47.10	406.0
48.00	254.0
49.00	1316.0
50.10	5380.0
51.00	1600.0
52.20	132.0
55.10	160.0
56.00	515.0
57.00	932.0
60.00	359.0
61.00	1538.0
62.00	1468.0
63.00	1160.0
64.00	224.0
65.00	400.0
67.00	205.0
68.00	3136.0
69.00	2975.0
70.20	209.0
71.90	214.0
73.10	1176.0
74.10	4649.0
75.10	13989.0
76.10	1305.0
76.90	189.0
78.00	166.0
79.00	1284.0
79.90	376.0
80.90	1148.0
81.90	287.0
85.80	154.0
86.90	1281.0
88.00	1126.0
90.80	182.0
92.00	898.0
93.10	1380.0
94.00	3657.0
95.10	28424.0
96.10	1922.0
104.10	207.0
105.80	113.0
116.00	141.0
116.90	358.0
117.90	147.0
119.00	232.0
127.80	153.0
129.80	146.0
136.70	117.0
140.90	396.0
143.00	515.0
145.00	230.0
148.00	152.0
154.90	155.0
171.10	104.0
171.90	307.0
173.10	421.0
174.00	25288.0
175.00	1898.0
176.00	24392.0
177.00	1667.0

Instrument :
MSVOA_V
ClientSampleId :
BFB233

m/z	Abundance
36.00	449.0
37.10	1550.0
38.00	1275.0
39.00	664.0
40.00	223.0
44.00	394.0
45.00	253.0
46.20	104.0
47.10	342.0
47.90	292.0
49.00	1169.0
50.10	4948.0
51.10	1448.0
52.10	145.0
55.10	176.0
56.00	496.0
57.00	849.0
60.10	325.0
61.00	1509.0
62.00	1433.0
63.00	1201.0
63.90	212.0
64.90	418.0
67.00	166.0
68.00	2942.0
69.00	2772.0
70.20	215.0
71.90	198.0
73.10	1139.0
74.10	4463.0
75.10	13270.0
76.00	1283.0
77.00	194.0
78.00	214.0
78.90	1171.0
79.90	303.0
80.90	1058.0
81.90	265.0
85.80	120.0
86.90	1202.0
88.00	1078.0
90.90	169.0
92.00	807.0
93.00	1355.0
94.00	3347.0
95.10	26608.0
96.10	1688.0
104.10	184.0
105.90	103.0
115.90	128.0
116.90	313.0
117.90	136.0
119.00	221.0
127.90	130.0
128.80	115.0
129.90	154.0
136.70	103.0
140.90	324.0
143.00	474.0
145.00	221.0
148.00	156.0
154.90	135.0
172.00	300.0
173.10	403.0
174.00	24048.0
175.00	1817.0
176.00	23064.0
177.00	1595.0

Instrument :
MSVOA_V
ClientSampleId :
BFB233