


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV031719\
Data File : VV009727.D
Acq On : 16 Mar 2019 13:56
Operator : SY/MD
Sample : BFB79
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB79

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031719WMA.M
Title : VOC Analysis
Last Update : Mon Mar 18 12:32:58 2019

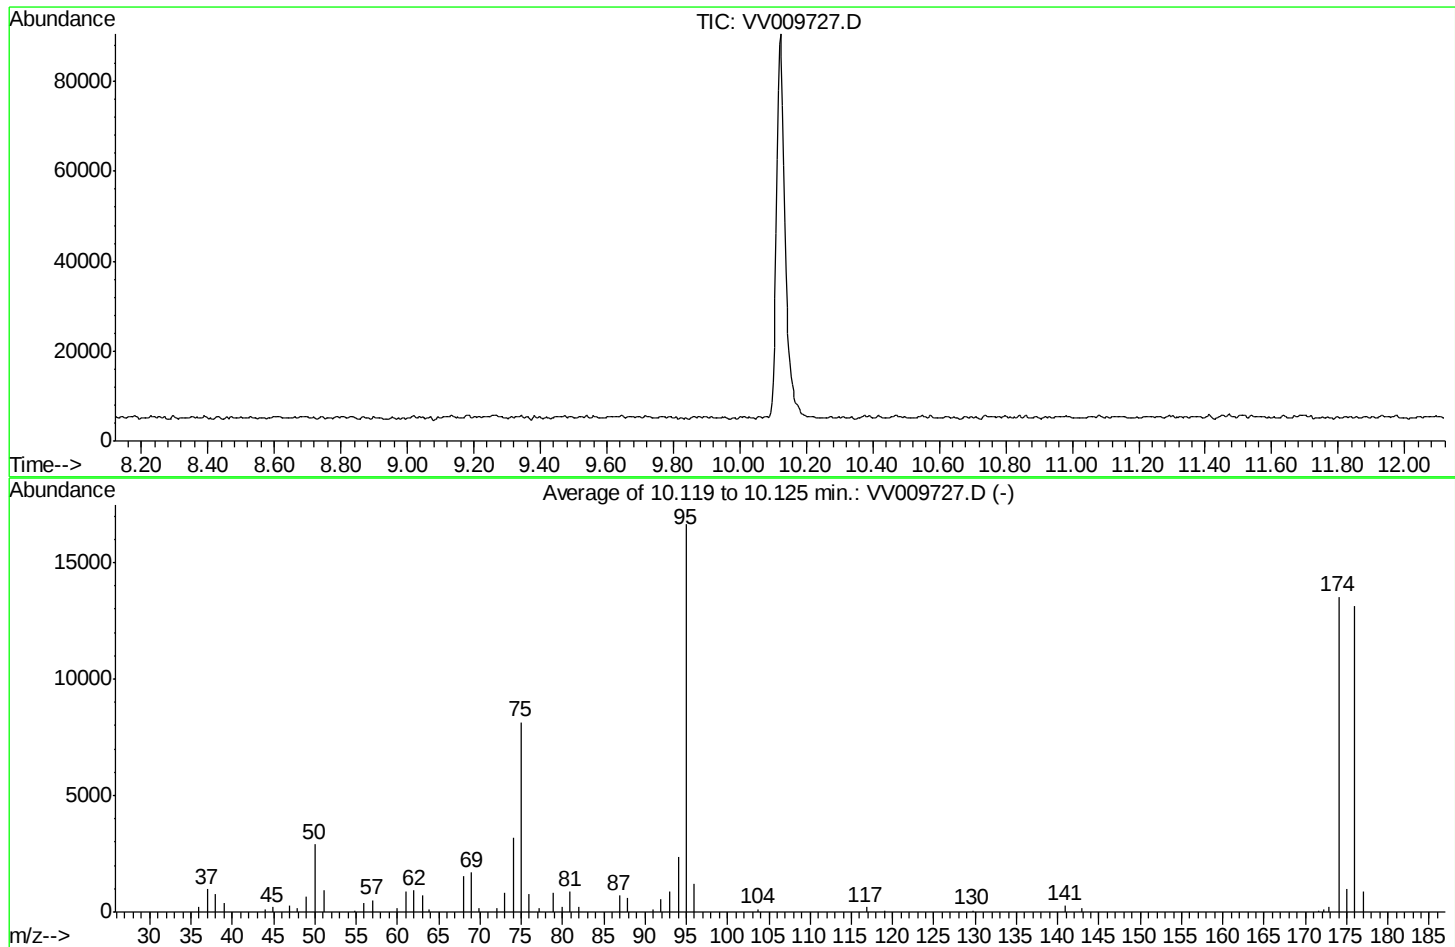

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2797

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	2907	PASS
75	95	30	80	49.0	8148	PASS
95	95	100	100	100.0	16642	PASS
96	95	5	9	7.3	1215	PASS
173	174	0.00	2	1.5	197	PASS
174	95	50	120	81.3	13532	PASS
175	174	5	9	7.3	982	PASS
176	174	95	101	97.1	13139	PASS
177	176	5	9	6.6	861	PASS

m/z	Abundance
40.00	5155.0
44.00	139.0

Instrument :
MSVOA_V
ClientSampleId :
BFB79

m/z	Abundance
35.90	235.0
37.00	1056.0
38.00	836.0
38.90	384.0
40.00	4917.0
44.00	253.0
44.90	236.0
47.00	266.0
47.80	191.0
48.90	698.0
50.00	2958.0
51.00	1029.0
54.90	105.0
56.00	374.0
57.00	432.0
60.00	172.0
61.00	841.0
62.00	828.0
63.00	673.0
63.90	122.0
68.00	1561.0
69.00	1751.0
69.90	214.0
72.10	181.0
73.00	816.0
74.00	3181.0
75.00	8449.0
76.00	798.0
77.10	177.0
78.90	793.0
79.90	261.0
80.90	847.0
81.90	175.0
86.90	799.0
87.90	725.0
90.90	112.0
92.00	493.0
93.00	820.0
94.00	2353.0
95.00	16728.0
96.00	1197.0
103.80	167.0
116.80	196.0
119.00	119.0
129.70	112.0
140.90	299.0
142.90	214.0
172.20	115.0
172.80	146.0
174.00	13248.0
174.90	956.0
176.00	12825.0
176.90	892.0

Instrument :
MSVOA_V
ClientSampleId :
BFB79

m/z	Abundance
35.90	199.0
37.00	1022.0
38.00	836.0
39.00	399.0
40.00	4794.0
44.00	257.0
44.90	218.0
47.00	258.0
47.80	176.0
48.90	663.0
50.00	3030.0
51.00	966.0
56.00	433.0
57.00	537.0
60.00	190.0
61.00	902.0
62.00	971.0
63.00	705.0
63.80	118.0
68.00	1612.0
69.00	1719.0
69.90	178.0
72.10	218.0
73.00	858.0
74.00	3269.0
75.00	8385.0
75.90	808.0
77.10	160.0
79.00	882.0
79.90	246.0
80.90	925.0
81.90	199.0
86.90	739.0
87.90	627.0
90.90	118.0
91.90	537.0
93.00	922.0
94.00	2473.0
95.00	17080.0
96.00	1264.0
103.70	137.0
116.80	229.0
129.70	106.0
140.90	274.0
142.90	193.0
172.20	140.0
172.90	197.0
174.00	13964.0
174.90	983.0
176.00	13574.0
176.90	888.0

Instrument :
MSVOA_V
ClientSampleId :
BFB79

m/z	Abundance
35.90	174.0
37.00	866.0
38.00	717.0
39.00	366.0
40.00	4760.0
44.00	270.0
44.80	183.0
46.90	226.0
47.90	158.0
49.00	658.0
50.00	2734.0
51.10	891.0
56.00	400.0
57.00	590.0
60.00	180.0
61.00	863.0
62.00	1003.0
63.00	716.0
63.80	103.0
68.00	1490.0
69.00	1601.0
69.90	126.0
72.10	162.0
73.00	842.0
74.00	3038.0
75.00	7612.0
75.90	761.0
77.10	134.0
79.00	870.0
79.90	223.0
80.90	814.0
81.90	226.0
86.90	557.0
87.90	499.0
90.90	105.0
92.00	639.0
93.00	835.0
94.00	2345.0
95.00	16118.0
96.00	1184.0
103.70	110.0
116.90	192.0
140.90	219.0
143.00	153.0
171.60	110.0
172.20	137.0
173.00	250.0
174.00	13386.0
175.00	1009.0
176.00	13019.0
177.00	803.0

Instrument :
MSVOA_V
ClientSampleId :
BFB79