
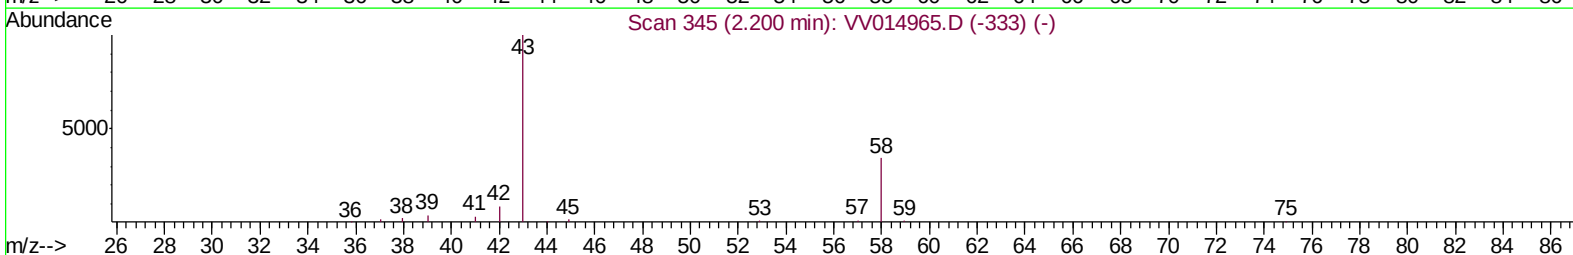
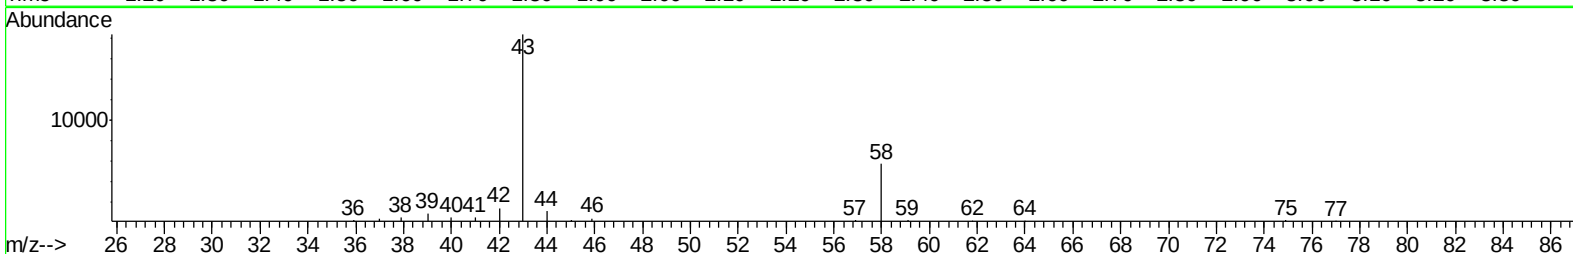


Data File : VV014990.D
Acq On : 17 Mar 2020 21:51
Operator : SY/MD
Sample : VSTDCCC050
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Quant Time: Mar 18 05:28:08 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Mar 18 05:21:28 2020
Response via : Initial Calibration

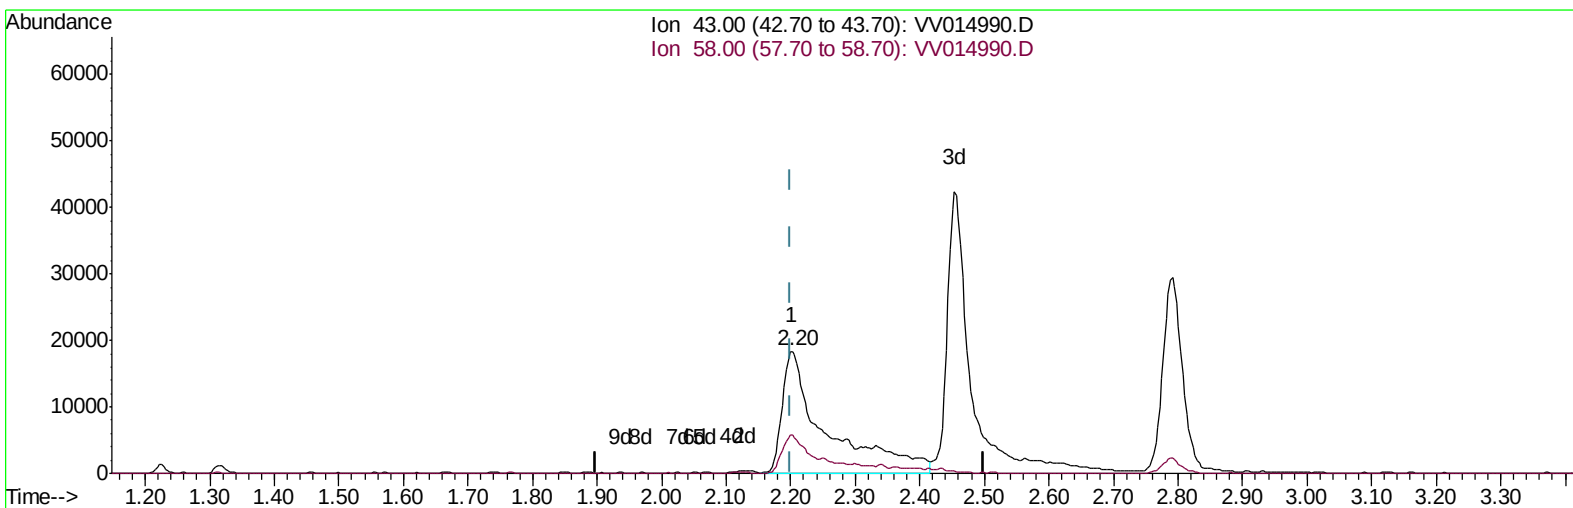

TIC: VV014990.D

(13) Acetone (T)

2.203min (+0.003) 64.29ug/L m

response 86535

Ion	Exp%	Act%
43.00	100	100
58.00	25.80	17.44
0.00	0.00	0.00
0.00	0.00	0.00