
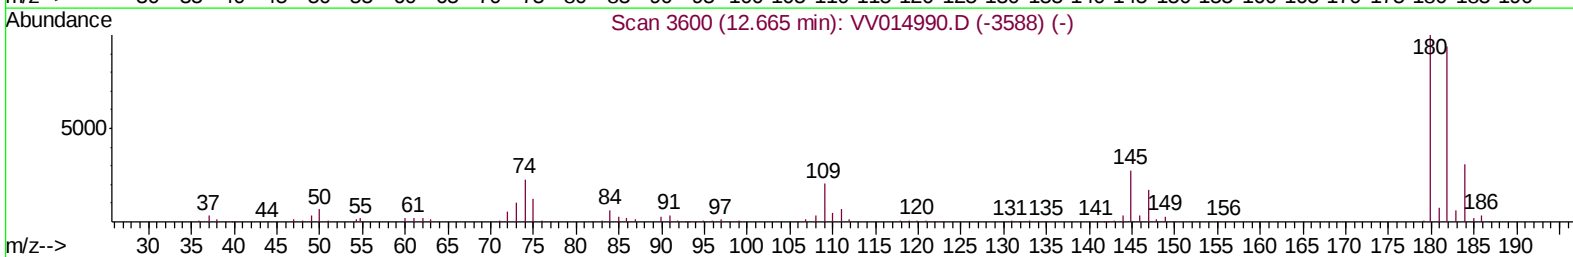
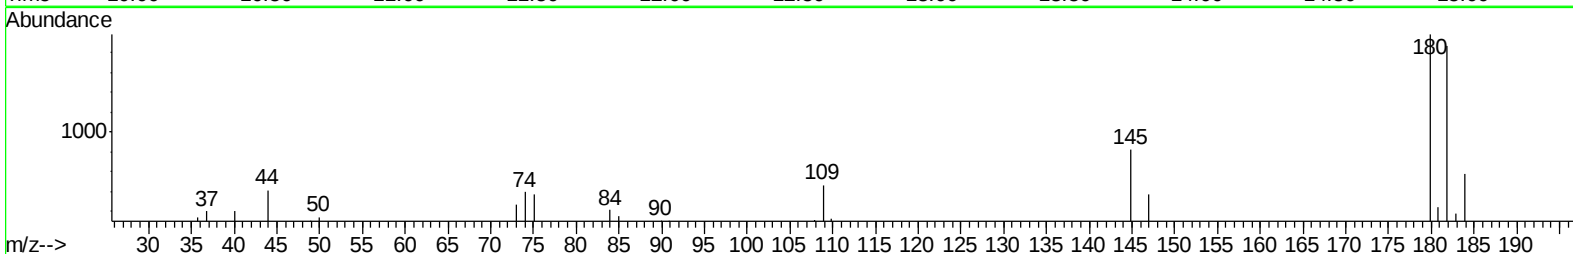


Data File : VV014993.D
Acq On : 17 Mar 2020 23:34
Operator : SY/MD
Sample : L1940-16DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Quant Time: Mar 18 07:45:20 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Mar 18 07:43:00 2020
Response via : Initial Calibration

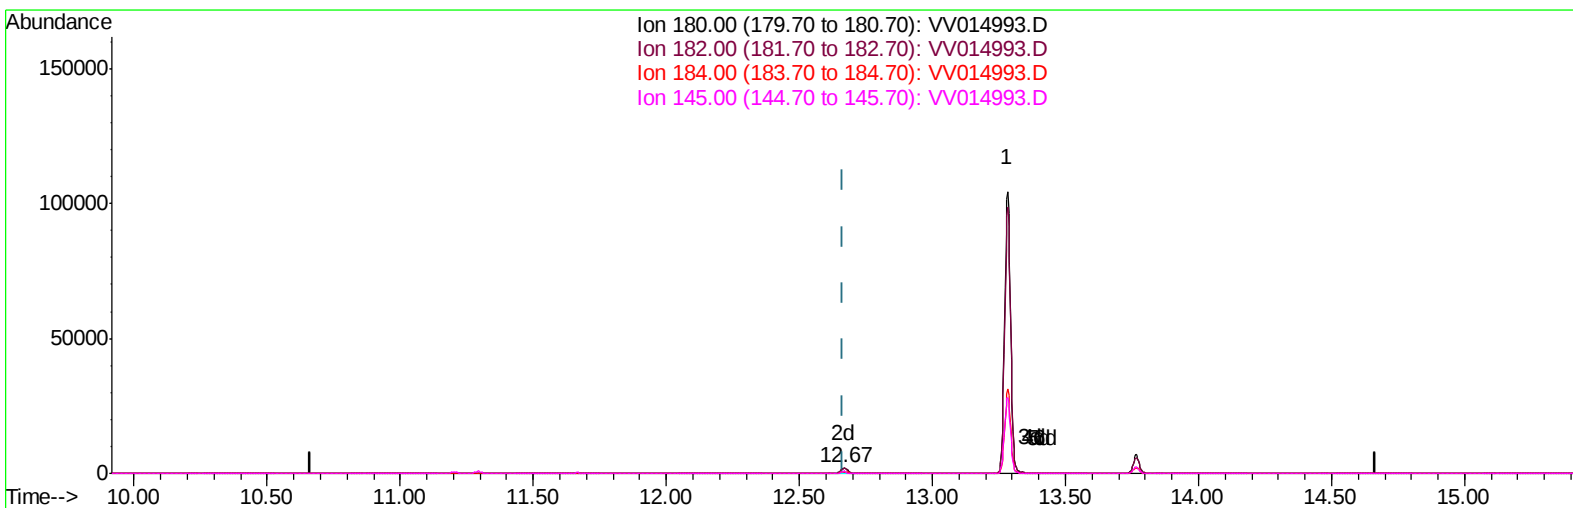

TIC: VV014993.D

(67) 1,3,5-Trichlorobenzene

12.665min (-0.000) 0.77ug/L m

response 3230

Ion	Exp%	Act%
180.00	100	100
182.00	94.60	4666.63#
184.00	30.30	1441.61#
145.00	27.50	1347.03#