
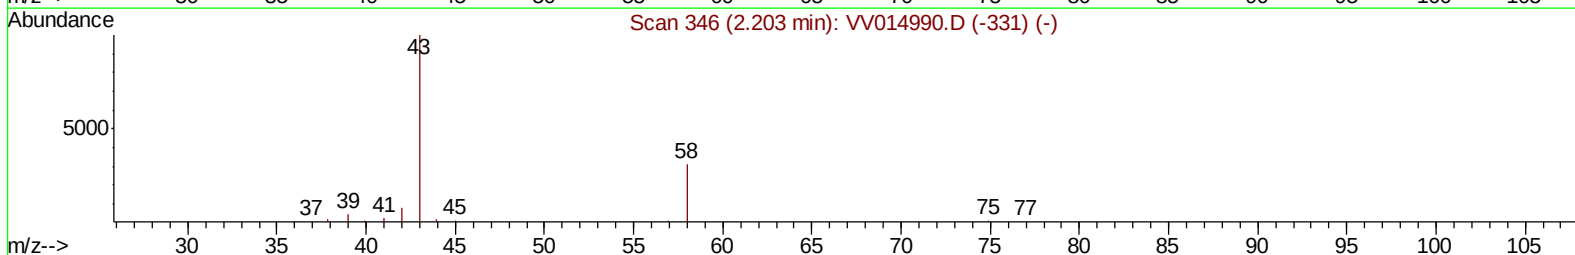
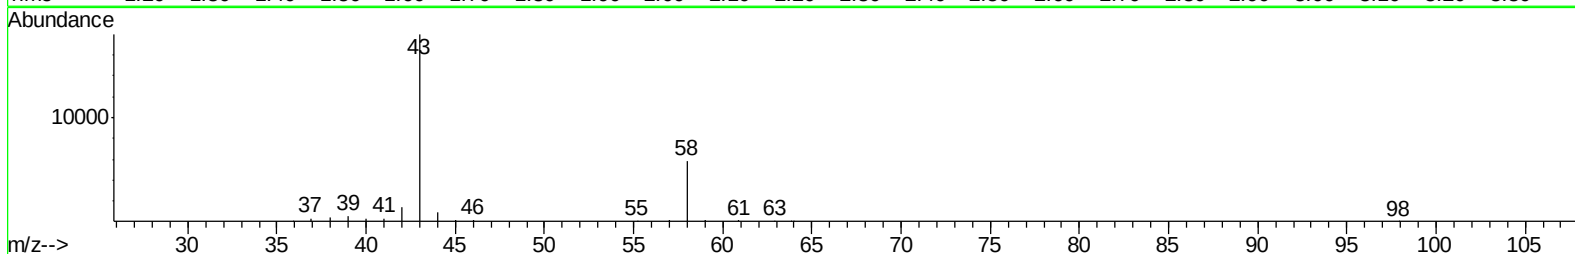


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV031720\
Data File : VV015012.D
Acq On : 18 Mar 2020 07:13
Operator : SY/MD
Sample : VSTDCCC050EC
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 51 Sample Multiplier: 1

Quant Time: Mar 18 07:49:31 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Mar 18 07:43:00 2020
Response via : Initial Calibration

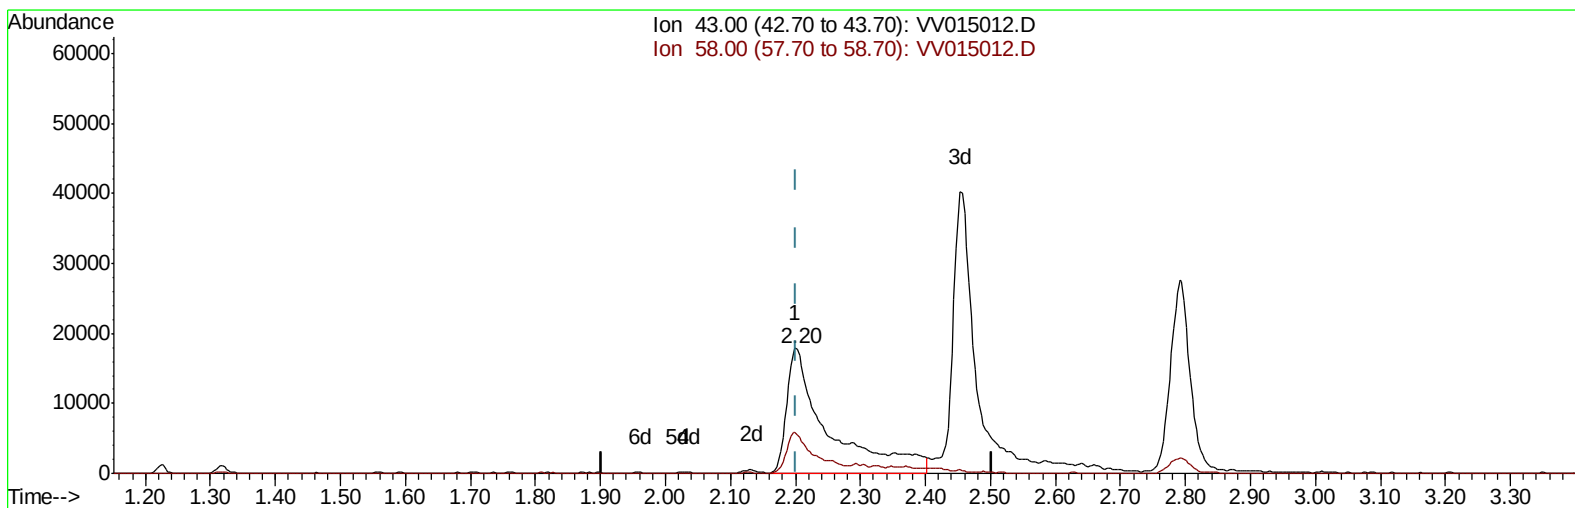

TIC: VV015012.D

(13) Acetone (T)

2.200min (-0.003) 63.03ug/L m

response 79284

Ion	Exp%	Act%
43.00	100	100
58.00	25.80	19.08
0.00	0.00	0.00
0.00	0.00	0.00