

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV031720\
Quantitation Report (QT Reviewed)


Data File : VV014974.D
Acq On : 17 Mar 2020 15:23
Operator : SY/MD
Sample : L1940-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Quant Time: Mar 18 06:03:47 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Mar 18 05:21:28 2020
Response via : Initial Calibration

Instrument :
MSVOA_V
ClientSampleId :
C0DM8

Manual Integrations
APPROVED

apatel
3/18/2020 3:02:06 PM

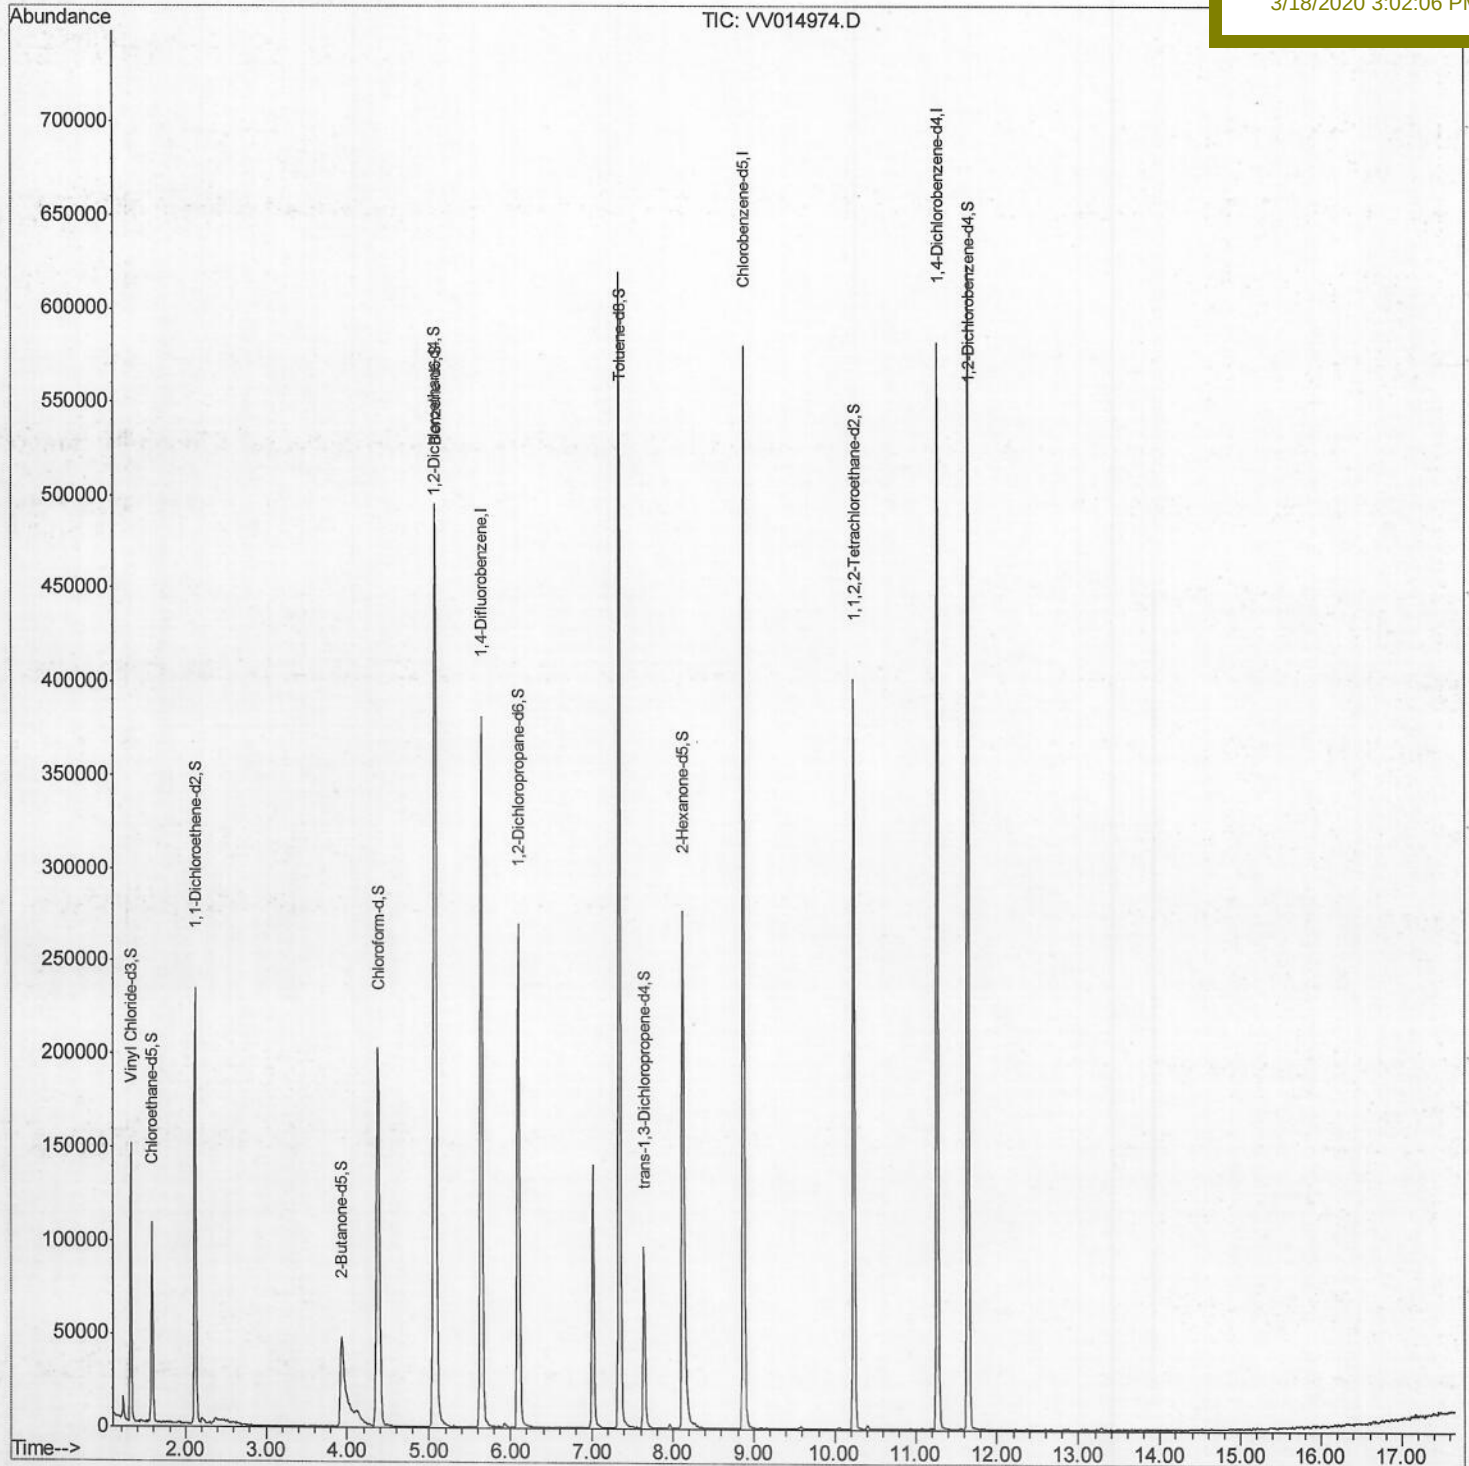




Data File : VV014974.D
Acq On : 17 Mar 2020 15:23
Operator : SY/MD
Sample : L1940-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Quant Time: Mar 18 05:25:04 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Mar 18 05:21:28 2020
Response via : Initial Calibration

Instrument :
MSVOA_V
ClientSampleId :
C0DM8

Manual Integrations
APPROVED

apatel
3/18/2020 3:02:06 PM

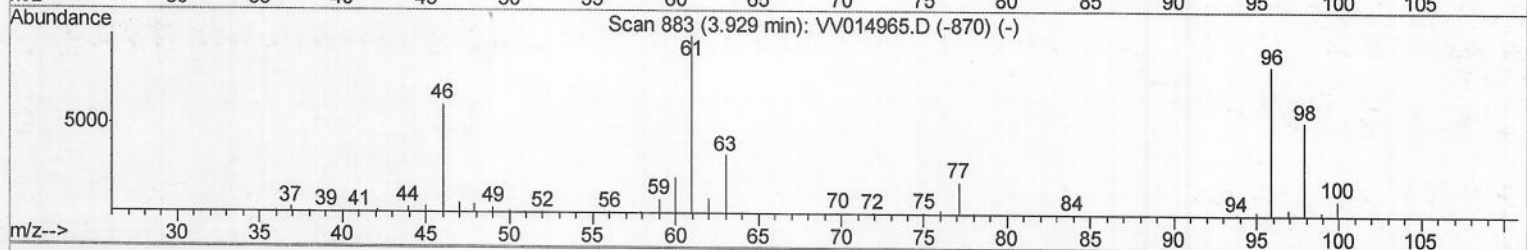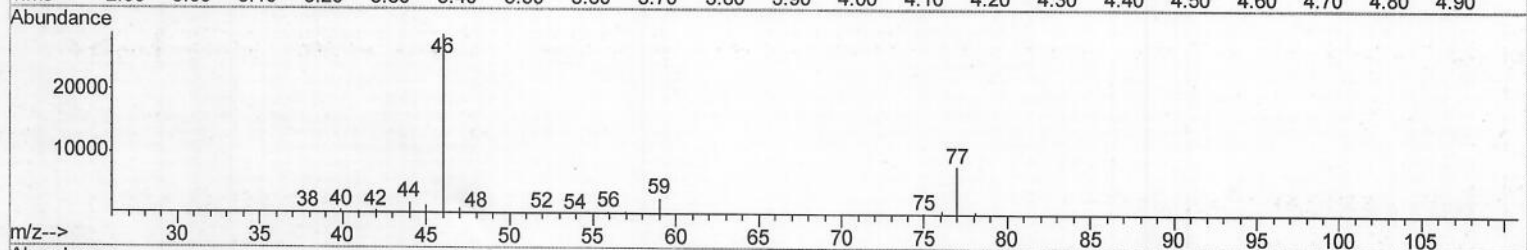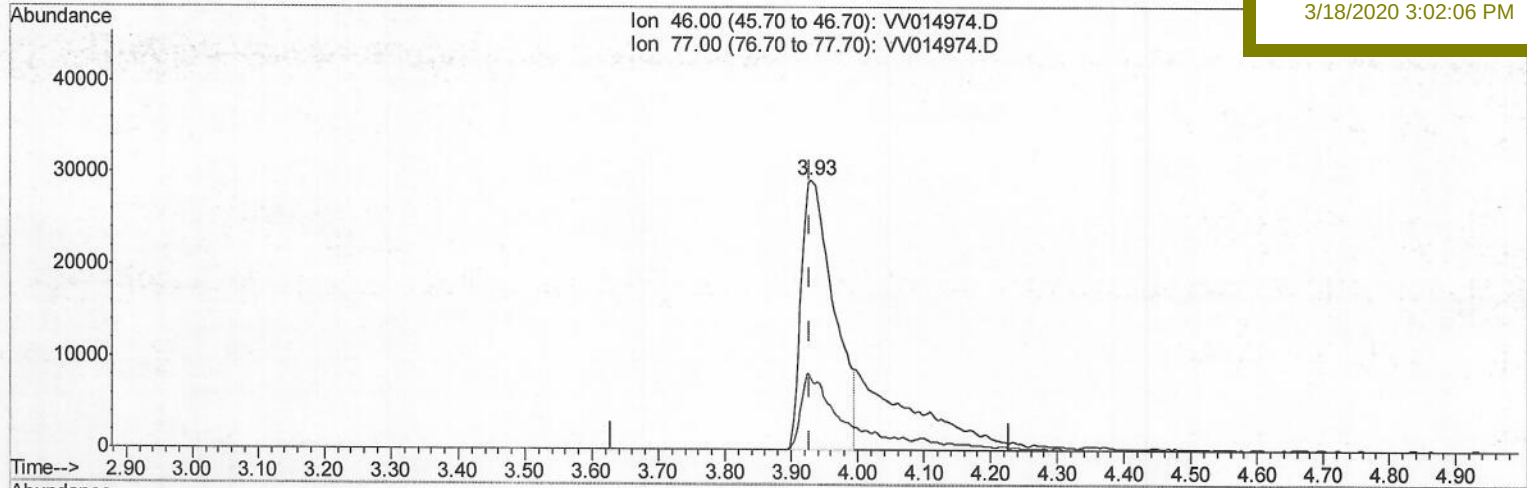

TIC: VV014974.D

(21) 2-Butanone-d5 (S)

3.930min (+0.000) 70.88ug/L

response 99511

Ion	Exp%	Act%
46.00	100	100
77.00	20.50	12.01#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV031720\
Quantitation Report (Qedit)




Data File : VV014974.D
Acq On : 17 Mar 2020 15:23
Operator : SY/MD
Sample : L1940-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Quant Time: Mar 18 05:25:04 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Mar 18 05:21:28 2020
Response via : Initial Calibration

Instrument :
MSVOA_V
ClientSampleId :
C0DM8

Manual Integrations
APPROVED

apatel
3/18/2020 3:02:06 PM

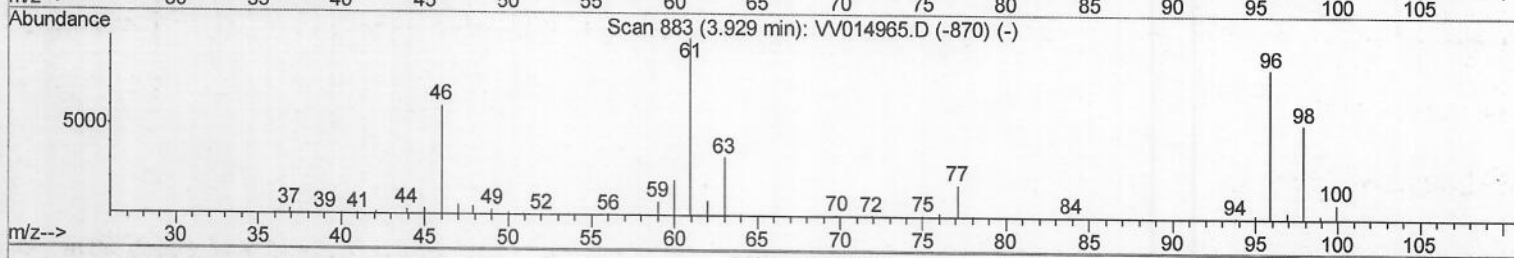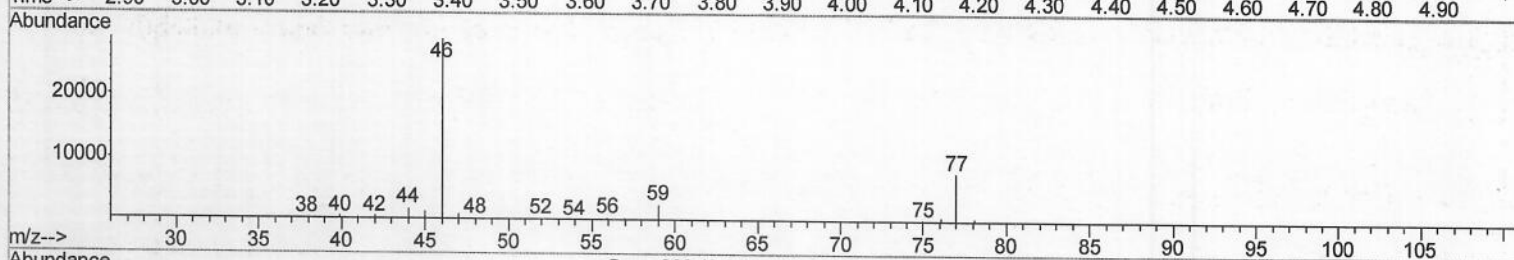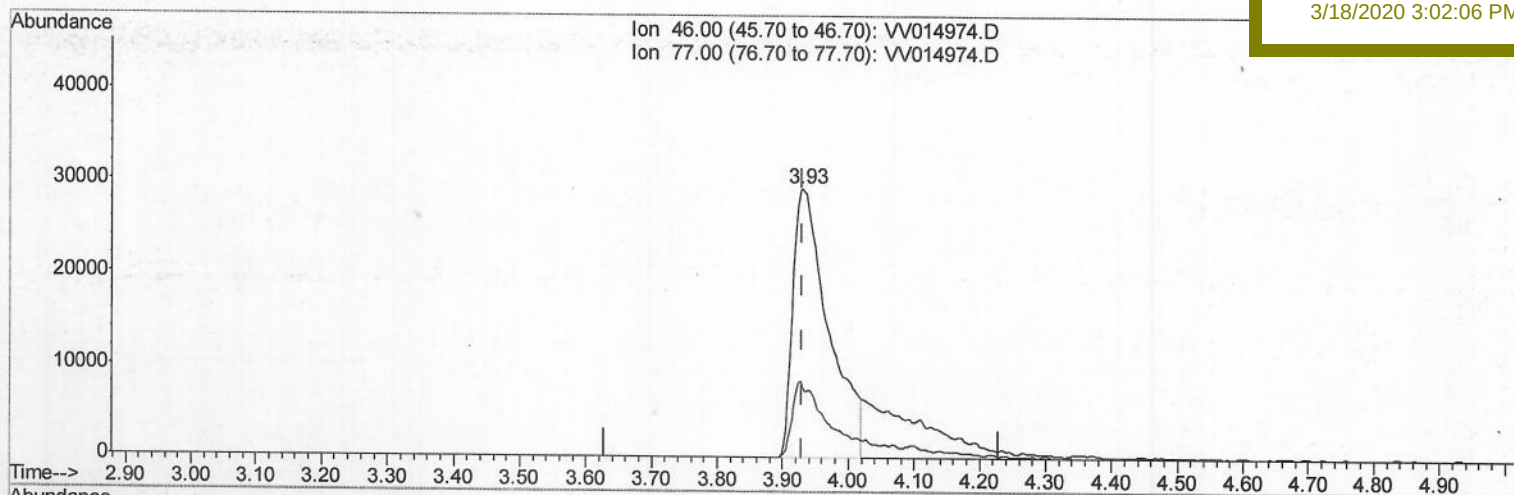

TIC: VV014974.D

(21) 2-Butanone-d5 (S)

3.930min (+0.000) 79.27ug/L m

response 111287

Ion	Exp%	Act%
46.00	100	100
77.00	20.50	10.74#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV031720\
Quantitation Report (QT Reviewed)

Data File : VV014974.D
Acq On : 17 Mar 2020 15:23
Operator : SY/MD
Sample : L1940-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Quant Time: Mar 18 06:03:47 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Mar 18 05:21:28 2020
Response via : Initial Calibration

Instrument :
MSVOA_V
ClientSampleId :
C0DM8

Manual Integrations
APPROVED

apatel
3/18/2020 3:02:06 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	345600	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	338679	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	159465	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	92824	40.32	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	80.64%	
7) Chloroethane-d5	1.58	69	73679	43.09	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	86.18%	
11) 1,1-Dichloroethene-d2	2.12	63	117033	33.13	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	66.26%	
21) 2-Butanone-d5	3.93	46	111287m	79.27	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	79.27%	
24) Chloroform-d	4.38	84	214765	44.77	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	89.54%	
26) 1,2-Dichloroethane-d4	5.06	65	144764	47.63	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	95.26%	
32) Benzene-d6	5.08	84	435612	46.69	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	93.38%	
36) 1,2-Dichloropropane-d6	6.10	67	131689	47.40	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	94.80%	
41) Toluene-d8	7.34	98	416719	45.16	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	90.32%	
43) trans-1,3-Dichloropropene-	7.64	79	57819	39.14	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	78.28%	
47) 2-Hexanone-d5	8.12	63	117448	93.65	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	93.65%	
57) 1,1,2,2-Tetrachloroethane-	10.24	84	187493	46.09	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	92.18%	
64) 1,2-Dichlorobenzene-d4	11.65	152	176274	50.46	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	100.92%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

03/20/2020