

Quantitation Report (QT Reviewed)

Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV031720\
 Data File : VV015011.D
 Acq On : 18 Mar 2020 06:49
 Operator : SY/MD
 Sample : L1941-09
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 MSVOA_V
 Client Sample ID :
 C0DB9

Manual Integrations
 APPROVED

apatel
 3/18/2020 3:02:22 PM

Quant Time: Mar 18 09:02:18 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Mar 18 07:43:00 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	311197	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	316011	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	175338	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.32	65	74453	35.91	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	71.82%		
7) Chloroethane-d5	1.58	69	59350	38.54	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	77.08%		
11) 1,1-Dichloroethene-d2	2.12	63	96705	30.40	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	60.80%		
21) 2-Butanone-d5	3.93	46	91822	72.64	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	72.64%		
24) Chloroform-d	4.38	84	181994	42.13	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	84.26%		
26) 1,2-Dichloroethane-d4	5.06	65	123954	45.29	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	90.58%		
32) Benzene-d6	5.08	84	377193	43.33	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	86.66%		
36) 1,2-Dichloropropane-d6	6.10	67	112385	43.35	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	86.70%		
41) Toluene-d8	7.34	98	370699	43.05	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	86.10%		
43) trans-1,3-Dichloropropene	7.64	79	47219	34.26	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	68.52%		
47) 2-Hexanone-d5	8.12	63	98158	83.88	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	83.88%		
57) 1,1,2,2-Tetrachloroethane	10.24	84	162155	42.73	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	85.46%		
64) 1,2-Dichlorobenzene-d4	11.66	152	183574	47.79	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	95.58%		
Target Compounds						
25) Chloroform	4.41	83	7606	1.867	ug/L	93
33) Benzene	5.13	78	41659	4.845	ug/L	100
51) Chlorobenzene	8.90	112	7513645	1127.643	ug/L	99
62) 1,3-Dichlorobenzene	11.20	146	665775	115.225	ug/L	99
63) 1,4-Dichlorobenzene	11.30	146	2370426	407.261	ug/L	98
65) 1,2-Dichlorobenzene	11.67	146	17512089m	3034.110	ug/L	98
67) 1,3,5-Trichlorobenzene	12.67	180	2488	0.549	ug/L	87
68) 1,2,4-trichlorobenzene	13.29	180	3301646	817.684	ug/L	99
70) 1,2,3-Trichlorobenzene	13.76	180	521190	130.396	ug/L	100

MD
 03/18/2020

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quantitation Report (QT Reviewed)


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV031720\
 Data File : VV015011.D
 Acq On : 18 Mar 2020 06:49
 Operator : SY/MD
 Sample : L1941-09
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DB9

Manual Integrations
 APPROVED

apatel
 3/18/2020 3:02:22 PM

Quant Time: Mar 18 09:02:18 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Mar 18 07:43:00 2020
 Response via : Initial Calibration

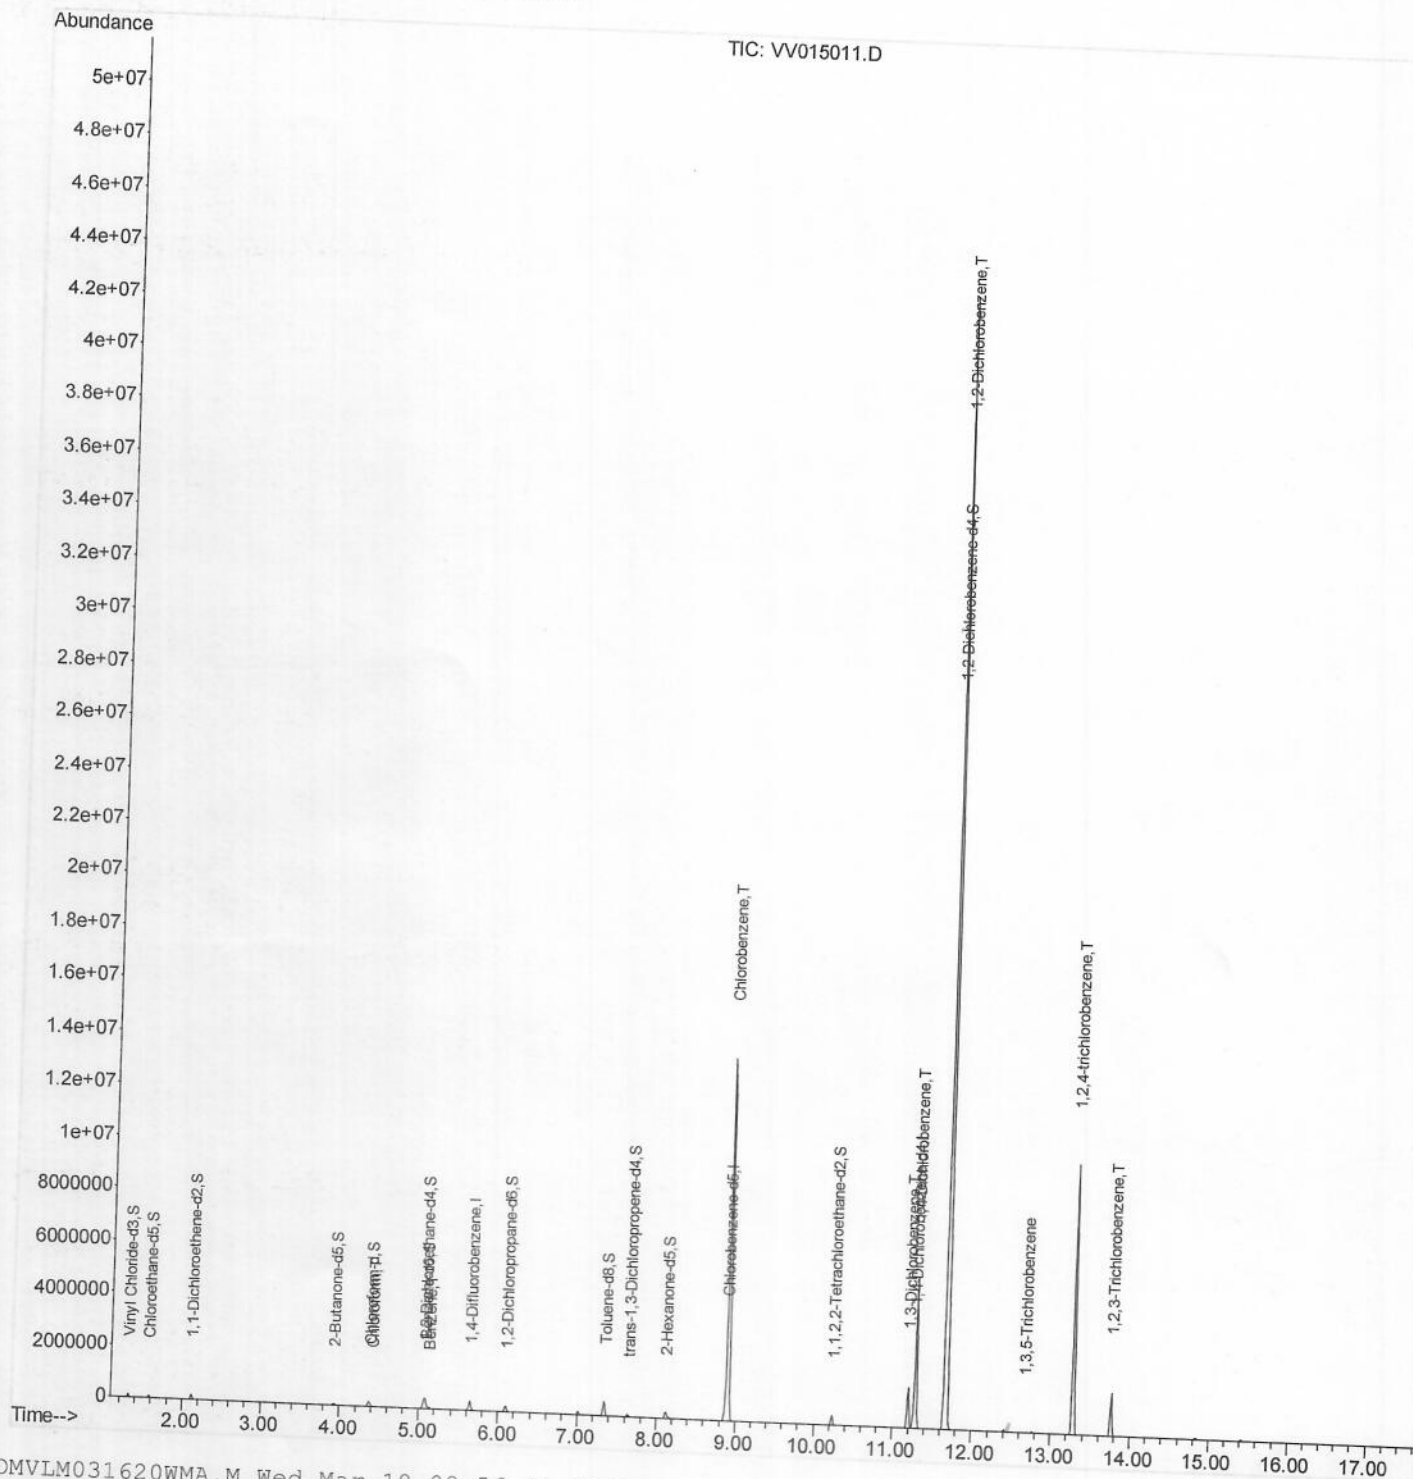

SOMVLM031620WMA.M Wed Mar 18 08:56:41 2020

Quantitation Report (Qedit)


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV031720\
 Data File : VV015011.D
 Acq On : 18 Mar 2020 06:49
 Operator : SY/MD
 Sample : L1941-09
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DB9

Manual Integrations
 APPROVED

apatel
 3/18/2020 3:02:22 PM

Quant Time: Mar 18 07:49:17 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Mar 18 07:43:00 2020
 Response via : Initial Calibration

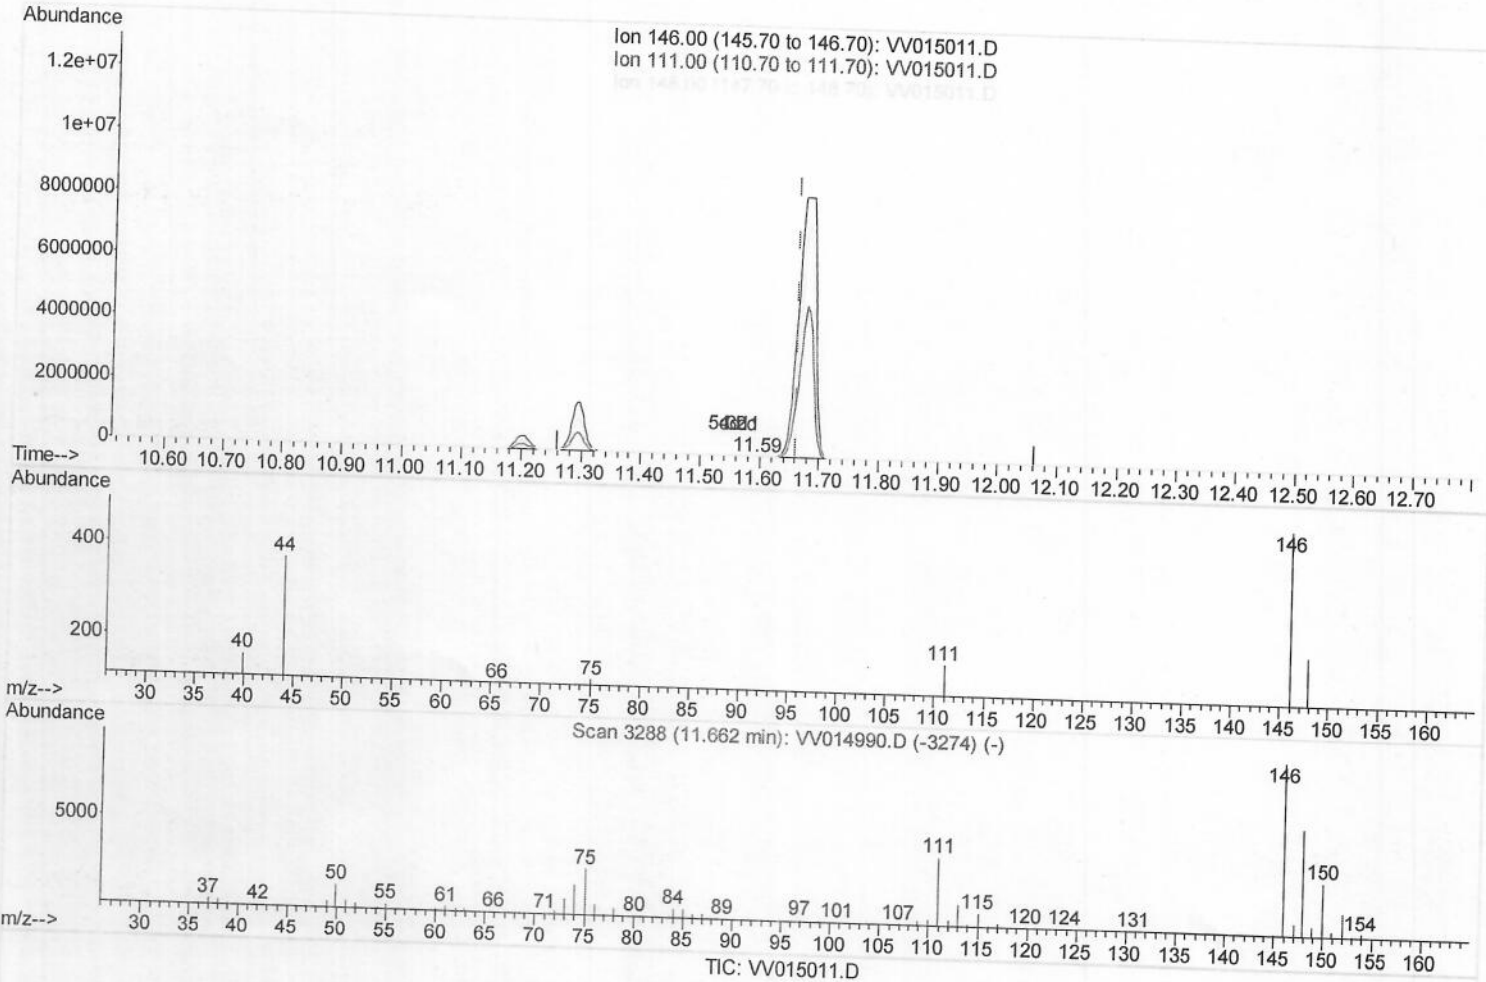

(65) 1,2-Dichlorobenzene (T)

11.591min (-0.071) 0.02ug/L

response 108

Ion	Exp%	Act%
146.00	100	100
111.00	39.50	36.84
148.00	65.30	44.53#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV031720\
 Data File : VV015011.D
 Acq On : 18 Mar 2020 06:49
 Operator : SY/MD
 Sample : L1941-09
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DB9

Manual Integrations
 APPROVED

apatel
 3/18/2020 3:02:22 PM

Quant Time: Mar 18 07:49:17 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Mar 18 07:43:00 2020
 Response via : Initial Calibration

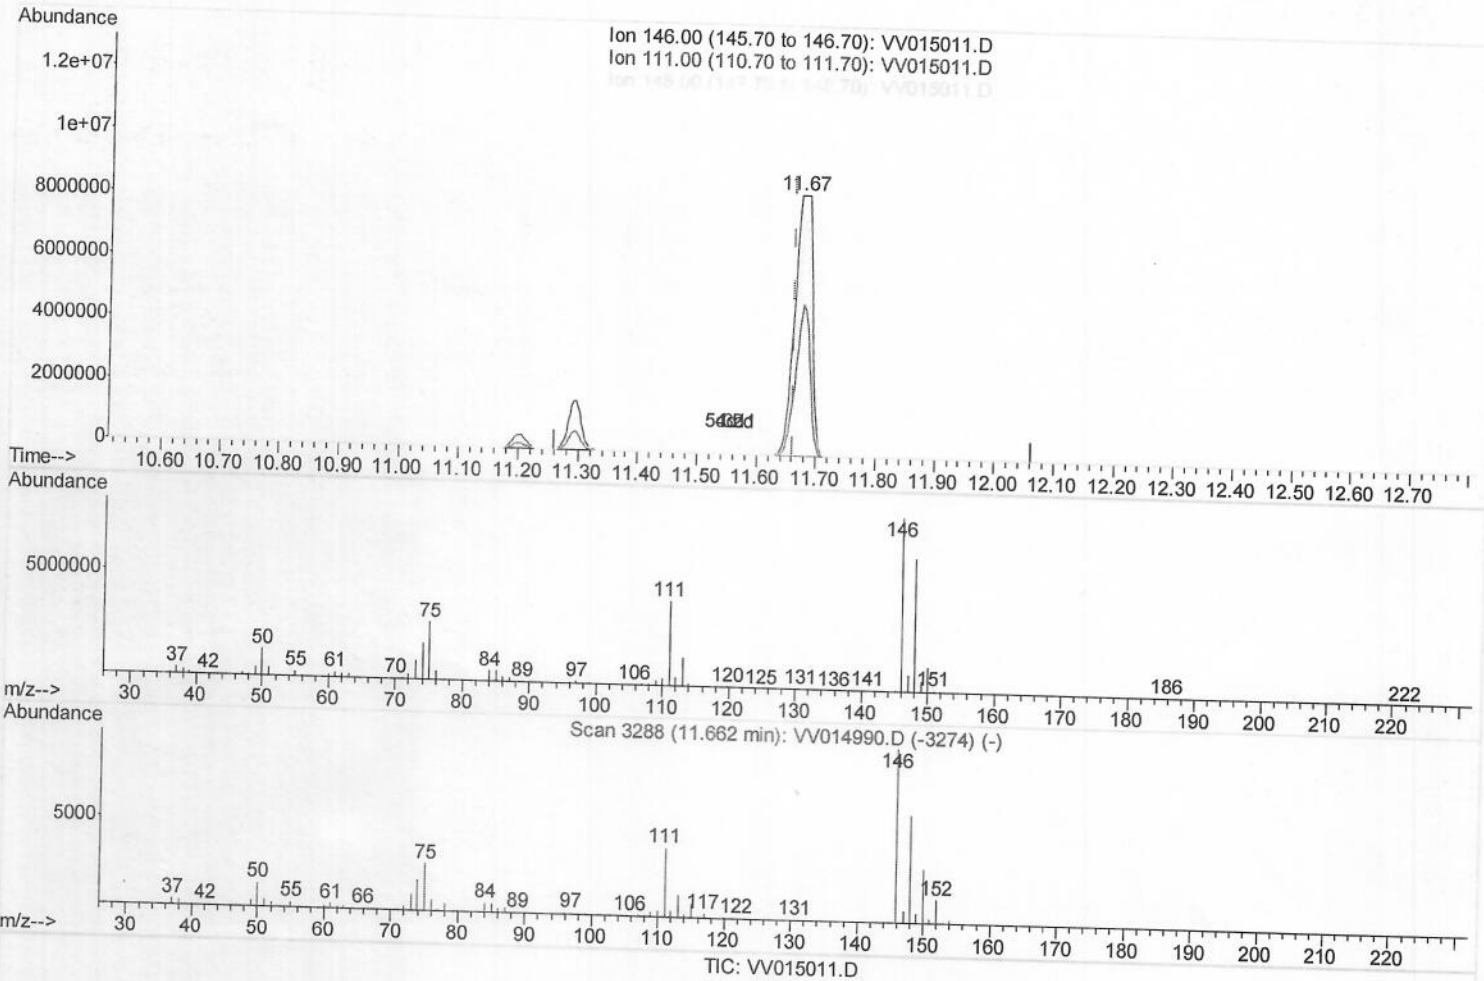

(65) 1,2-Dichlorobenzene (T)

11.672min (+0.009) 3034.11ug/L m

response 17512089

Ion	Exp%	Act%
146.00	100	100
111.00	39.50	49.18#
148.00	65.30	76.95
0.00	0.00	0.00

MD
 03/18/2020