

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031720\
 Data File : VV014972.D
 Acq On : 17 Mar 2020 14:35
 Operator : SY/MD
 Sample : L1940-04
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D91

Manual Integrations
 APPROVED

apatel
 3/18/2020 3:01:45 PM

Quant Time: Mar 18 05:57:00 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Mar 18 05:21:28 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	332645	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	326320	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	154328	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	90687	40.92	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	81.84%
7) Chloroethane-d5	1.58	69	73722	44.79	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	89.58%
11) 1,1-Dichloroethene-d2	2.12	63	112236	33.01	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	66.02%
21) 2-Butanone-d5	3.93	46	111813m	82.75	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	82.75%
24) Chloroform-d	4.38	84	209563	45.39	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	90.78%
26) 1,2-Dichloroethane-d4	5.06	65	140238	47.94	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.88%
32) Benzene-d6	5.08	84	425478	47.33	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.66%
36) 1,2-Dichloropropane-d6	6.10	67	127080	47.47	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	94.94%
41) Toluene-d8	7.34	98	414081	46.57	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	93.14%
43) trans-1,3-Dichloropropene-	7.64	79	57401	40.33	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	80.66%
47) 2-Hexanone-d5	8.12	63	115935	95.94	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	95.94%
57) 1,1,2,2-Tetrachloroethane-	10.24	84	182204	46.49	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	92.98%
64) 1,2-Dichlorobenzene-d4	11.65	152	171280	50.66	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	101.32%

Target Compounds					Ovalue
51) Chlorobenzene	8.90	112	6405	0.931 ug/L	97
63) 1,4-Dichlorobenzene	11.30	146	4709	0.919 ug/L	93
65) 1,2-Dichlorobenzene	11.67	146	3517	0.692 ug/L #	91

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV031720\
Data File : VV014972.D
Acq On : 17 Mar 2020 14:35
Operator : SY/MD
Sample : L1940-04
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 10 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
C0D91

Manual Integrations
APPROVED

apatel
3/18/2020 3:01:45 PM

Quant Time: Mar 18 05:57:00 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Mar 18 05:21:28 2020
Response via : Initial Calibration

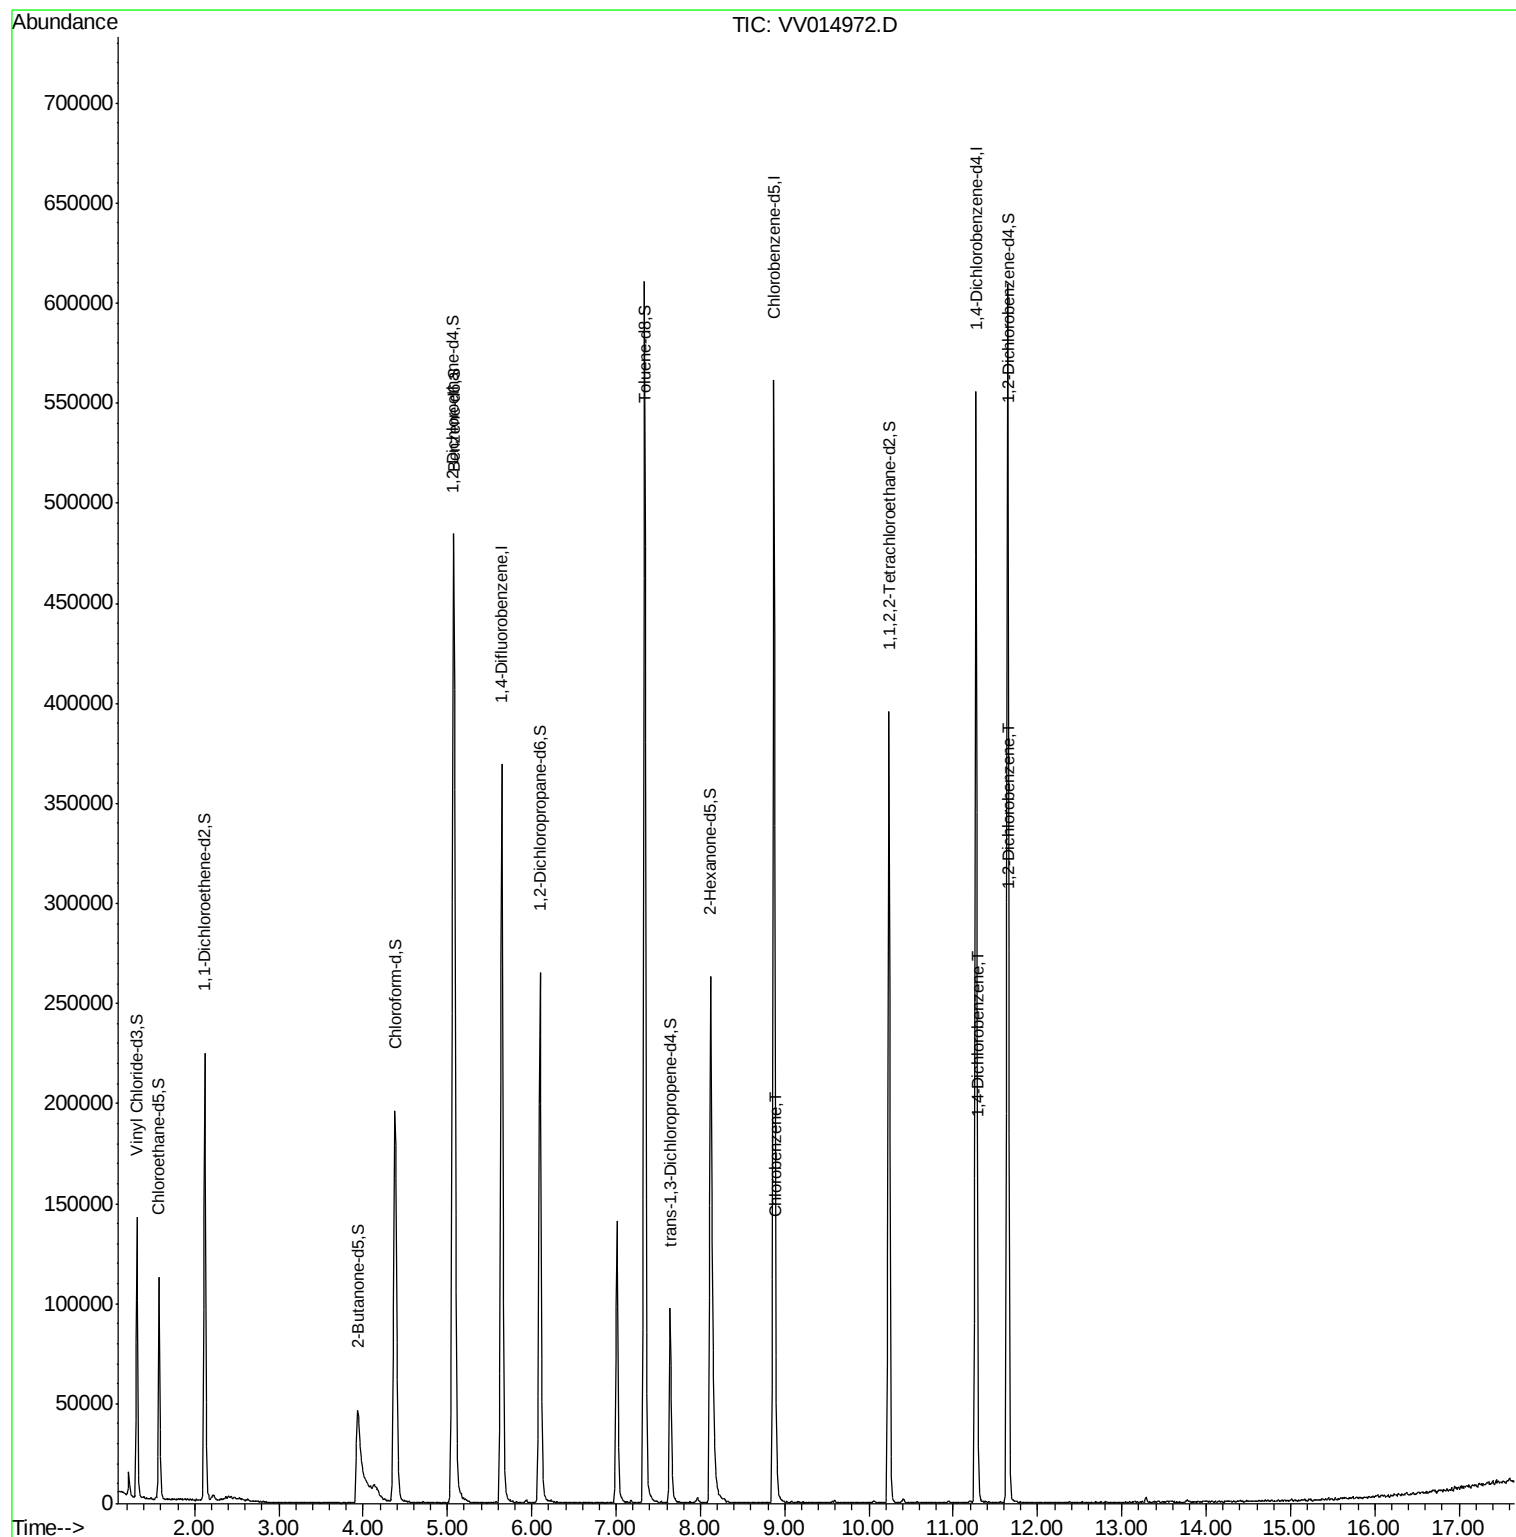

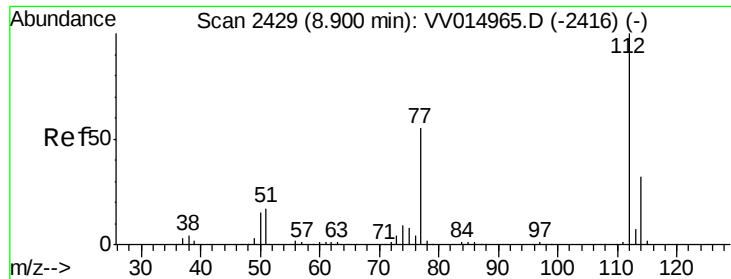





#51
Chlorobenzene
Concen: 0.931 ug/L
RT: 8.90 min Scan# 2430
Delta R.T. 0.00 min
Lab File: VV014972.D
Acq: 17 Mar 2020 14:35

Instrument :
MSVOA_V
ClientSampled :
C0D91

Tot Ion	Ratio	Lower	Upper
112	100		
114	32.5	22.8	42.4
77	52.6	44.5	66.7




Manual Integrations
APPROVED


apatel
3/18/2020 3:01:45 PM

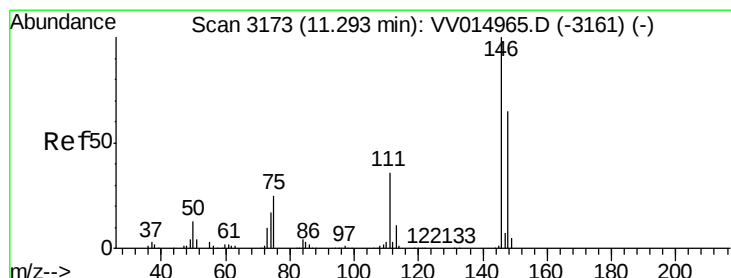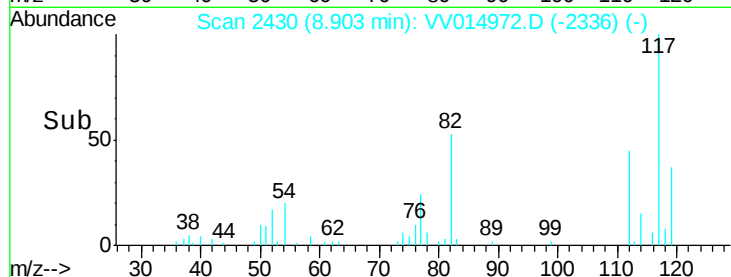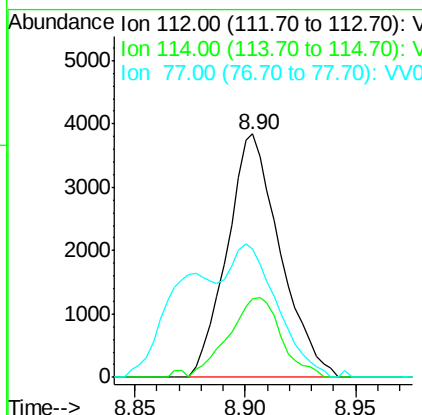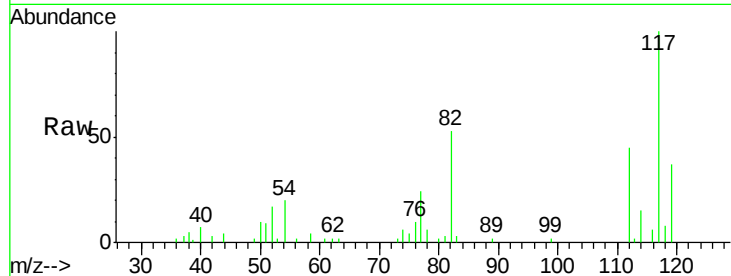

#63
1,4-Dichlorobenzene
Concen: 0.919 ug/L
RT: 11.30 min Scan# 3174
Delta R.T. 0.00 min
Lab File: VV014972.D
Acq: 17 Mar 2020 14:35

Tgt Ion	Ratio	Lower	Upper
146	100		
111	39.8	26.0	48.2
148	59.5	46.1	85.5

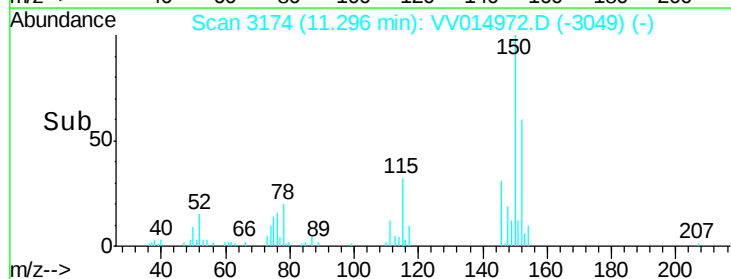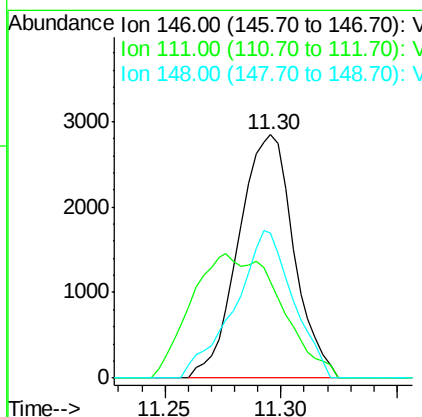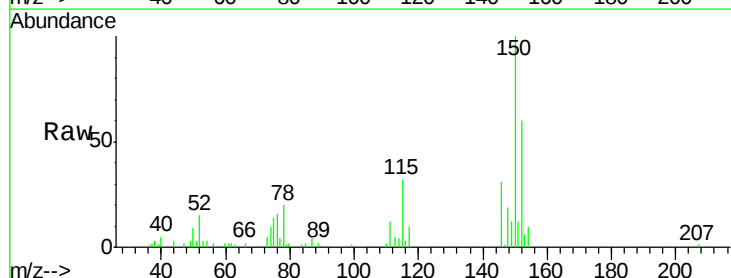

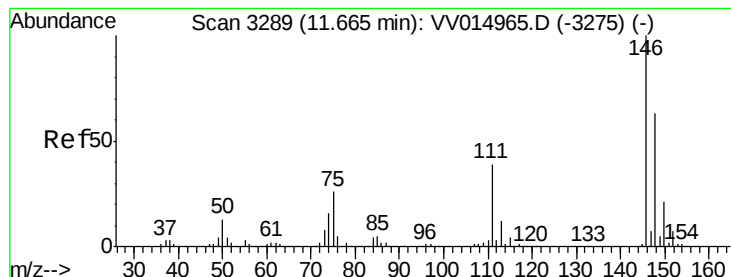

#65
 1,2-Dichlorobenzene
 Concen: 0.692 ug/L
 RT: 11.67 min Scan# 3290
 Delta R.T. 0.00 min
 Lab File: VV014972.D
 Acq: 17 Mar 2020 14:35

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D91

Tot Ion	Ratio	Lower	Upper
146	100		
111	52.2	31.6	47.4#
148	66.3	52.2	78.4

Manual Integrations
 APPROVED

apatel
 3/18/2020 3:01:45 PM

