

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031720\
 Data File : VV014972.D
 Acq On : 17 Mar 2020 14:35
 Operator : SY/MD
 Sample : L1940-04
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D91

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	86	rVB	139745	148873	12.28%	1.604%
2	1.579	145	152	169	rVB	111206	134977	11.13%	1.454%
3	2.122	310	321	332	rBV	223620	320599	26.44%	3.454%
4	2.801	529	532	533	rBV2	430	215	0.02%	0.002%
5	2.997	590	593	596	rBV	238	158	0.01%	0.002%
6	3.235	663	667	669	rBV2	263	175	0.01%	0.002%
7	3.524	754	757	760	rVV2	186	135	0.01%	0.001%
8	3.637	789	792	797	rVV2	268	226	0.02%	0.002%
9	3.714	813	816	823	rVB2	381	279	0.02%	0.003%
10	3.826	846	851	853	rBV	211	207	0.02%	0.002%
11	3.936	870	885	915	rBV2	46591	189855	15.66%	2.045%
12	4.380	1007	1023	1054	rVB	194998	491809	40.56%	5.298%
13	4.637	1101	1103	1106	rBV2	200	141	0.01%	0.002%
14	4.711	1122	1126	1133	rVB3	663	633	0.05%	0.007%
15	4.868	1172	1175	1178	rBV2	242	172	0.01%	0.002%
16	4.945	1195	1199	1200	rBV	207	136	0.01%	0.001%
17	4.994	1211	1214	1219	rBV2	382	355	0.03%	0.004%
18	5.074	1221	1239	1263	rBV2	484134	1212622	100.00%	13.064%
19	5.309	1309	1312	1318	rVB4	353	262	0.02%	0.003%
20	5.424	1345	1348	1351	rBV2	376	217	0.02%	0.002%
21	5.486	1365	1367	1370	rBV	309	167	0.01%	0.002%
22	5.498	1370	1371	1373	rBV	366	166	0.01%	0.002%
23	5.643	1403	1416	1442	rBV	368547	728826	60.10%	7.852%
24	5.916	1496	1501	1502	rBV4	937	728	0.06%	0.008%
25	6.096	1542	1557	1581	rBV	264925	535586	44.17%	5.770%
26	6.299	1618	1620	1623	rVB3	421	178	0.01%	0.002%
27	6.399	1648	1651	1655	rVB	343	225	0.02%	0.002%
28	6.428	1655	1660	1663	rVB2	294	260	0.02%	0.003%
29	6.450	1663	1667	1668	rBV	267	160	0.01%	0.002%
30	6.566	1700	1703	1706	rVV2	372	258	0.02%	0.003%
31	6.627	1717	1722	1723	rBV	305	184	0.02%	0.002%
32	6.746	1754	1759	1764	rBV3	287	249	0.02%	0.003%
33	6.772	1764	1767	1771	rBV	442	259	0.02%	0.003%
34	6.916	1806	1812	1815	rBV2	254	267	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031720\
 Data File : VV014972.D
 Acq On : 17 Mar 2020 14:35
 Operator : SY/MD
 Sample : L1940-04
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D91

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
 Title : VOC Analysis

35	7.010	1828	1841	1857	rBV2	140569	249483	20.57%	2.688%
36	7.135	1878	1880	1882	rBV3	403	146	0.01%	0.002%
37	7.180	1888	1894	1900	rBV5	1143	1444	0.12%	0.016%
38	7.235	1906	1911	1914	rVB2	323	293	0.02%	0.003%
39	7.277	1920	1924	1925	rBV2	315	195	0.02%	0.002%
40	7.338	1931	1943	1967	rBV	610034	1050168	86.60%	11.314%
41	7.601	2023	2025	2026	rBV	411	193	0.02%	0.002%
42	7.643	2028	2038	2066	rVV	96980	169504	13.98%	1.826%
43	7.762	2073	2075	2078	rBV	319	140	0.01%	0.002%
44	7.813	2088	2091	2092	rBV2	422	164	0.01%	0.002%
45	7.842	2098	2100	2103	rBV2	354	240	0.02%	0.003%
46	7.878	2110	2111	2114	rVB	677	200	0.02%	0.002%
47	7.903	2114	2119	2120	rBV	224	146	0.01%	0.002%
48	7.916	2120	2123	2125	rBV3	328	210	0.02%	0.002%
49	7.936	2125	2129	2130	rBV2	563	367	0.03%	0.004%
50	8.074	2169	2172	2175	rBV2	210	146	0.01%	0.002%
51	8.122	2175	2187	2218	rBV3	262775	613810	50.62%	6.613%
52	8.402	2271	2274	2275	rBV	332	142	0.01%	0.002%
53	8.421	2275	2280	2282	rBV	289	251	0.02%	0.003%
54	8.547	2317	2319	2323	rBV2	346	162	0.01%	0.002%
55	8.569	2323	2326	2329	rVB2	311	169	0.01%	0.002%
56	8.704	2362	2368	2374	rBV3	444	620	0.05%	0.007%
57	8.781	2389	2392	2396	rVB	285	214	0.02%	0.002%
58	8.810	2399	2401	2403	rBV	352	169	0.01%	0.002%
59	8.874	2408	2421	2441	rBV	560974	931212	76.79%	10.032%
60	9.022	2464	2467	2469	rBV2	575	387	0.03%	0.004%
61	9.084	2482	2486	2489	rBV2	767	585	0.05%	0.006%
62	9.154	2505	2508	2509	rBV	696	414	0.03%	0.004%
63	9.193	2519	2520	2526	rVB2	504	286	0.02%	0.003%
64	9.222	2526	2529	2531	rVB	780	378	0.03%	0.004%
65	9.254	2535	2539	2542	rBV2	220	176	0.01%	0.002%
66	9.325	2556	2561	2563	rBV	245	213	0.02%	0.002%
67	9.421	2588	2591	2592	rBV	334	136	0.01%	0.001%
68	9.752	2691	2694	2696	rBV2	359	197	0.02%	0.002%
69	9.797	2705	2708	2710	rBV2	320	181	0.01%	0.002%
70	9.852	2723	2725	2727	rBV2	320	148	0.01%	0.002%
71	9.894	2735	2738	2741	rBV	368	201	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031720\
 Data File : VV014972.D
 Acq On : 17 Mar 2020 14:35
 Operator : SY/MD
 Sample : L1940-04
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D91

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
 Title : VOC Analysis

72	9.955	2753	2757	2761	rBV2	477	403	0.03%	0.004%
73	10.029	2778	2780	2782	rBV	256	157	0.01%	0.002%
74	10.051	2782	2787	2789	rBV3	830	763	0.06%	0.008%
75	10.122	2806	2809	2811	rBV2	193	142	0.01%	0.002%
76	10.238	2832	2845	2863	rBV	395137	627033	51.71%	6.755%
77	10.328	2871	2873	2877	rVB2	386	209	0.02%	0.002%
78	10.402	2888	2896	2905	rBV7	2278	4095	0.34%	0.044%
79	10.485	2918	2922	2924	rBV	263	152	0.01%	0.002%
80	10.540	2935	2939	2941	rBV2	383	303	0.02%	0.003%
81	10.569	2944	2948	2954	rBV3	630	694	0.06%	0.007%
82	10.775	3009	3012	3016	rVB	403	310	0.03%	0.003%
83	10.820	3023	3026	3029	rBV2	355	269	0.02%	0.003%
84	11.045	3093	3096	3100	rBV2	186	173	0.01%	0.002%
85	11.186	3137	3140	3142	rBV3	527	380	0.03%	0.004%
86	11.270	3154	3166	3185	rBV	555382	874078	72.08%	9.416%
87	11.646	3270	3283	3305	rBV	609007	974057	80.33%	10.494%
88	11.810	3332	3334	3338	rBV2	322	272	0.02%	0.003%
89	11.907	3362	3364	3367	rVB2	364	207	0.02%	0.002%
90	12.038	3403	3405	3408	rBV	425	205	0.02%	0.002%
91	12.231	3463	3465	3469	rVB2	393	197	0.02%	0.002%
92	12.347	3497	3501	3502	rBV2	261	197	0.02%	0.002%
93	12.675	3598	3603	3605	rBV3	412	389	0.03%	0.004%
94	12.688	3605	3607	3609	rBV2	401	190	0.02%	0.002%
95	12.804	3641	3643	3646	rBV	344	203	0.02%	0.002%
96	12.878	3664	3666	3669	rBV2	309	211	0.02%	0.002%
97	13.042	3715	3717	3721	rVB2	349	172	0.01%	0.002%
98	13.128	3740	3744	3747	rBV3	504	392	0.03%	0.004%
99	13.286	3786	3793	3798	rBV4	2757	3539	0.29%	0.038%
100	13.357	3810	3815	3817	rBV2	454	386	0.03%	0.004%


Sum of corrected areas: 9282427

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV031720\
Data File : VV014972.D
Acq On : 17 Mar 2020 14:35
Operator : SY/MD
Sample : L1940-04
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0D91

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

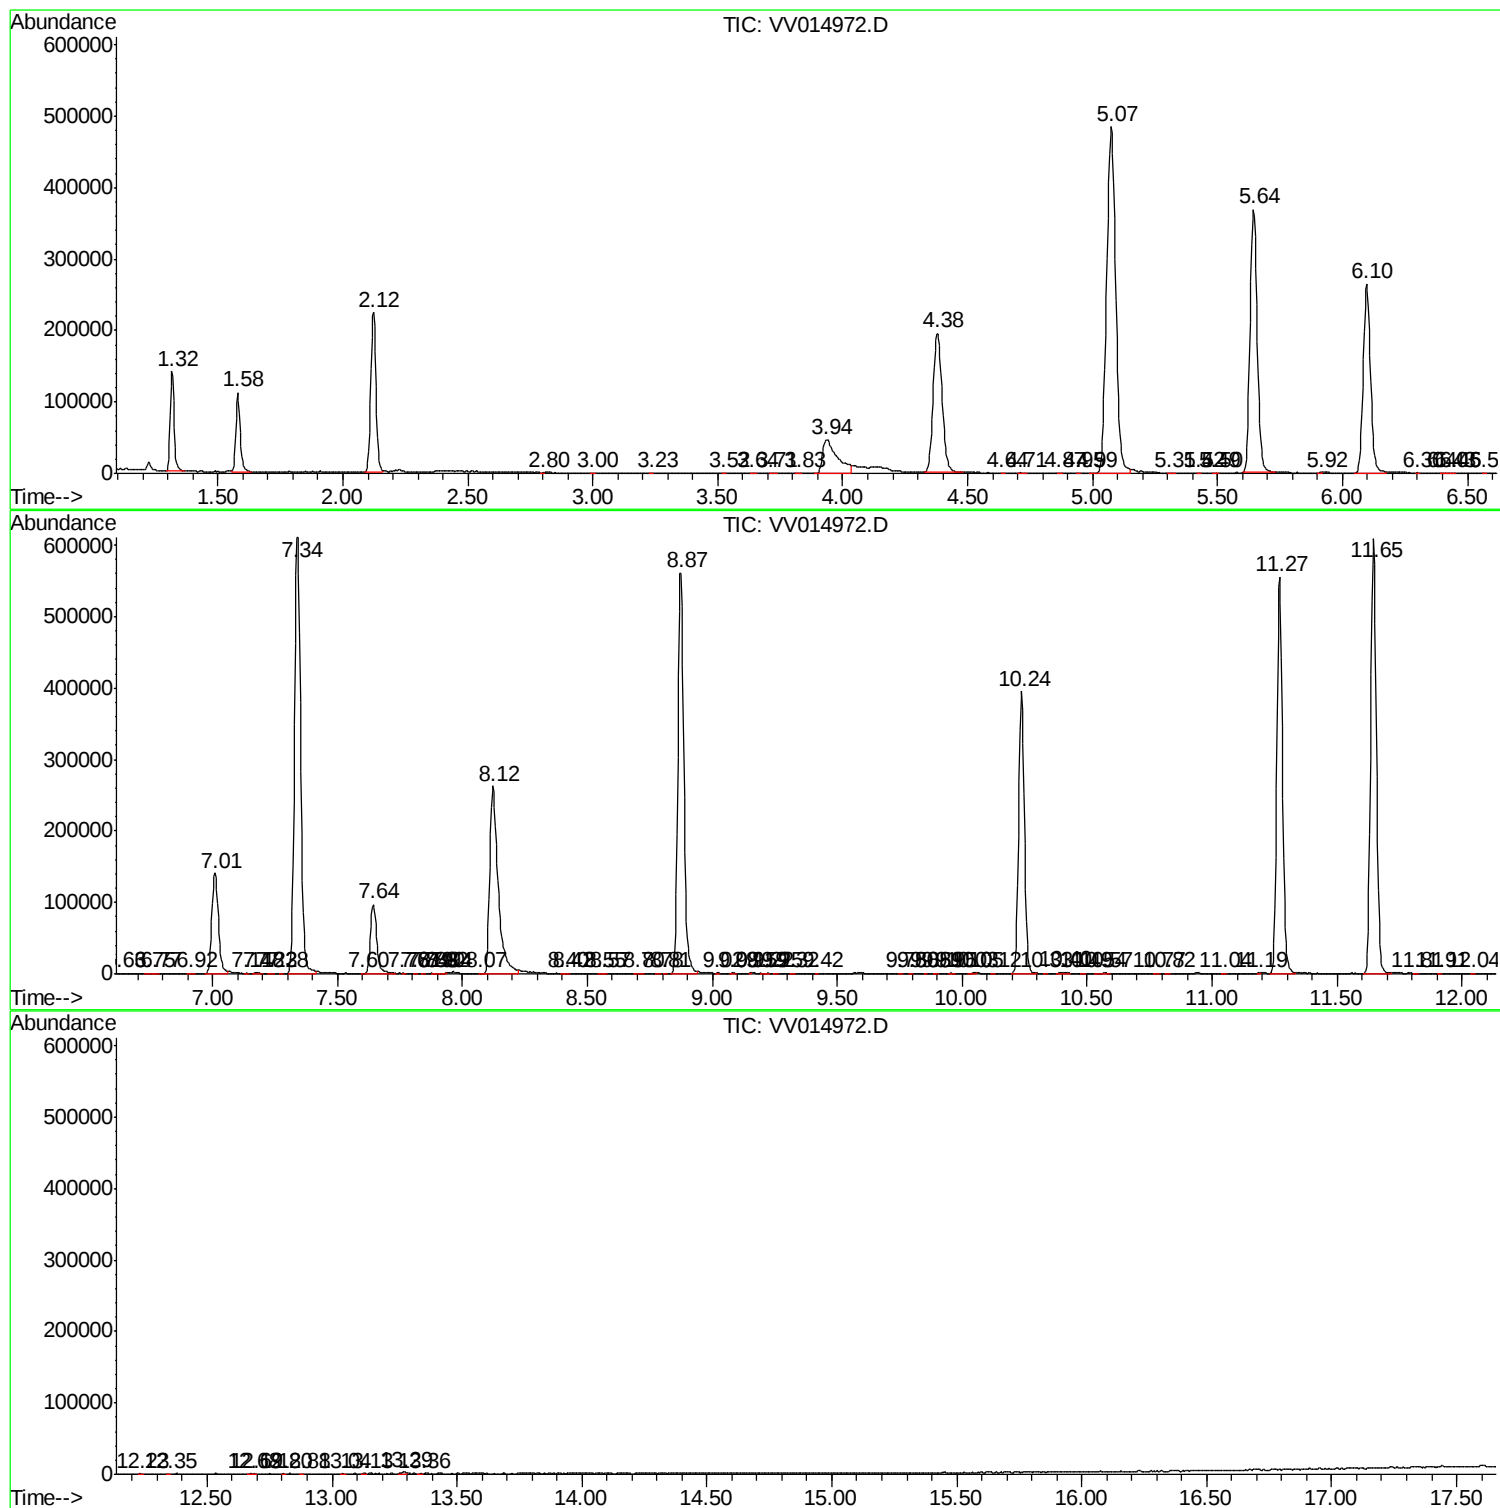

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV031720\
Data File : VV014972.D
Acq On : 17 Mar 2020 14:35
Operator : SY/MD
Sample : L1940-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0D91

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV031720\
Data File : VV014972.D
Acq On : 17 Mar 2020 14:35
Operator : SY/MD
Sample : L1940-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0D91

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc