

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031720\
 Data File : VV014978.D
 Acq On : 17 Mar 2020 17:00
 Operator : SY/MD
 Sample : L1940-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D93

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	85	rVB	136882	143102	12.41%	1.621%
2	1.579	145	152	175	rVB	102035	126852	11.01%	1.437%
3	1.958	268	270	272	rBV2	819	452	0.04%	0.005%
4	2.122	311	321	339	rVB	214595	307156	26.65%	3.480%
5	3.026	599	602	604	rBV	407	223	0.02%	0.003%
6	3.145	637	639	640	rBV	212	86	0.01%	0.001%
7	3.216	657	661	662	rBV	202	134	0.01%	0.002%
8	3.409	719	721	723	rVB	246	65	0.01%	0.001%
9	3.720	815	818	820	rBV	167	95	0.01%	0.001%
10	3.762	829	831	834	rBV	281	154	0.01%	0.002%
11	3.830	849	852	853	rBV	208	124	0.01%	0.001%
12	3.933	872	884	922	rBV2	47155	200974	17.44%	2.277%
13	4.380	1007	1023	1046	rBV	186611	460224	39.93%	5.215%
14	4.511	1062	1064	1067	rBV2	551	158	0.01%	0.002%
15	4.650	1103	1107	1110	rVB2	468	360	0.03%	0.004%
16	4.666	1110	1112	1116	rBV2	344	273	0.02%	0.003%
17	4.794	1150	1152	1155	rBV	303	162	0.01%	0.002%
18	4.843	1165	1167	1169	rBV2	269	111	0.01%	0.001%
19	4.900	1183	1185	1186	rVB2	312	96	0.01%	0.001%
20	4.923	1186	1192	1194	rBV2	355	318	0.03%	0.004%
21	5.074	1221	1239	1266	rBV2	454414	1152665	100.00%	13.060%
22	5.373	1330	1332	1334	rBV3	387	192	0.02%	0.002%
23	5.425	1345	1348	1349	rBV	363	160	0.01%	0.002%
24	5.643	1402	1416	1449	rBV	361045	713305	61.88%	8.082%
25	5.923	1499	1503	1504	rBV2	1212	739	0.06%	0.008%
26	6.010	1528	1530	1531	rBV2	192	92	0.01%	0.001%
27	6.019	1531	1533	1536	rVB	307	143	0.01%	0.002%
28	6.096	1542	1557	1581	rBV	250234	512101	44.43%	5.802%
29	6.244	1600	1603	1605	rBV3	515	341	0.03%	0.004%
30	6.283	1612	1615	1616	rBV	205	122	0.01%	0.001%
31	6.402	1646	1652	1655	rBV2	405	341	0.03%	0.004%
32	6.421	1655	1658	1661	rVB2	290	165	0.01%	0.002%
33	6.463	1669	1671	1673	rBV	193	66	0.01%	0.001%
34	6.627	1720	1722	1723	rBV	261	96	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031720\
 Data File : VV014978.D
 Acq On : 17 Mar 2020 17:00
 Operator : SY/MD
 Sample : L1940-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D93

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
 Title : VOC Analysis

35	6.723	1749	1752	1753	rBV	152	107	0.01%	0.001%
36	6.778	1766	1769	1770	rBV	237	146	0.01%	0.002%
37	6.887	1798	1803	1805	rBV2	341	318	0.03%	0.004%
38	7.010	1829	1841	1863	rBV	129636	234459	20.34%	2.657%
39	7.206	1898	1902	1903	rBV	299	209	0.02%	0.002%
40	7.235	1908	1911	1915	rVV2	445	307	0.03%	0.003%
41	7.267	1919	1921	1923	rBV	286	117	0.01%	0.001%
42	7.341	1930	1944	1960	rBV	562198	986693	85.60%	11.180%
43	7.643	2025	2038	2065	rBV	90343	160688	13.94%	1.821%
44	7.904	2116	2119	2121	rBV	275	192	0.02%	0.002%
45	7.926	2124	2126	2128	rBV	217	87	0.01%	0.001%
46	7.958	2131	2136	2143	rVV5	1427	2282	0.20%	0.026%
47	8.022	2154	2156	2159	rBV	242	111	0.01%	0.001%
48	8.122	2174	2187	2222	rBV2	256834	585460	50.79%	6.634%
49	8.492	2300	2302	2303	rBV	204	67	0.01%	0.001%
50	8.518	2308	2310	2311	rBV	466	136	0.01%	0.002%
51	8.662	2352	2355	2357	rBV	348	200	0.02%	0.002%
52	8.765	2383	2387	2389	rBV	384	319	0.03%	0.004%
53	8.875	2408	2421	2444	rBV	540477	880677	76.40%	9.979%
54	9.122	2495	2498	2501	rVB2	403	201	0.02%	0.002%
55	9.492	2611	2613	2615	rBV	284	72	0.01%	0.001%
56	9.556	2632	2633	2634	rBV	309	110	0.01%	0.001%
57	10.055	2787	2788	2789	rBV	286	86	0.01%	0.001%
58	10.186	2826	2829	2830	rBV	230	140	0.01%	0.002%
59	10.238	2832	2845	2861	rVV	382773	600652	52.11%	6.806%
60	10.408	2889	2898	2905	rBV2	2516	3915	0.34%	0.044%
61	11.270	3155	3166	3185	rBV	538461	829680	71.98%	9.401%
62	11.646	3271	3283	3302	rBV	585072	915157	79.39%	10.369%
63	11.890	3357	3359	3361	rVB	410	159	0.01%	0.002%
64	12.019	3396	3399	3402	rBV2	262	157	0.01%	0.002%
65	12.032	3402	3403	3404	rBV2	247	58	0.01%	0.001%
66	12.472	3538	3540	3542	rBV	288	144	0.01%	0.002%
67	12.633	3588	3590	3592	rBV	381	141	0.01%	0.002%
68	13.276	3787	3790	3792	rBV3	1016	687	0.06%	0.008%


Sum of corrected areas: 8825581

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV031720\
Data File : VV014978.D
Acq On : 17 Mar 2020 17:00
Operator : SY/MD
Sample : L1940-06
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0D93

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

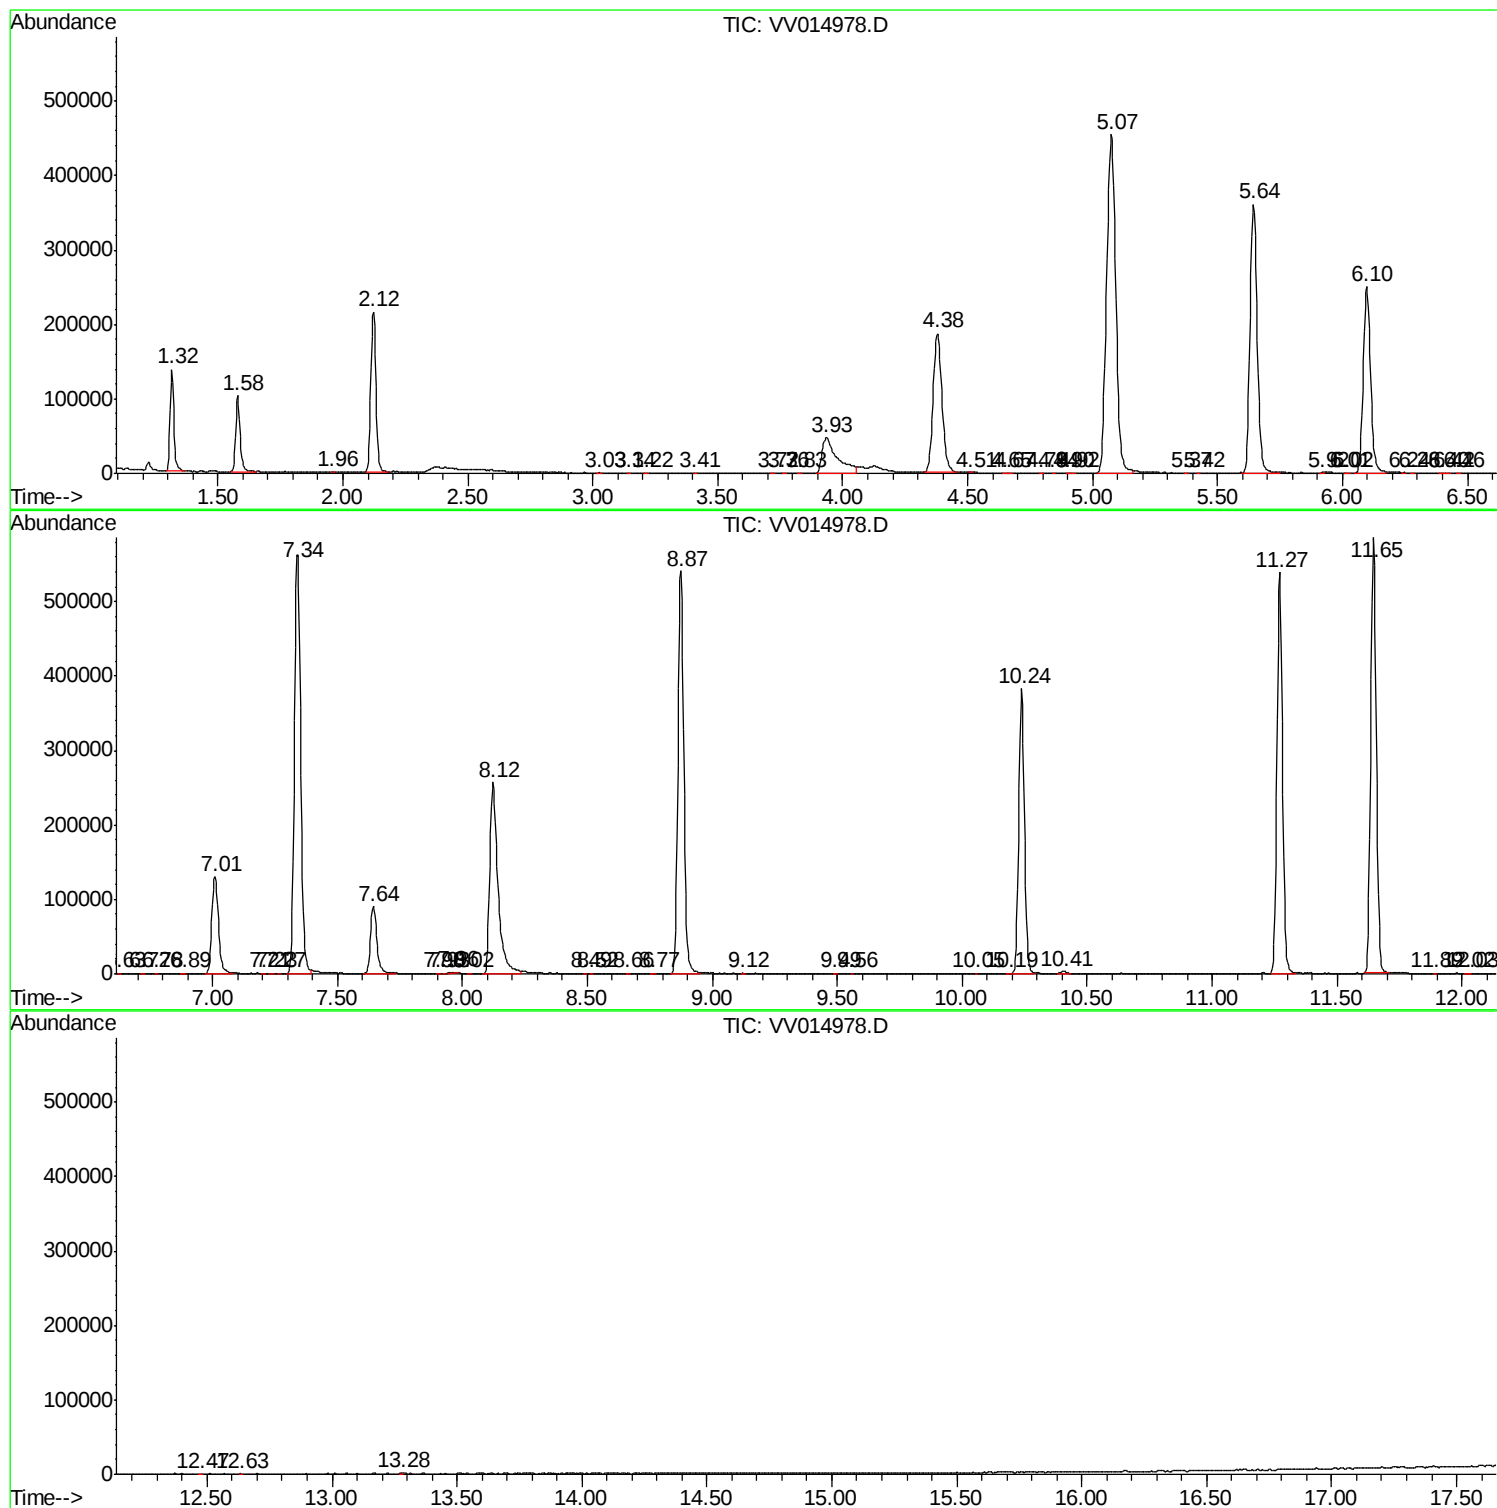

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV031720\
Data File : VV014978.D
Acq On : 17 Mar 2020 17:00
Operator : SY/MD
Sample : L1940-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0D93

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV031720\
Data File : VV014978.D
Acq On : 17 Mar 2020 17:00
Operator : SY/MD
Sample : L1940-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0D93

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc