

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031720\
 Data File : VV014984.D
 Acq On : 17 Mar 2020 19:25
 Operator : SY/MD
 Sample : L1941-02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DA3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	87	rVB	132993	142477	12.05%	1.565%
2	1.579	144	152	169	rVB	102684	126461	10.69%	1.389%
3	2.122	311	321	341	rVB	221340	312593	26.44%	3.434%
4	3.052	608	610	613	rBV2	418	221	0.02%	0.002%
5	3.129	631	634	637	rBV3	398	189	0.02%	0.002%
6	3.183	648	651	654	rVB2	255	162	0.01%	0.002%
7	3.209	656	659	661	rBV	182	120	0.01%	0.001%
8	3.261	673	675	676	rBV	362	173	0.01%	0.002%
9	3.331	695	697	700	rBV	185	146	0.01%	0.002%
10	3.518	753	755	760	rVB2	279	171	0.01%	0.002%
11	3.637	789	792	793	rBV	85	45	0.00%	0.000%
12	3.663	796	800	803	rBV2	342	215	0.02%	0.002%
13	3.714	813	816	820	rBV2	296	194	0.02%	0.002%
14	3.785	834	838	843	rBV2	204	207	0.02%	0.002%
15	3.933	871	884	911	rBV2	47509	185853	15.72%	2.042%
16	4.380	1007	1023	1048	rBV2	193712	477494	40.38%	5.246%
17	4.537	1070	1072	1080	rBV4	593	514	0.04%	0.006%
18	4.627	1098	1100	1105	rBV2	350	228	0.02%	0.003%
19	4.646	1105	1106	1109	rVB	399	138	0.01%	0.002%
20	4.682	1112	1117	1120	rVV3	362	361	0.03%	0.004%
21	4.711	1123	1126	1127	rVV2	385	122	0.01%	0.001%
22	4.730	1127	1132	1134	rVV2	371	310	0.03%	0.003%
23	4.753	1137	1139	1141	rVB2	429	155	0.01%	0.002%
24	4.785	1147	1149	1153	rBV2	319	191	0.02%	0.002%
25	4.807	1153	1156	1157	rBV2	283	160	0.01%	0.002%
26	4.849	1168	1169	1171	rBV2	197	91	0.01%	0.001%
27	4.900	1183	1185	1189	rBV	115	76	0.01%	0.001%
28	4.917	1189	1190	1191	rVB	113	22	0.00%	0.000%
29	4.939	1196	1197	1198	rBV	163	44	0.00%	0.000%
30	4.958	1198	1203	1207	rBV2	251	257	0.02%	0.003%
31	5.074	1221	1239	1262	rBV2	468863	1182485	100.00%	12.992%
32	5.347	1323	1324	1326	rBV	328	186	0.02%	0.002%
33	5.415	1341	1345	1349	rBV	350	343	0.03%	0.004%
34	5.544	1382	1385	1388	rBV3	438	324	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031720\
 Data File : VV014984.D
 Acq On : 17 Mar 2020 19:25
 Operator : SY/MD
 Sample : L1941-02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DA3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
 Title : VOC Analysis

35	5.643	1403	1416	1444	rBV	371297	743403	62.87%	8.168%
36	5.913	1498	1500	1503	rBV2	885	759	0.06%	0.008%
37	5.978	1518	1520	1523	rBV	245	107	0.01%	0.001%
38	6.000	1523	1527	1529	rVB2	525	322	0.03%	0.004%
39	6.016	1529	1532	1533	rBV	259	150	0.01%	0.002%
40	6.097	1543	1557	1582	rBV	257042	523411	44.26%	5.751%
41	6.328	1627	1629	1631	rBV	219	93	0.01%	0.001%
42	6.408	1653	1654	1656	rBV	377	124	0.01%	0.001%
43	6.444	1663	1665	1667	rBV	373	146	0.01%	0.002%
44	6.650	1726	1729	1730	rBV	215	117	0.01%	0.001%
45	7.010	1829	1841	1867	rBV	132647	238568	20.18%	2.621%
46	7.161	1885	1888	1889	rBV2	782	385	0.03%	0.004%
47	7.235	1909	1911	1912	rBV	309	98	0.01%	0.001%
48	7.248	1912	1915	1920	rVV3	482	461	0.04%	0.005%
49	7.270	1920	1922	1926	rVB2	311	132	0.01%	0.001%
50	7.338	1930	1943	1971	rBV	576535	1010715	85.47%	11.105%
51	7.466	1981	1983	1989	rBV3	647	541	0.05%	0.006%
52	7.563	2010	2013	2016	rBV3	271	201	0.02%	0.002%
53	7.643	2022	2038	2064	rBV	93233	164042	13.87%	1.802%
54	7.781	2079	2081	2087	rVB2	513	417	0.04%	0.005%
55	7.817	2087	2092	2096	rBV3	414	438	0.04%	0.005%
56	7.865	2106	2107	2109	rBV	135	52	0.00%	0.001%
57	8.006	2150	2151	2155	rVB	227	96	0.01%	0.001%
58	8.122	2175	2187	2219	rBV2	270796	606992	51.33%	6.669%
59	8.363	2260	2262	2263	rBV	300	104	0.01%	0.001%
60	8.405	2273	2275	2277	rBV	416	214	0.02%	0.002%
61	8.608	2335	2338	2339	rBV	289	165	0.01%	0.002%
62	8.772	2388	2389	2390	rBB	202	39	0.00%	0.000%
63	8.871	2406	2420	2454	rBV	556286	927581	78.44%	10.191%
64	9.090	2484	2488	2495	rVB2	943	980	0.08%	0.011%
65	9.122	2495	2498	2503	rBV2	588	527	0.04%	0.006%
66	9.154	2503	2508	2510	rBV2	687	545	0.05%	0.006%
67	9.183	2516	2517	2519	rVB	297	66	0.01%	0.001%
68	9.331	2560	2563	2564	rBV	246	105	0.01%	0.001%
69	9.576	2634	2639	2645	rBV3	438	617	0.05%	0.007%
70	9.688	2672	2674	2675	rBV	163	48	0.00%	0.001%
71	9.733	2685	2688	2689	rBV	230	128	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031720\
 Data File : VV014984.D
 Acq On : 17 Mar 2020 19:25
 Operator : SY/MD
 Sample : L1941-02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DA3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
 Title : VOC Analysis

72	10.145	2814	2816	2818	rBV2	275	150	0.01%	0.002%
73	10.238	2833	2845	2863	rBV	394297	611275	51.69%	6.716%
74	10.450	2908	2911	2912	rBV	279	162	0.01%	0.002%
75	10.556	2942	2944	2945	rBV	299	115	0.01%	0.001%
76	10.640	2968	2970	2973	rVB	285	106	0.01%	0.001%
77	10.688	2982	2985	2989	rBV3	289	221	0.02%	0.002%
78	10.833	3025	3030	3033	rBV2	251	190	0.02%	0.002%
79	10.939	3059	3063	3068	rBV3	585	639	0.05%	0.007%
80	11.270	3154	3166	3187	rBV	568481	873294	73.85%	9.595%
81	11.514	3240	3242	3246	rBV2	488	183	0.02%	0.002%
82	11.646	3270	3283	3304	rBV	607623	954562	80.73%	10.488%
83	12.029	3400	3402	3404	rBV	211	88	0.01%	0.001%
84	12.116	3425	3429	3432	rVB2	503	346	0.03%	0.004%
85	12.161	3440	3443	3445	rBV	547	267	0.02%	0.003%
86	12.399	3515	3517	3519	rBV	279	130	0.01%	0.001%
87	12.608	3580	3582	3585	rBV2	313	164	0.01%	0.002%
88	12.665	3598	3600	3602	rBV2	285	155	0.01%	0.002%
89	12.868	3661	3663	3669	rVB2	562	383	0.03%	0.004%
90	12.923	3677	3680	3687	rBV3	345	391	0.03%	0.004%
91	13.035	3713	3715	3721	rBV2	345	303	0.03%	0.003%
92	13.064	3721	3724	3727	rVV2	428	263	0.02%	0.003%
93	13.292	3786	3795	3802	rBV7	1096	1979	0.17%	0.022%
94	14.620	4204	4208	4212	rBV3	766	805	0.07%	0.009%


Sum of corrected areas: 9101788

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV031720\
Data File : VV014984.D
Acq On : 17 Mar 2020 19:25
Operator : SY/MD
Sample : L1941-02
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DA3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

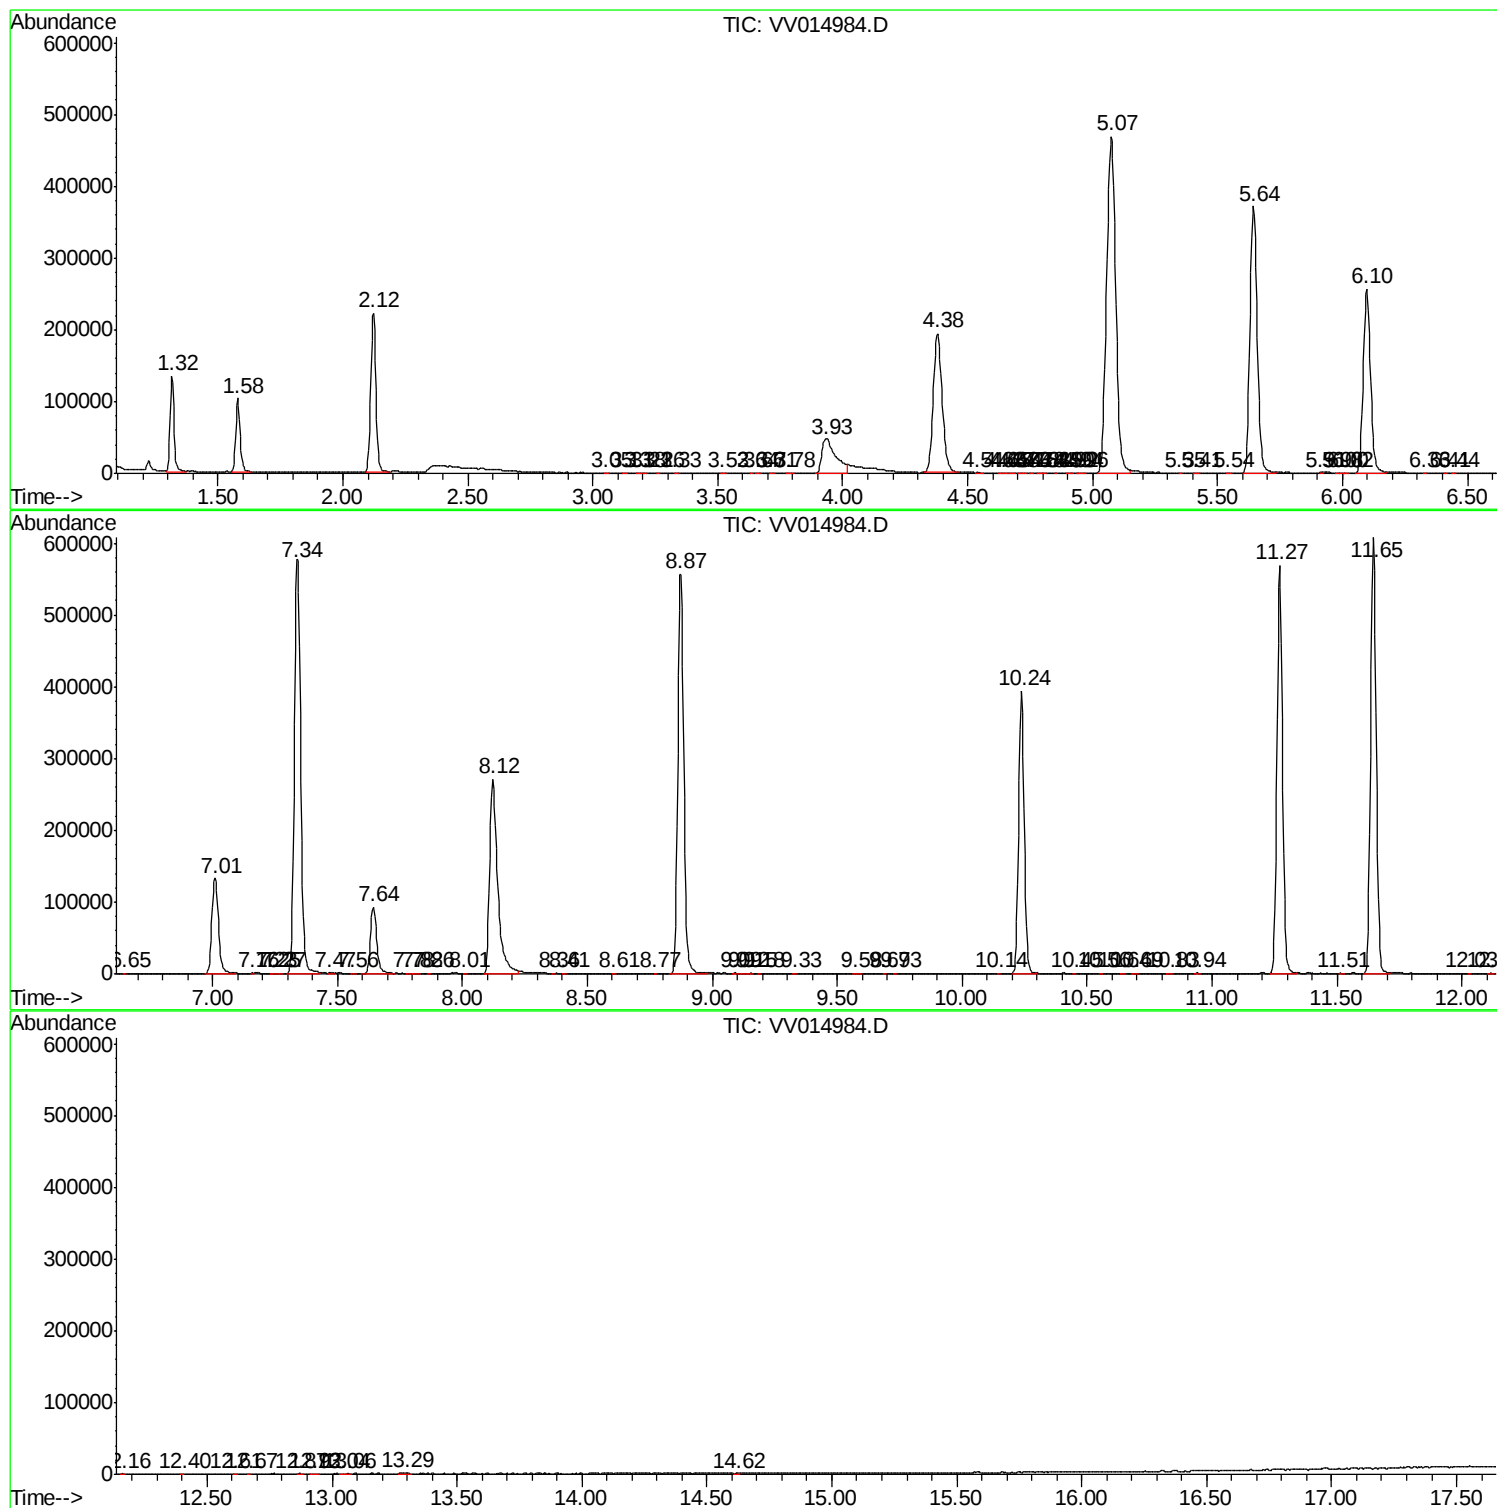

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV031720\
Data File : VV014984.D
Acq On : 17 Mar 2020 19:25
Operator : SY/MD
Sample : L1941-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DA3

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV031720\
Data File : VV014984.D
Acq On : 17 Mar 2020 19:25
Operator : SY/MD
Sample : L1941-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DA3

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc