

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031720\
 Data File : VV014987.D
 Acq On : 17 Mar 2020 20:38
 Operator : SY/MD
 Sample : L1941-05
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DB5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	83	rVB	130344	138284	0.25%	0.150%
2	1.579	145	152	164	rVB	94899	115911	0.21%	0.125%
3	1.721	188	196	202	rBV	26396	34499	0.06%	0.037%
4	1.766	203	210	220	rVB	47356	62900	0.12%	0.068%
5	2.122	310	321	336	rBV	206423	301563	0.55%	0.326%
6	2.955	578	580	582	rVB	363	155	0.00%	0.000%
7	2.978	582	587	592	rVB2	515	513	0.00%	0.001%
8	3.003	592	595	597	rBV2	449	324	0.00%	0.000%
9	3.158	640	643	644	rBV	301	146	0.00%	0.000%
10	3.267	673	677	679	rBV2	260	157	0.00%	0.000%
11	3.569	768	771	774	rBV2	199	180	0.00%	0.000%
12	3.669	799	802	804	rBV	386	175	0.00%	0.000%
13	3.743	823	825	829	rBV2	202	145	0.00%	0.000%
14	3.785	829	838	839	rBV3	1595	1560	0.00%	0.002%
15	3.926	869	882	914	rBV2	45885	184537	0.34%	0.200%
16	4.380	1005	1023	1053	rBV	184555	471065	0.87%	0.510%
17	4.627	1098	1100	1101	rBV	269	138	0.00%	0.000%
18	4.682	1115	1117	1118	rBV	364	135	0.00%	0.000%
19	4.765	1141	1143	1145	rVB	406	162	0.00%	0.000%
20	4.785	1145	1149	1150	rBV2	351	227	0.00%	0.000%
21	4.859	1160	1172	1179	rBV6	1307	2616	0.00%	0.003%
22	4.955	1200	1202	1207	rBV2	322	245	0.00%	0.000%
23	4.990	1209	1213	1215	rBV2	347	224	0.00%	0.000%
24	5.074	1220	1239	1249	rBV2	456033	1152689	2.12%	1.247%
25	5.347	1321	1324	1326	rVB3	434	252	0.00%	0.000%
26	5.515	1372	1376	1380	rVB	308	299	0.00%	0.000%
27	5.643	1402	1416	1437	rBV	372663	724137	1.33%	0.783%
28	5.855	1479	1482	1487	rBV3	381	347	0.00%	0.000%
29	5.933	1502	1506	1512	rVB5	1374	1523	0.00%	0.002%
30	5.965	1512	1516	1518	rVB2	272	204	0.00%	0.000%
31	5.981	1518	1521	1526	rVB2	320	258	0.00%	0.000%
32	6.003	1526	1528	1531	rBV2	310	160	0.00%	0.000%
33	6.035	1535	1538	1541	rBV2	417	222	0.00%	0.000%
34	6.097	1541	1557	1577	rBV	245640	506053	0.93%	0.547%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031720\
 Data File : VV014987.D
 Acq On : 17 Mar 2020 20:38
 Operator : SY/MD
 Sample : L1941-05
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DB5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
 Title : VOC Analysis

35	6.322	1624	1627	1630	rBV2	682	382	0.00%	0.000%
36	6.351	1634	1636	1638	rVV	366	185	0.00%	0.000%
37	6.386	1645	1647	1651	rVB	349	176	0.00%	0.000%
38	6.441	1662	1664	1666	rBV2	270	124	0.00%	0.000%
39	6.633	1722	1724	1727	rBV2	197	151	0.00%	0.000%
40	6.669	1732	1735	1740	rVB	325	312	0.00%	0.000%
41	6.695	1740	1743	1750	rBV2	424	338	0.00%	0.000%
42	6.762	1761	1764	1770	rBV2	279	272	0.00%	0.000%
43	6.801	1770	1776	1777	rBV2	237	189	0.00%	0.000%
44	6.933	1815	1817	1819	rVB2	374	150	0.00%	0.000%
45	7.010	1829	1841	1858	rBV	128572	231660	0.43%	0.251%
46	7.193	1896	1898	1900	rBV2	595	305	0.00%	0.000%
47	7.209	1900	1903	1906	rVB2	588	370	0.00%	0.000%
48	7.338	1930	1943	1964	rBV	584720	1004868	1.85%	1.087%
49	7.592	2019	2022	2026	rVB	453	279	0.00%	0.000%
50	7.643	2028	2038	2061	rBV	94131	159731	0.29%	0.173%
51	7.846	2098	2101	2103	rVV	342	171	0.00%	0.000%
52	7.952	2128	2134	2135	rBV2	1099	724	0.00%	0.001%
53	8.119	2174	2186	2228	rBV2	257557	579346	1.06%	0.627%
54	8.431	2280	2283	2286	rVB2	533	349	0.00%	0.000%
55	8.543	2316	2318	2321	rVB2	245	123	0.00%	0.000%
56	8.572	2325	2327	2330	rBV	279	186	0.00%	0.000%
57	8.640	2346	2348	2351	rBV	219	132	0.00%	0.000%
58	8.740	2377	2379	2382	rVB2	433	278	0.00%	0.000%
59	8.759	2382	2385	2387	rVB2	284	128	0.00%	0.000%
60	8.903	2408	2430	2455	rBV2	1878785	3898659	7.16%	4.218%
61	9.035	2464	2471	2483	rVB	12581	19688	0.04%	0.021%
62	9.135	2500	2502	2504	rBV	380	160	0.00%	0.000%
63	9.164	2504	2511	2523	rVB4	3183	6054	0.01%	0.007%
64	9.212	2523	2526	2530	rBV3	631	441	0.00%	0.000%
65	9.424	2589	2592	2594	rBV2	310	224	0.00%	0.000%
66	9.508	2615	2618	2620	rBV2	252	171	0.00%	0.000%
67	9.566	2625	2636	2647	rBV2	38052	61550	0.11%	0.067%
68	9.759	2694	2696	2698	rBV	260	143	0.00%	0.000%
69	9.849	2721	2724	2727	rVB	462	303	0.00%	0.000%
70	10.016	2773	2776	2777	rBV	272	139	0.00%	0.000%
71	10.161	2819	2821	2823	rBV	297	139	0.00%	0.000%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031720\
 Data File : VV014987.D
 Acq On : 17 Mar 2020 20:38
 Operator : SY/MD
 Sample : L1941-05
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DB5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
 Title : VOC Analysis

72	10.238	2832	2845	2865	rBV	376409	593665	1.09%	0.642%
73	10.370	2883	2886	2890	rBV4	812	721	0.00%	0.001%
74	10.559	2939	2945	2953	rVB3	1781	2198	0.00%	0.002%
75	10.720	2989	2995	3000	rBV4	648	956	0.00%	0.001%
76	10.759	3002	3007	3016	rVB2	3016	4571	0.01%	0.005%
77	10.936	3052	3062	3079	rVB	13866	20816	0.04%	0.023%
78	11.000	3080	3082	3088	rVB2	289	128	0.00%	0.000%
79	11.087	3106	3109	3113	rBV2	349	326	0.00%	0.000%
80	11.112	3116	3117	3121	rBV2	257	190	0.00%	0.000%
81	11.202	3130	3145	3157	rBV	2588217	3903533	7.17%	4.223%
82	11.302	3157	3176	3200	rVB	33490844	54427860	100.00%	58.880%
83	11.665	3271	3289	3310	rBV	9690433	15764881	28.96%	17.054%
84	12.241	3466	3468	3471	rVB	484	239	0.00%	0.000%
85	12.341	3491	3499	3505	rVB5	1311	1846	0.00%	0.002%
86	12.370	3505	3508	3510	rBV2	656	377	0.00%	0.000%
87	12.421	3514	3524	3536	rBV4	10160	17234	0.03%	0.019%
88	12.543	3560	3562	3567	rVB	498	274	0.00%	0.000%
89	12.749	3621	3626	3628	rBV2	1850	1787	0.00%	0.002%
90	12.833	3650	3652	3657	rVB4	461	347	0.00%	0.000%
91	12.855	3657	3659	3661	rBV	349	238	0.00%	0.000%
92	12.903	3668	3674	3686	rVB9	3132	4706	0.01%	0.005%
93	12.948	3686	3688	3690	rBV	392	157	0.00%	0.000%
94	13.067	3722	3725	3726	rBV2	1115	626	0.00%	0.001%
95	13.202	3765	3767	3770	rBV	333	214	0.00%	0.000%
96	13.283	3779	3792	3816	rBV	3501912	5228979	9.61%	5.657%
97	13.524	3860	3867	3877	rVB2	14998	21808	0.04%	0.024%
98	13.765	3930	3942	3957	rBV	660459	1014328	1.86%	1.097%
99	14.842	4263	4277	4292	rVB	677927	1062643	1.95%	1.150%
100	15.418	4445	4456	4476	rVB	445818	692178	1.27%	0.749%


Sum of corrected areas: 92438431

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031720\
Data File : VV014987.D
Acq On : 17 Mar 2020 20:38
Operator : SY/MD
Sample : L1941-05
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DB5

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

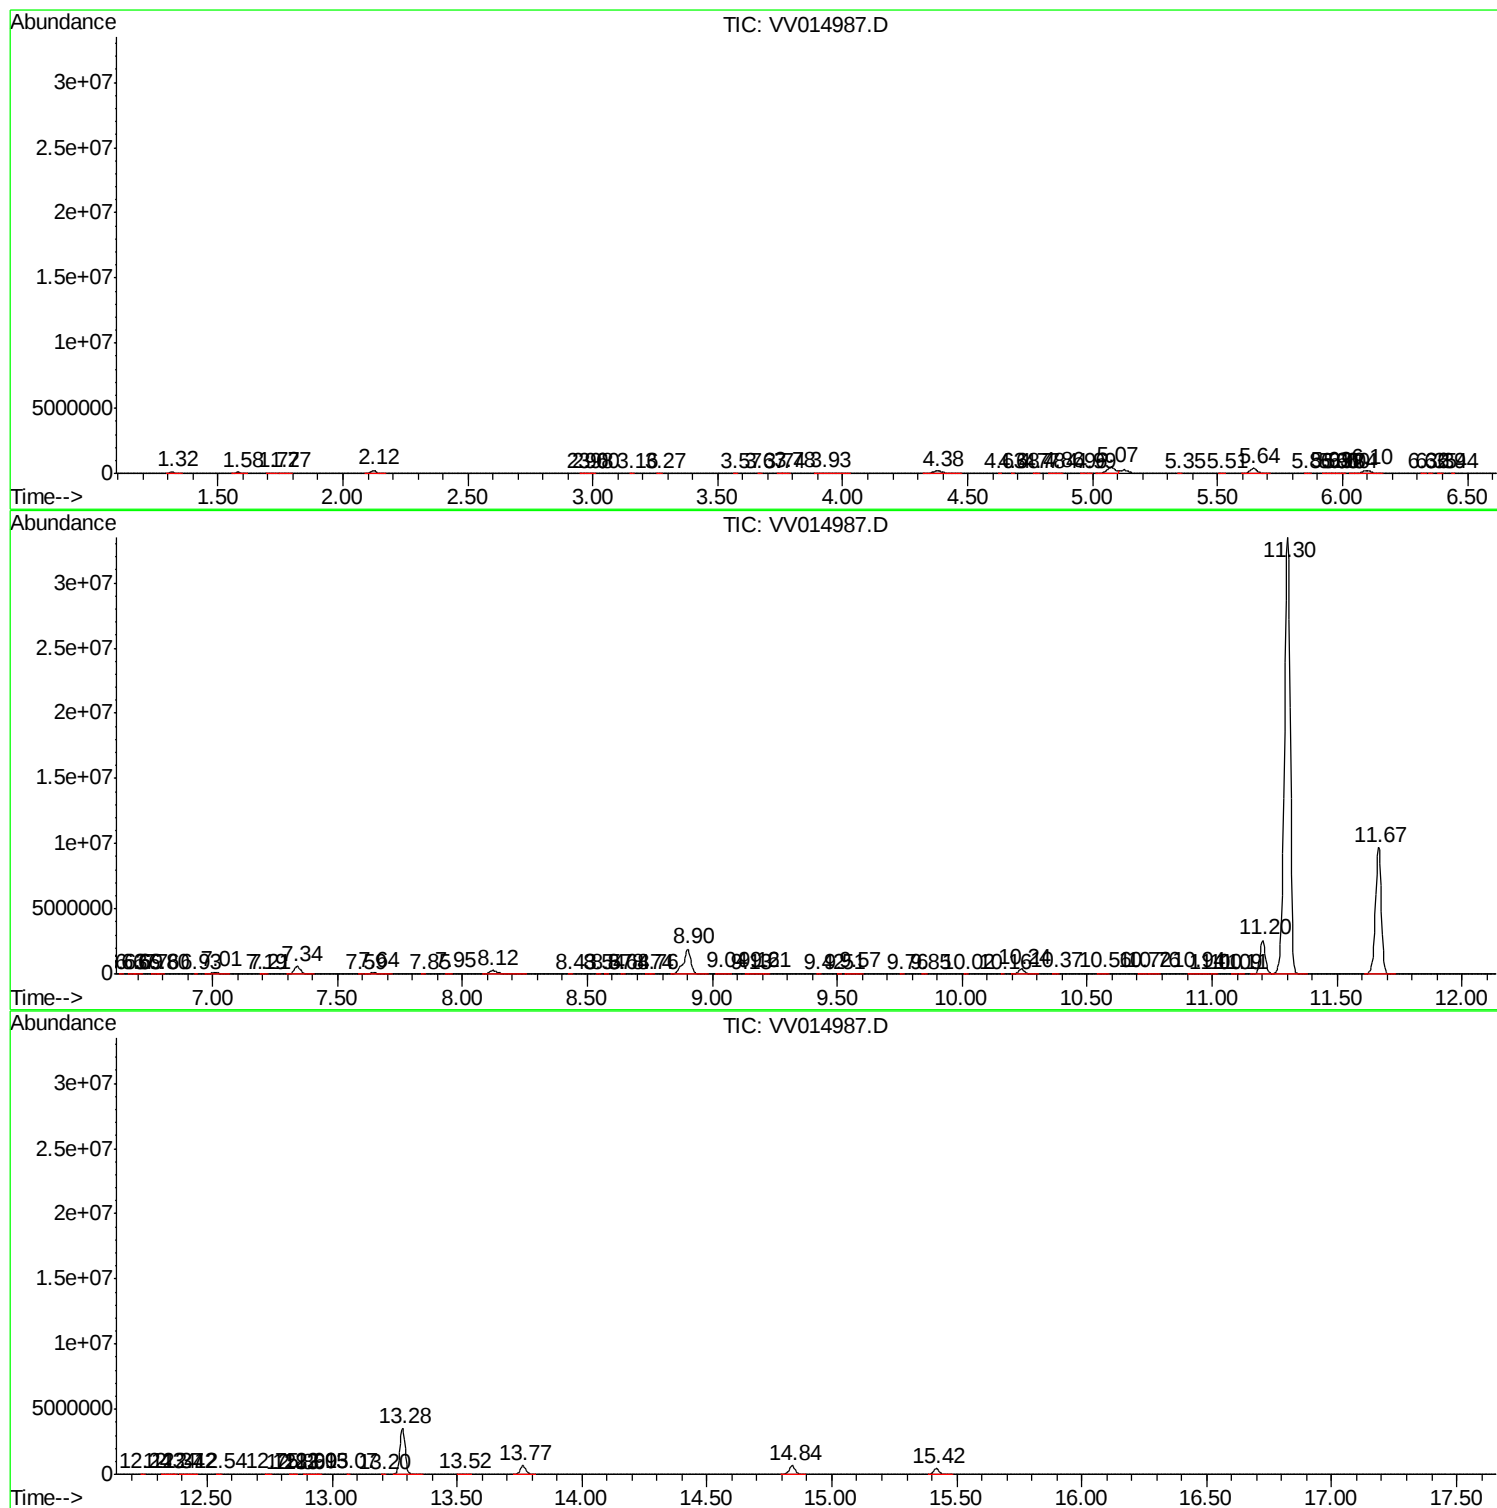

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV031720\
Data File : VV014987.D
Acq On : 17 Mar 2020 20:38
Operator : SY/MD
Sample : L1941-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DB5

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV031720\
Data File : VV014987.D
Acq On : 17 Mar 2020 20:38
Operator : SY/MD
Sample : L1941-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DB5

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc