

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031720\
 Data File : VV014988.D
 Acq On : 17 Mar 2020 21:02
 Operator : SY/MD
 Sample : L1941-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DB6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	82	rVB	128402	134676	0.09%	0.031%
2	1.579	145	152	166	rVB	96732	117465	0.08%	0.027%
3	2.122	310	321	333	rBV	207361	300579	0.20%	0.069%
4	2.299	373	376	378	rBV	671	423	0.00%	0.000%
5	2.930	569	572	576	rBV3	374	293	0.00%	0.000%
6	2.971	582	585	586	rBV2	378	233	0.00%	0.000%
7	3.065	605	614	622	rVB4	1291	2501	0.00%	0.001%
8	3.100	622	625	627	rVB2	477	277	0.00%	0.000%
9	3.116	627	630	633	rBV	323	220	0.00%	0.000%
10	3.132	633	635	639	rBV2	204	132	0.00%	0.000%
11	3.151	639	641	647	rBV2	270	195	0.00%	0.000%
12	3.212	657	660	664	rBV	224	154	0.00%	0.000%
13	3.238	664	668	670	rVB2	323	187	0.00%	0.000%
14	3.438	727	730	732	rBV2	228	169	0.00%	0.000%
15	3.486	739	745	748	rBV2	318	402	0.00%	0.000%
16	3.589	773	777	779	rBV2	293	193	0.00%	0.000%
17	3.656	795	798	801	rBV2	258	181	0.00%	0.000%
18	3.791	825	840	859	rVB4	13117	31328	0.02%	0.007%
19	3.872	860	865	867	rBV	180	164	0.00%	0.000%
20	3.933	871	884	915	rBV2	47683	189508	0.12%	0.043%
21	4.380	1007	1023	1052	rVB	184520	467353	0.31%	0.107%
22	4.511	1062	1064	1066	rBV	303	145	0.00%	0.000%
23	4.624	1096	1099	1104	rVB3	331	224	0.00%	0.000%
24	4.698	1108	1122	1140	rBV8	8194	20455	0.01%	0.005%
25	4.772	1141	1145	1146	rBV2	780	480	0.00%	0.000%
26	4.936	1186	1196	1198	rBV5	3083	4486	0.00%	0.001%
27	5.074	1221	1239	1267	rBV2	462338	1181833	0.77%	0.270%
28	5.354	1316	1326	1336	rVB6	10040	21259	0.01%	0.005%
29	5.434	1348	1351	1354	rVB2	431	241	0.00%	0.000%
30	5.511	1367	1375	1378	rBV4	2275	2774	0.00%	0.001%
31	5.553	1385	1388	1391	rBV2	339	244	0.00%	0.000%
32	5.643	1402	1416	1442	rBV	387209	758465	0.50%	0.173%
33	5.849	1477	1480	1483	rBV3	504	339	0.00%	0.000%
34	5.897	1493	1495	1498	rVB2	301	154	0.00%	0.000%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031720\
 Data File : VV014988.D
 Acq On : 17 Mar 2020 21:02
 Operator : SY/MD
 Sample : L1941-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DB6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
 Title : VOC Analysis

35	5.933	1498	1506	1513	rBV8	1070	1788	0.00%	0.000%
36	6.042	1537	1540	1542	rBV2	304	119	0.00%	0.000%
37	6.097	1542	1557	1568	rBV	256971	543737	0.36%	0.124%
38	6.286	1614	1616	1618	rVB2	425	182	0.00%	0.000%
39	6.389	1639	1648	1662	rVB2	11989	22416	0.01%	0.005%
40	6.457	1667	1669	1672	rBV	343	147	0.00%	0.000%
41	6.482	1674	1677	1686	rVB2	426	384	0.00%	0.000%
42	6.527	1686	1691	1693	rBV2	247	261	0.00%	0.000%
43	6.614	1714	1718	1719	rBV	229	174	0.00%	0.000%
44	6.662	1728	1733	1736	rBV2	296	225	0.00%	0.000%
45	6.704	1741	1746	1750	rBV3	323	341	0.00%	0.000%
46	6.794	1770	1774	1775	rBV	248	155	0.00%	0.000%
47	6.823	1775	1783	1786	rBV6	1032	1388	0.00%	0.000%
48	6.962	1823	1826	1830	rBV	132	129	0.00%	0.000%
49	7.010	1830	1841	1860	rBV2	134922	238379	0.16%	0.054%
50	7.161	1886	1888	1890	rBV2	447	239	0.00%	0.000%
51	7.206	1900	1902	1905	rBV	401	197	0.00%	0.000%
52	7.257	1914	1918	1920	rBV	252	198	0.00%	0.000%
53	7.280	1922	1925	1930	rVB2	435	379	0.00%	0.000%
54	7.338	1930	1943	1961	rBV	597560	1028505	0.67%	0.235%
55	7.643	2027	2038	2058	rBV	94695	165061	0.11%	0.038%
56	7.769	2073	2077	2081	rBV2	470	428	0.00%	0.000%
57	7.910	2114	2121	2125	rBV3	434	468	0.00%	0.000%
58	7.949	2131	2133	2134	rBV	589	233	0.00%	0.000%
59	7.997	2140	2148	2160	rVB4	6755	10687	0.01%	0.002%
60	8.119	2174	2186	2217	rBV2	281634	599334	0.39%	0.137%
61	8.524	2308	2312	2315	rBV	228	190	0.00%	0.000%
62	8.704	2365	2368	2373	rVB3	458	348	0.00%	0.000%
63	8.814	2399	2402	2404	rVB	315	168	0.00%	0.000%
64	8.907	2406	2431	2465	rBV	17947446	29922078	19.60%	6.829%
65	9.518	2619	2621	2622	rBV	379	126	0.00%	0.000%
66	9.563	2630	2635	2637	rBV2	1189	1146	0.00%	0.000%
67	9.698	2675	2677	2684	rVV2	464	354	0.00%	0.000%
68	9.736	2688	2689	2693	rVB2	255	170	0.00%	0.000%
69	9.752	2693	2694	2696	rBV2	400	150	0.00%	0.000%
70	9.987	2765	2767	2770	rBV	272	162	0.00%	0.000%
71	10.193	2828	2831	2832	rBV	308	170	0.00%	0.000%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031720\
 Data File : VV014988.D
 Acq On : 17 Mar 2020 21:02
 Operator : SY/MD
 Sample : L1941-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DB6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
 Title : VOC Analysis

72	10.238	2832	2845	2860	rVV	404020	632297	0.41%	0.144%
73	10.331	2873	2874	2878	rVB3	533	183	0.00%	0.000%
74	10.405	2891	2897	2900	rBV4	1249	1301	0.00%	0.000%
75	10.447	2902	2910	2925	rVB2	16500	27229	0.02%	0.006%
76	10.563	2938	2946	2960	rVB3	9354	14400	0.01%	0.003%
77	10.765	3001	3009	3012	rBV3	522	631	0.00%	0.000%
78	10.797	3016	3019	3024	rBV2	322	227	0.00%	0.000%
79	10.842	3024	3033	3040	rBV2	371	475	0.00%	0.000%
80	10.871	3040	3042	3044	rBV2	368	157	0.00%	0.000%
81	10.939	3054	3063	3069	rBV6	2469	3408	0.00%	0.001%
82	11.116	3117	3118	3122	rBV	493	292	0.00%	0.000%
83	11.151	3122	3129	3131	rBV2	769	899	0.00%	0.000%
84	11.206	3131	3146	3158	rBV	8470238	13272084	8.70%	3.029%
85	11.305	3159	3177	3200	rVB2	41968937	70813655	46.39%	16.161%
86	11.691	3273	3297	3312	rBV3	70609995	152634768	100.00%	34.834%
87	12.418	3513	3523	3535	rBV	109134	162532	0.11%	0.037%
88	12.601	3569	3580	3592	rBV4	28278	63858	0.04%	0.015%
89	12.669	3592	3601	3611	rVB	49540	73077	0.05%	0.017%
90	12.768	3622	3632	3649	rBV2	47576	74027	0.05%	0.017%
91	13.016	3703	3709	3718	rVB4	5583	8987	0.01%	0.002%
92	13.164	3751	3755	3756	rBV3	642	486	0.00%	0.000%
93	13.305	3778	3799	3823	rBV2	65190671	122374088	80.17%	27.928%
94	13.527	3860	3868	3882	rVB	48730	77551	0.05%	0.018%
95	13.768	3928	3943	3964	rBV	12084900	18308819	12.00%	4.178%
96	14.315	4099	4113	4129	rVB	104151	219543	0.14%	0.050%
97	14.643	4207	4215	4227	rVB8	8142	16847	0.01%	0.004%
98	14.839	4249	4276	4293	rBV	1541106	3886693	2.55%	0.887%
99	15.421	4443	4457	4481	rBV	12758425	19542119	12.80%	4.460%
100	16.659	4833	4842	4857	rVB	120410	190752	0.12%	0.044%


Sum of corrected areas: 438179733

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031720\
Data File : VV014988.D
Acq On : 17 Mar 2020 21:02
Operator : SY/MD
Sample : L1941-06
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DB6

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

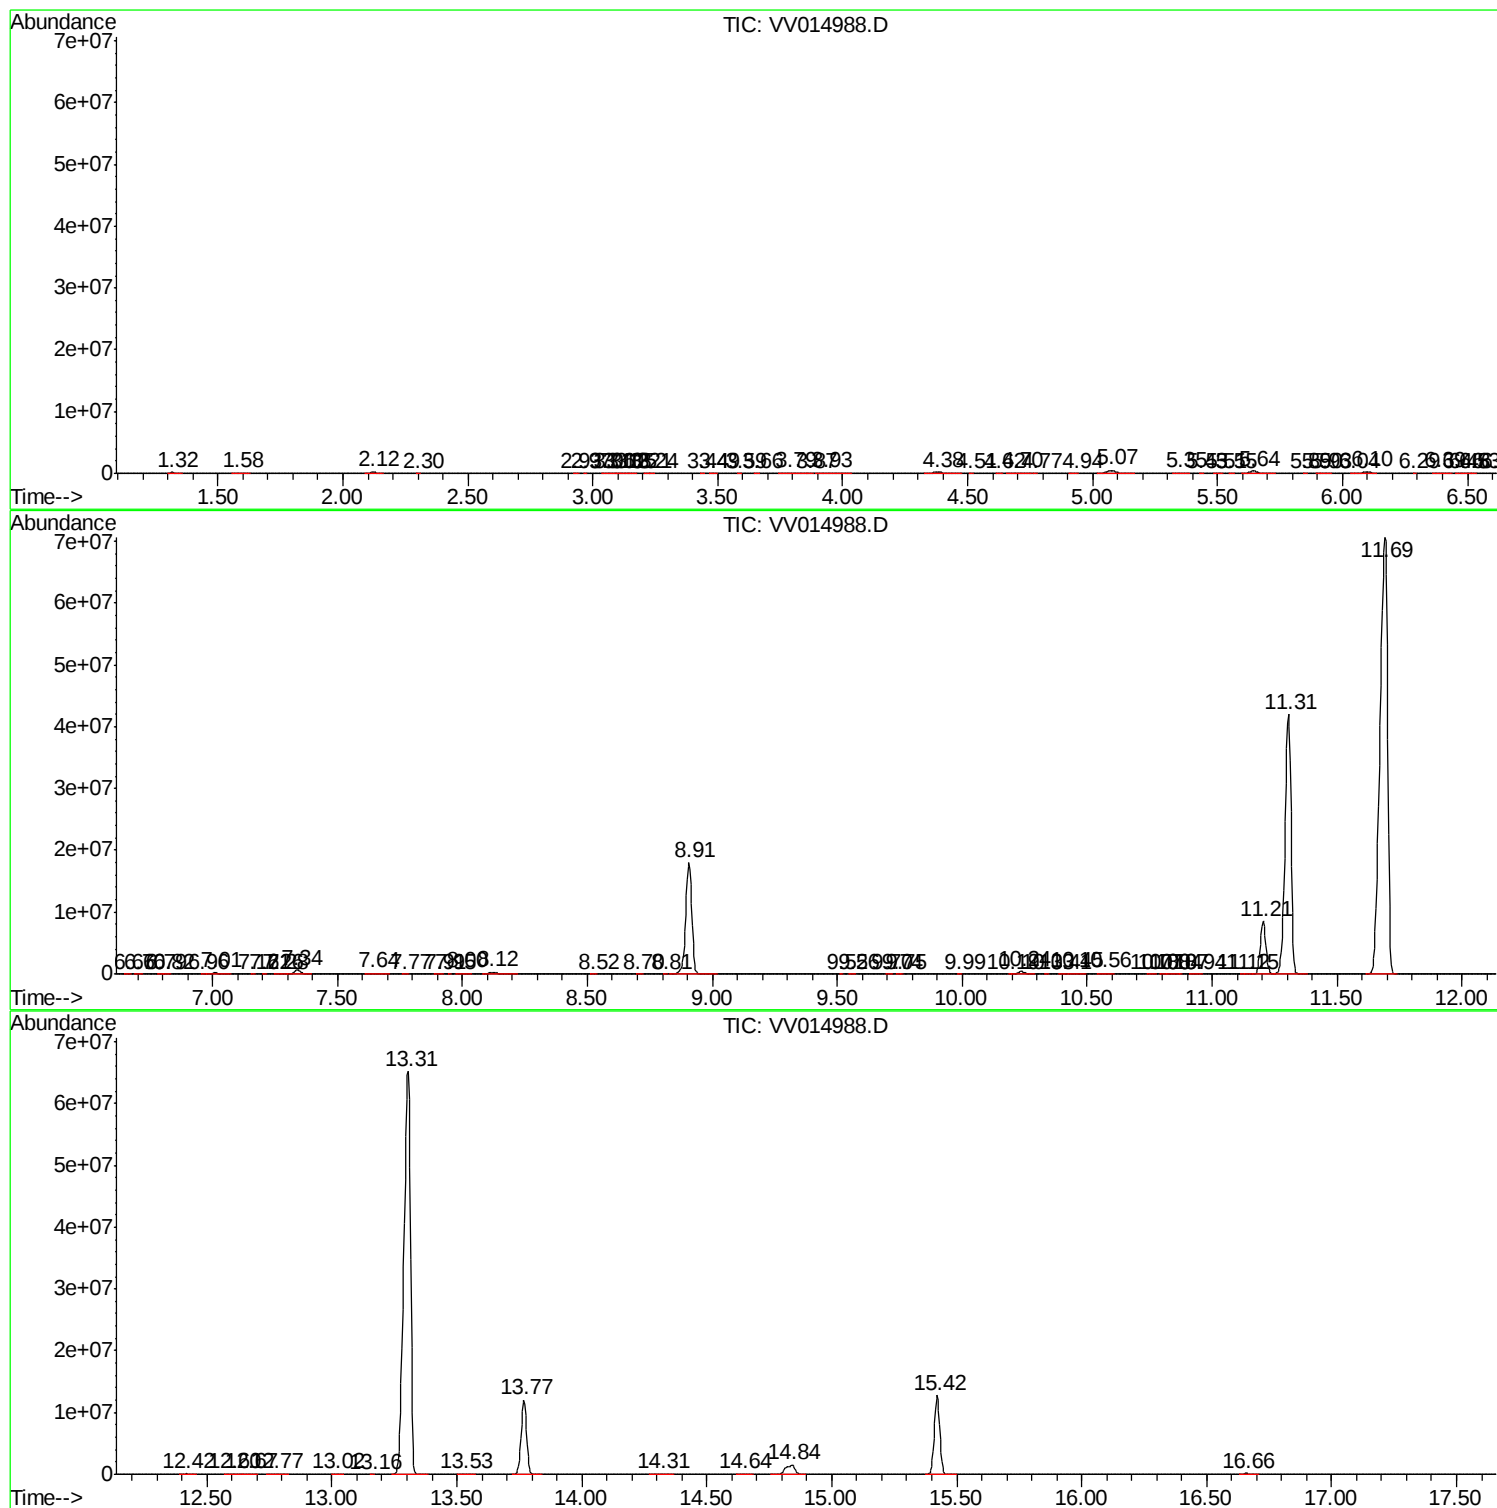

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV031720\
Data File : VV014988.D
Acq On : 17 Mar 2020 21:02
Operator : SY/MD
Sample : L1941-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DB6

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV031720\
Data File : VV014988.D
Acq On : 17 Mar 2020 21:02
Operator : SY/MD
Sample : L1941-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DB6

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc