

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031720\
 Data File : VV014993.D
 Acq On : 17 Mar 2020 23:34
 Operator : SY/MD
 Sample : L1940-16DL 10X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DB7DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	89	rVB	117512	127342	10.75%	1.192%
2	1.579	145	152	169	rVB	97078	116785	9.86%	1.094%
3	2.122	311	321	335	rBV	198127	282539	23.85%	2.646%
4	2.688	494	497	500	rVB2	698	480	0.04%	0.004%
5	2.849	543	547	550	rBV	354	304	0.03%	0.003%
6	2.926	565	571	576	rBV2	412	620	0.05%	0.006%
7	2.997	590	593	596	rBV2	399	208	0.02%	0.002%
8	3.032	601	604	608	rBV	235	239	0.02%	0.002%
9	3.087	615	621	625	rBV2	359	333	0.03%	0.003%
10	3.196	647	655	658	rBV2	514	636	0.05%	0.006%
11	3.408	718	721	728	rBV2	194	176	0.01%	0.002%
12	3.511	748	753	755	rBV	212	182	0.02%	0.002%
13	3.666	797	801	807	rBV2	201	242	0.02%	0.002%
14	3.743	820	825	828	rBV2	285	192	0.02%	0.002%
15	3.765	828	832	835	rBV2	255	228	0.02%	0.002%
16	3.875	863	866	872	rBV	208	187	0.02%	0.002%
17	3.936	872	885	921	rBV	45754	207702	17.53%	1.945%
18	4.380	1008	1023	1047	rVB	188959	456786	38.55%	4.277%
19	4.659	1106	1110	1113	rBV3	468	291	0.02%	0.003%
20	4.711	1123	1126	1135	rVB2	494	453	0.04%	0.004%
21	4.765	1141	1143	1148	rVB2	228	182	0.02%	0.002%
22	4.804	1153	1155	1160	rVB3	244	204	0.02%	0.002%
23	4.849	1163	1169	1173	rBV3	319	410	0.03%	0.004%
24	4.955	1199	1202	1208	rVB2	312	256	0.02%	0.002%
25	5.074	1221	1239	1271	rBV2	451897	1151458	97.18%	10.782%
26	5.306	1310	1311	1316	rBV3	262	221	0.02%	0.002%
27	5.331	1316	1319	1321	rBV2	353	249	0.02%	0.002%
28	5.386	1332	1336	1340	rBV2	171	194	0.02%	0.002%
29	5.441	1351	1353	1356	rVB2	425	175	0.01%	0.002%
30	5.460	1356	1359	1361	rBV2	258	163	0.01%	0.002%
31	5.643	1398	1416	1436	rBV	364038	719712	60.74%	6.739%
32	5.900	1494	1496	1499	rBV2	340	211	0.02%	0.002%
33	5.968	1513	1517	1522	rVB3	480	284	0.02%	0.003%
34	6.000	1525	1527	1531	rVB2	336	191	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031720\
 Data File : VV014993.D
 Acq On : 17 Mar 2020 23:34
 Operator : SY/MD
 Sample : L1940-16DL 10X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DB7DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
 Title : VOC Analysis

35	6.035	1535	1538	1541	rBV	355	204	0.02%	0.002%
36	6.096	1541	1557	1580	rBV	246174	508517	42.92%	4.762%
37	6.293	1615	1618	1620	rVB2	335	188	0.02%	0.002%
38	6.315	1620	1625	1629	rBV3	330	278	0.02%	0.003%
39	6.363	1637	1640	1646	rBV2	260	180	0.02%	0.002%
40	6.402	1651	1652	1658	rBV2	377	250	0.02%	0.002%
41	6.550	1690	1698	1701	rBV2	240	246	0.02%	0.002%
42	6.592	1704	1711	1715	rBV2	187	237	0.02%	0.002%
43	6.646	1723	1728	1731	rBV3	241	219	0.02%	0.002%
44	6.672	1731	1736	1738	rBV2	382	287	0.02%	0.003%
45	6.823	1777	1783	1784	rBV2	287	196	0.02%	0.002%
46	6.859	1791	1794	1796	rBV2	228	173	0.01%	0.002%
47	7.010	1829	1841	1859	rBV	136610	249777	21.08%	2.339%
48	7.174	1889	1892	1897	rVB2	696	436	0.04%	0.004%
49	7.212	1902	1904	1907	rBV	325	185	0.02%	0.002%
50	7.257	1915	1918	1921	rBV3	535	412	0.03%	0.004%
51	7.286	1925	1927	1930	rBV3	512	387	0.03%	0.004%
52	7.341	1931	1944	1963	rBV	566865	977976	82.54%	9.157%
53	7.569	2012	2015	2019	rVB2	501	344	0.03%	0.003%
54	7.643	2027	2038	2059	rBV	97223	167965	14.18%	1.573%
55	8.122	2175	2187	2216	rBV3	263369	604800	51.04%	5.663%
56	8.543	2313	2318	2319	rBV	253	160	0.01%	0.001%
57	8.608	2332	2338	2341	rBV3	343	476	0.04%	0.004%
58	8.669	2356	2357	2362	rVB	369	238	0.02%	0.002%
59	8.823	2402	2405	2408	rBV2	377	287	0.02%	0.003%
60	8.874	2408	2421	2426	rBV	559227	944868	79.74%	8.847%
61	9.129	2497	2500	2503	rBV2	291	204	0.02%	0.002%
62	9.161	2506	2510	2512	rBV2	431	268	0.02%	0.003%
63	9.209	2522	2525	2528	rBV3	296	186	0.02%	0.002%
64	9.289	2545	2550	2555	rBV2	273	245	0.02%	0.002%
65	9.315	2555	2558	2561	rVB	274	164	0.01%	0.002%
66	9.492	2611	2613	2619	rVB2	366	292	0.02%	0.003%
67	9.669	2667	2668	2674	rVB2	372	175	0.01%	0.002%
68	9.858	2722	2727	2731	rBV2	243	246	0.02%	0.002%
69	9.923	2743	2747	2749	rBV	457	258	0.02%	0.002%
70	9.945	2751	2754	2756	rBV	318	163	0.01%	0.002%
71	9.958	2756	2758	2762	rBV2	263	174	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031720\
 Data File : VV014993.D
 Acq On : 17 Mar 2020 23:34
 Operator : SY/MD
 Sample : L1940-16DL 10X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DB7DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
 Title : VOC Analysis

72	10.083	2795	2797	2803	rBV2	324	225	0.02%	0.002%
73	10.238	2833	2845	2861	rBV	387579	613739	51.80%	5.747%
74	10.447	2905	2910	2918	rVB4	2740	3537	0.30%	0.033%
75	10.543	2937	2940	2942	rVV2	286	161	0.01%	0.002%
76	10.563	2942	2946	2951	rVB2	688	684	0.06%	0.006%
77	10.646	2969	2972	2975	rBV	272	164	0.01%	0.002%
78	10.665	2976	2978	2984	rVB	361	258	0.02%	0.002%
79	10.794	3015	3018	3024	rBV	331	290	0.02%	0.003%
80	11.202	3133	3145	3156	rBV	315061	483209	40.78%	4.525%
81	11.270	3156	3166	3171	rBV	629304	1060318	89.49%	9.928%
82	11.505	3237	3239	3244	rBV2	369	268	0.02%	0.003%
83	11.588	3262	3265	3268	rVB2	454	243	0.02%	0.002%
84	11.646	3268	3283	3309	rBV2	651487	1184897	100.00%	11.095%
85	11.939	3371	3374	3378	rBV2	243	178	0.02%	0.002%
86	12.421	3518	3524	3532	rVB3	2394	3177	0.27%	0.030%
87	12.543	3558	3562	3566	rBV2	415	446	0.04%	0.004%
88	12.604	3572	3581	3592	rVB6	3675	8386	0.71%	0.079%
89	12.665	3593	3600	3611	rVB4	8708	12155	1.03%	0.114%
90	12.765	3626	3631	3634	rBV2	574	620	0.05%	0.006%
91	12.820	3646	3648	3652	rVV2	434	286	0.02%	0.003%
92	12.839	3652	3654	3660	rVB2	565	458	0.04%	0.004%
93	12.871	3661	3664	3666	rVB2	455	241	0.02%	0.002%
94	12.923	3677	3680	3686	rBV2	453	416	0.04%	0.004%
95	12.948	3686	3688	3693	rBV2	381	337	0.03%	0.003%
96	13.019	3708	3710	3714	rVB3	523	342	0.03%	0.003%
97	13.103	3732	3736	3742	rBV3	546	637	0.05%	0.006%
98	13.283	3777	3792	3809	rBV	474374	724821	61.17%	6.787%
99	13.765	3932	3942	3957	rVB2	30414	47475	4.01%	0.445%
100	13.890	3979	3981	3982	rBV	664	196	0.02%	0.002%


Sum of corrected areas: 10679660

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV031720\
Data File : VV014993.D
Acq On : 17 Mar 2020 23:34
Operator : SY/MD
Sample : L1940-16DL 10X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DB7DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

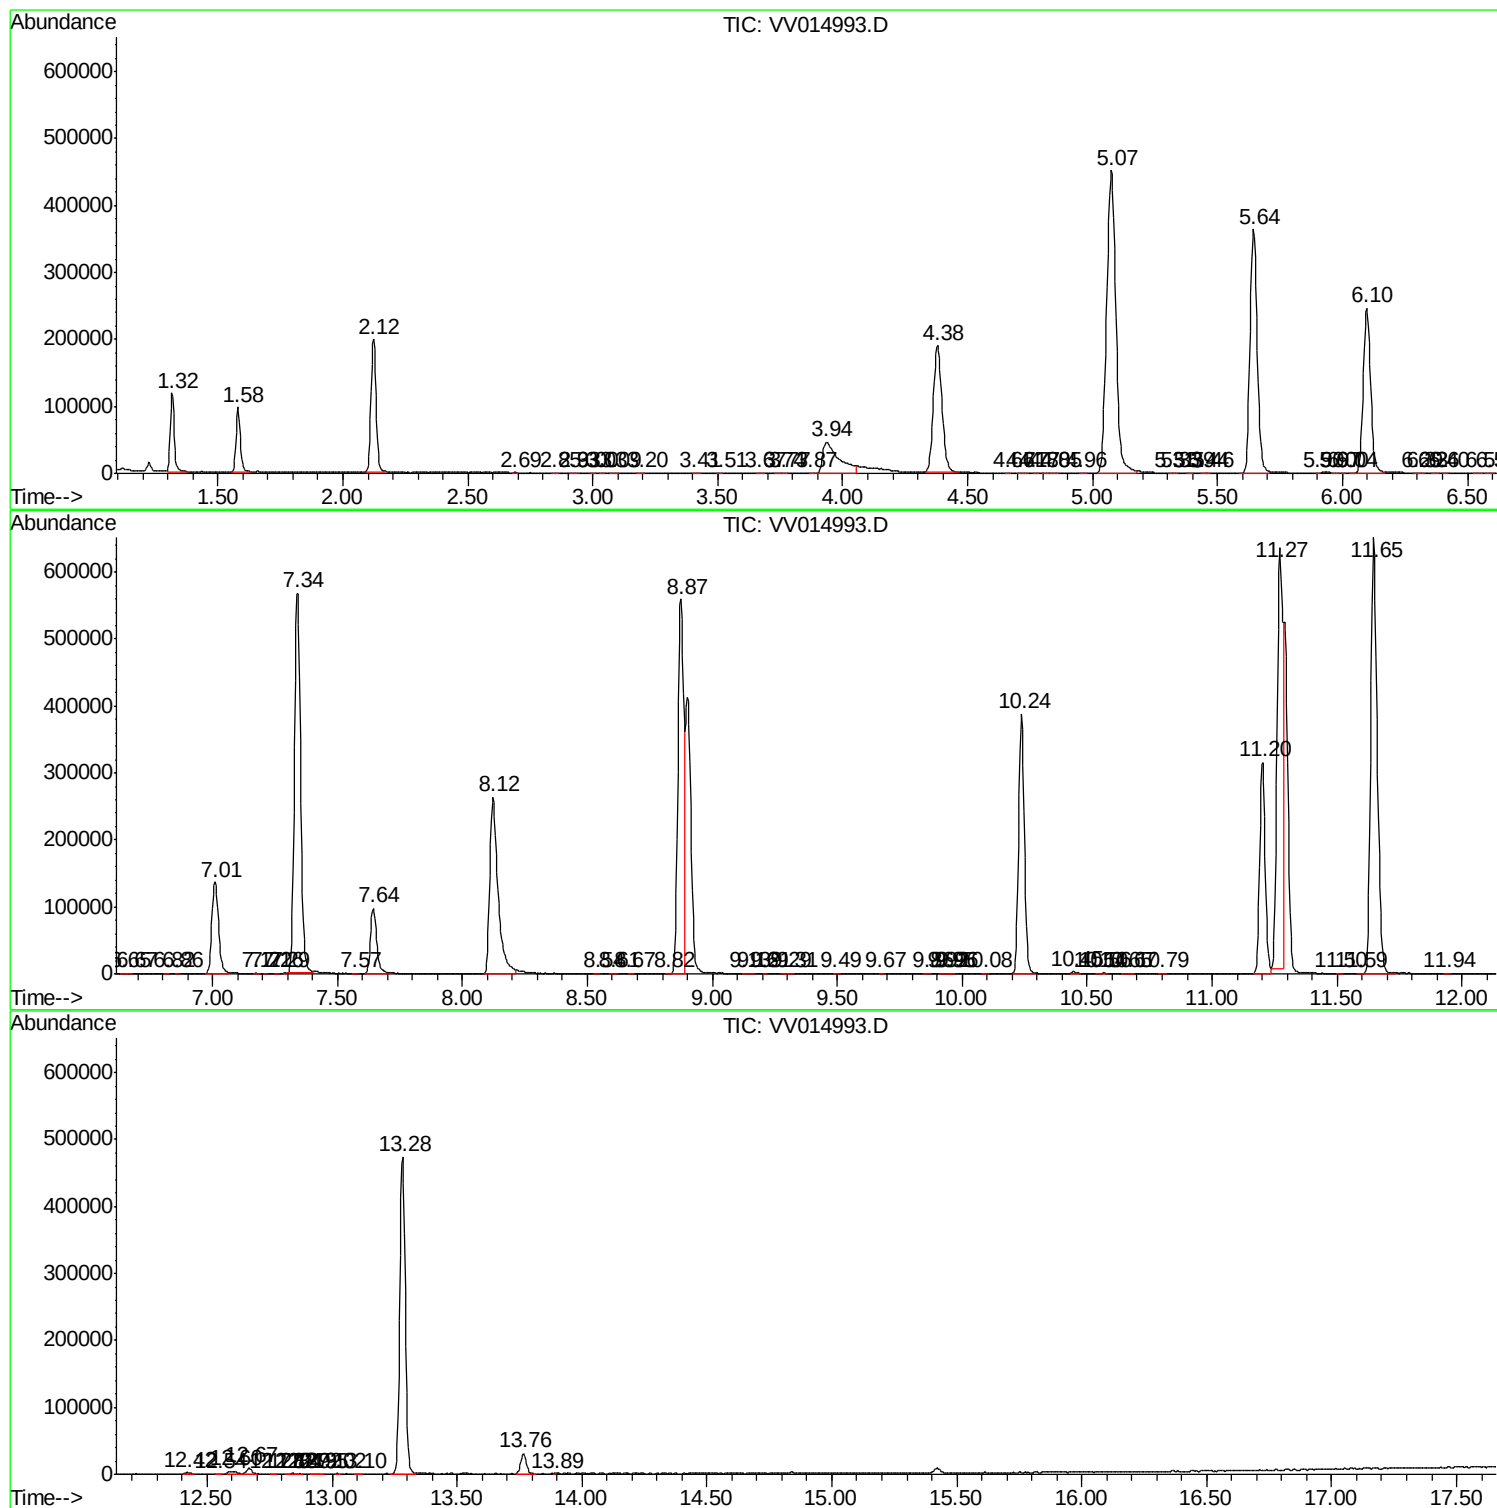

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV031720\
Data File : VV014993.D
Acq On : 17 Mar 2020 23:34
Operator : SY/MD
Sample : L1940-16DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DB7DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV031720\
Data File : VV014993.D
Acq On : 17 Mar 2020 23:34
Operator : SY/MD
Sample : L1940-16DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DB7DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc