

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031720\
 Data File : VV014996.D
 Acq On : 18 Mar 2020 00:46
 Operator : SY/MD
 Sample : L1940-11
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DA0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.222	37	41	56	rVB2	15287	17835	1.59%	0.206%
2	1.315	64	70	84	rVB	113610	123036	10.98%	1.418%
3	1.579	145	152	165	rBV	87722	107207	9.57%	1.236%
4	2.123	310	321	340	rBV	190767	275554	24.60%	3.176%
5	3.238	665	668	669	rBV3	378	208	0.02%	0.002%
6	3.274	677	679	681	rBV	348	138	0.01%	0.002%
7	3.306	681	689	693	rBV3	359	499	0.04%	0.006%
8	3.370	707	709	713	rBV2	169	133	0.01%	0.002%
9	3.415	721	723	726	rBV	266	159	0.01%	0.002%
10	3.447	732	733	736	rVB2	135	35	0.00%	0.000%
11	3.463	736	738	740	rBV2	128	61	0.01%	0.001%
12	3.483	741	744	747	rVV2	238	126	0.01%	0.001%
13	3.495	747	748	749	rVV2	111	22	0.00%	0.000%
14	3.566	767	770	774	rBV2	226	183	0.02%	0.002%
15	3.643	789	794	795	rBV2	374	277	0.02%	0.003%
16	3.679	803	805	807	rBV	322	119	0.01%	0.001%
17	3.807	843	845	846	rBV	255	113	0.01%	0.001%
18	3.939	874	886	910	rBV	41928	161235	14.39%	1.859%
19	4.380	1008	1023	1051	rVB2	183794	451317	40.29%	5.202%
20	4.624	1095	1099	1103	rBV3	384	420	0.04%	0.005%
21	4.643	1103	1105	1107	rBV	253	130	0.01%	0.001%
22	4.675	1113	1115	1118	rBV2	202	100	0.01%	0.001%
23	4.746	1136	1137	1140	rBV2	238	120	0.01%	0.001%
24	4.817	1156	1159	1161	rBV2	228	140	0.01%	0.002%
25	4.830	1161	1163	1166	rVV	350	177	0.02%	0.002%
26	4.859	1169	1172	1179	rVB3	403	471	0.04%	0.005%
27	4.888	1179	1181	1183	rBV	449	273	0.02%	0.003%
28	5.074	1222	1239	1265	rBV2	446663	1120097	100.00%	12.911%
29	5.412	1341	1344	1347	rBV3	448	201	0.02%	0.002%
30	5.499	1369	1371	1375	rVB2	261	159	0.01%	0.002%
31	5.528	1379	1380	1382	rVV2	340	133	0.01%	0.002%
32	5.547	1383	1386	1390	rVB3	392	257	0.02%	0.003%
33	5.592	1398	1400	1402	rBV	269	158	0.01%	0.002%
34	5.643	1403	1416	1440	rVV	350134	698635	62.37%	8.053%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031720\
 Data File : VV014996.D
 Acq On : 18 Mar 2020 00:46
 Operator : SY/MD
 Sample : L1940-11
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DA0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
 Title : VOC Analysis

35	5.926	1499	1504	1507	rBV4	1138	1353	0.12%	0.016%
36	6.097	1542	1557	1577	rBV	242303	493995	44.10%	5.694%
37	6.270	1608	1611	1616	rBV3	432	333	0.03%	0.004%
38	6.354	1635	1637	1640	rVB2	336	163	0.01%	0.002%
39	6.473	1672	1674	1679	rVB2	242	121	0.01%	0.001%
40	6.492	1679	1680	1683	rVB2	226	72	0.01%	0.001%
41	6.511	1683	1686	1690	rBV2	348	256	0.02%	0.003%
42	6.589	1709	1710	1712	rBV	153	58	0.01%	0.001%
43	6.653	1726	1730	1732	rBV2	453	302	0.03%	0.003%
44	6.820	1780	1782	1783	rBV	163	48	0.00%	0.001%
45	6.894	1803	1805	1808	rBV	292	223	0.02%	0.003%
46	6.926	1812	1815	1817	rBV	342	204	0.02%	0.002%
47	6.949	1821	1822	1825	rVB	287	106	0.01%	0.001%
48	7.010	1829	1841	1856	rBV2	137382	243923	21.78%	2.812%
49	7.158	1884	1887	1888	rBV	312	166	0.01%	0.002%
50	7.167	1888	1890	1892	rVV2	754	378	0.03%	0.004%
51	7.338	1931	1943	1969	rBV	550727	951732	84.97%	10.970%
52	7.482	1985	1988	1994	rVB3	688	609	0.05%	0.007%
53	7.524	1998	2001	2009	rVB4	457	529	0.05%	0.006%
54	7.556	2009	2011	2015	rBV2	494	346	0.03%	0.004%
55	7.643	2027	2038	2061	rBV	96963	168487	15.04%	1.942%
56	7.746	2068	2070	2074	rBV2	406	250	0.02%	0.003%
57	7.804	2086	2088	2091	rVB2	320	184	0.02%	0.002%
58	7.843	2098	2100	2105	rVB	476	327	0.03%	0.004%
59	7.955	2128	2135	2137	rBV2	1474	1280	0.11%	0.015%
60	8.122	2175	2187	2222	rBV2	249043	576677	51.48%	6.647%
61	8.453	2289	2290	2296	rBV	470	392	0.03%	0.005%
62	8.521	2309	2311	2312	rBV	182	78	0.01%	0.001%
63	8.601	2334	2336	2338	rBV	290	151	0.01%	0.002%
64	8.662	2351	2355	2356	rBV2	370	168	0.01%	0.002%
65	8.752	2381	2383	2385	rBV	170	50	0.00%	0.001%
66	8.875	2409	2421	2450	rBV	533978	868888	77.57%	10.015%
67	9.106	2491	2493	2496	rBV	318	166	0.01%	0.002%
68	9.261	2539	2541	2544	rBV	189	72	0.01%	0.001%
69	9.360	2570	2572	2578	rVB	557	261	0.02%	0.003%
70	9.399	2582	2584	2586	rBV2	317	161	0.01%	0.002%
71	9.457	2599	2602	2604	rBV	199	134	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031720\
 Data File : VV014996.D
 Acq On : 18 Mar 2020 00:46
 Operator : SY/MD
 Sample : L1940-11
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DA0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
 Title : VOC Analysis

72	9.527	2622	2624	2626	rBV2	357	125	0.01%	0.001%
73	9.547	2628	2630	2632	rBV2	271	130	0.01%	0.001%
74	9.592	2642	2644	2647	rBV	220	140	0.01%	0.002%
75	9.650	2659	2662	2665	rBV3	268	151	0.01%	0.002%
76	9.691	2673	2675	2679	rVB2	320	187	0.02%	0.002%
77	9.765	2693	2698	2704	rBV2	398	418	0.04%	0.005%
78	9.958	2756	2758	2761	rVB	444	152	0.01%	0.002%
79	9.978	2761	2764	2769	rVB2	326	202	0.02%	0.002%
80	10.100	2799	2802	2805	rBV	296	214	0.02%	0.002%
81	10.238	2833	2845	2862	rBV	377348	596718	53.27%	6.878%
82	10.367	2884	2885	2887	rBV	144	57	0.01%	0.001%
83	10.405	2889	2897	2906	rVB6	2082	3487	0.31%	0.040%
84	10.563	2944	2946	2950	rVB	488	244	0.02%	0.003%
85	10.820	3023	3026	3027	rBV	187	86	0.01%	0.001%
86	10.862	3037	3039	3040	rBV	279	97	0.01%	0.001%
87	10.875	3040	3043	3046	rBV2	716	390	0.03%	0.004%
88	11.042	3093	3095	3102	rBV2	249	221	0.02%	0.003%
89	11.270	3154	3166	3186	rBV	546418	854649	76.30%	9.851%
90	11.556	3253	3255	3262	rBV3	411	353	0.03%	0.004%
91	11.646	3271	3283	3298	rBV	583078	924860	82.57%	10.661%
92	12.543	3560	3562	3565	rBV2	275	200	0.02%	0.002%
93	13.177	3756	3759	3761	rBV2	492	308	0.03%	0.004%
94	13.283	3783	3792	3810	rBV4	11093	17778	1.59%	0.205%
95	13.772	3937	3944	3948	rBV3	1119	1432	0.13%	0.017%
96	14.267	4095	4098	4101	rBV2	740	536	0.05%	0.006%


Sum of corrected areas: 8675506

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV031720\
Data File : VV014996.D
Acq On : 18 Mar 2020 00:46
Operator : SY/MD
Sample : L1940-11
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DA0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

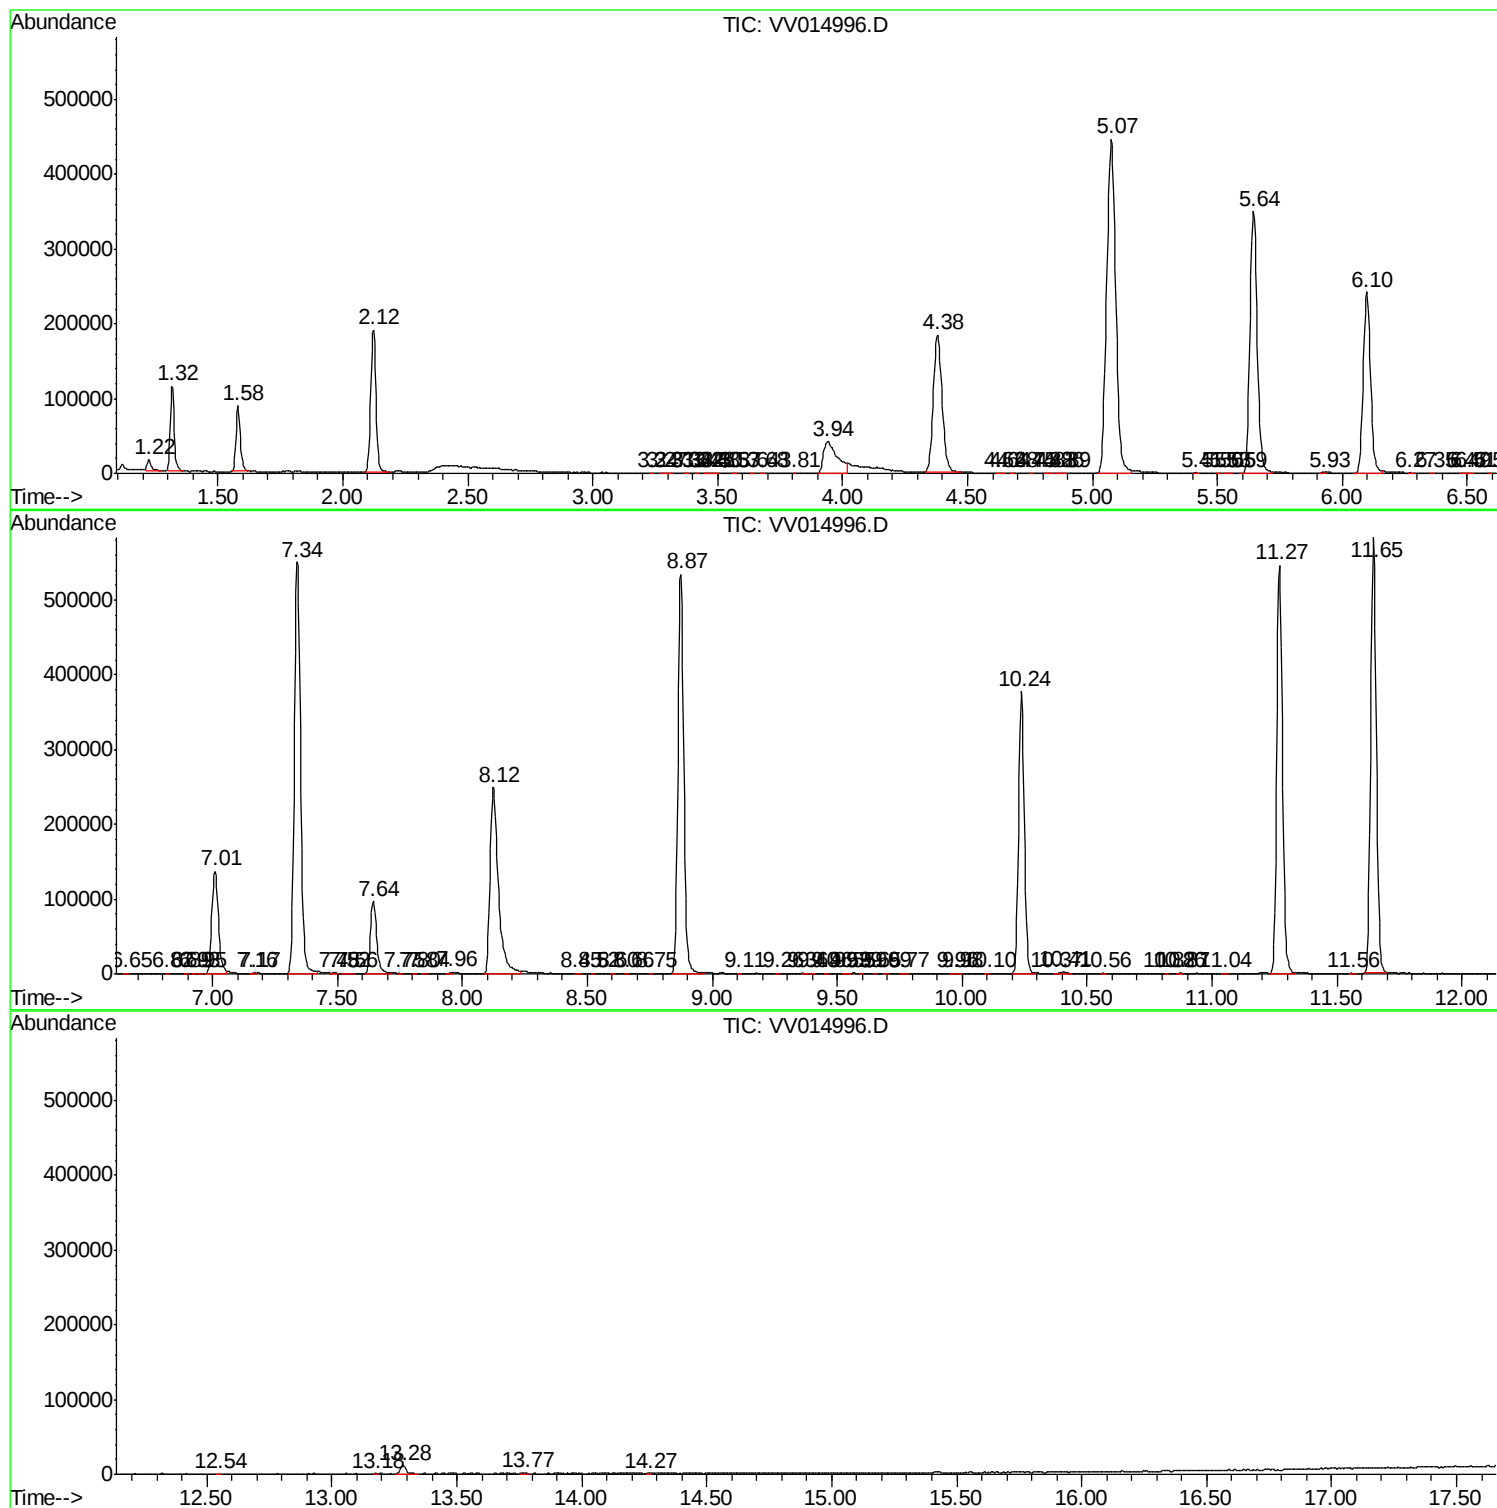

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV031720\
Data File : VV014996.D
Acq On : 18 Mar 2020 00:46
Operator : SY/MD
Sample : L1940-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DA0

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV031720\
Data File : VV014996.D
Acq On : 18 Mar 2020 00:46
Operator : SY/MD
Sample : L1940-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DA0

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc