

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031720\
 Data File : VV014998.D
 Acq On : 18 Mar 2020 01:34
 Operator : SY/MD
 Sample : L1940-13
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DA7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	87	rVB	115610	117722	10.65%	1.369%
2	1.579	144	152	166	rVB	91791	112255	10.16%	1.305%
3	2.122	310	321	336	rBV	190764	274962	24.89%	3.197%
4	3.026	599	602	608	rBV2	540	518	0.05%	0.006%
5	3.187	647	652	657	rBV2	294	380	0.03%	0.004%
6	3.357	703	705	708	rBV	264	125	0.01%	0.001%
7	3.531	756	759	761	rBV	234	122	0.01%	0.001%
8	3.592	776	778	781	rBV	246	165	0.01%	0.002%
9	3.679	802	805	807	rBV2	198	157	0.01%	0.002%
10	3.859	856	861	862	rBV2	195	164	0.01%	0.002%
11	3.936	873	885	916	rBV	44084	173934	15.74%	2.022%
12	4.380	1006	1023	1055	rVB	180634	446904	40.45%	5.197%
13	4.611	1090	1095	1098	rBV2	471	413	0.04%	0.005%
14	4.769	1141	1144	1147	rVB2	465	270	0.02%	0.003%
15	4.785	1147	1149	1152	rVB2	181	58	0.01%	0.001%
16	4.801	1152	1154	1155	rBV	320	64	0.01%	0.001%
17	4.862	1169	1173	1177	rBV2	391	301	0.03%	0.004%
18	4.929	1191	1194	1199	rVB2	277	209	0.02%	0.002%
19	4.952	1199	1201	1206	rVB	264	154	0.01%	0.002%
20	4.978	1206	1209	1211	rBV	281	197	0.02%	0.002%
21	5.074	1221	1239	1275	rBV2	439432	1104874	100.00%	12.847%
22	5.360	1324	1328	1331	rBV	186	156	0.01%	0.002%
23	5.376	1331	1333	1335	rBV	240	125	0.01%	0.001%
24	5.389	1335	1337	1339	rVB	251	87	0.01%	0.001%
25	5.473	1360	1363	1367	rBV	273	186	0.02%	0.002%
26	5.518	1375	1377	1383	rVB2	237	201	0.02%	0.002%
27	5.556	1387	1389	1392	rVB2	235	83	0.01%	0.001%
28	5.579	1392	1396	1397	rBV2	255	191	0.02%	0.002%
29	5.643	1403	1416	1441	rBV	349247	694949	62.90%	8.081%
30	5.823	1470	1472	1479	rBV4	399	501	0.05%	0.006%
31	5.855	1480	1482	1487	rVB2	528	288	0.03%	0.003%
32	5.936	1498	1507	1510	rBV5	1467	1977	0.18%	0.023%
33	6.097	1542	1557	1582	rBV2	240692	492295	44.56%	5.724%
34	6.286	1614	1616	1620	rVB2	419	256	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031720\
 Data File : VV014998.D
 Acq On : 18 Mar 2020 01:34
 Operator : SY/MD
 Sample : L1940-13
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DA7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
 Title : VOC Analysis

35	6.318	1621	1626	1630	rVV	342	281	0.03%	0.003%
36	6.334	1630	1631	1634	rVV2	170	88	0.01%	0.001%
37	6.351	1634	1636	1641	rVB	383	275	0.02%	0.003%
38	6.437	1660	1663	1664	rBV	224	105	0.01%	0.001%
39	6.460	1668	1670	1672	rVV	391	170	0.02%	0.002%
40	6.486	1676	1678	1684	rVB	318	216	0.02%	0.003%
41	6.614	1716	1718	1721	rBV2	285	138	0.01%	0.002%
42	6.849	1789	1791	1794	rBV	228	108	0.01%	0.001%
43	7.010	1829	1841	1869	rBV	131791	237141	21.46%	2.757%
44	7.190	1894	1897	1898	rBV	491	255	0.02%	0.003%
45	7.338	1929	1943	1965	rBV	537859	934631	84.59%	10.868%
46	7.598	2022	2024	2025	rBV	187	62	0.01%	0.001%
47	7.643	2027	2038	2063	rVV	93161	162694	14.73%	1.892%
48	8.122	2175	2187	2226	rBV3	241499	581040	52.59%	6.756%
49	8.424	2277	2281	2282	rBV3	551	321	0.03%	0.004%
50	8.624	2340	2343	2345	rBV	308	196	0.02%	0.002%
51	8.662	2354	2355	2358	rBV	383	198	0.02%	0.002%
52	8.875	2408	2421	2441	rBV	528615	869327	78.68%	10.108%
53	9.350	2565	2569	2570	rBV	216	159	0.01%	0.002%
54	9.569	2631	2637	2642	rVB4	455	568	0.05%	0.007%
55	9.592	2642	2644	2645	rBV	216	56	0.01%	0.001%
56	9.723	2683	2685	2689	rBV3	308	162	0.01%	0.002%
57	10.038	2780	2783	2786	rBV	252	234	0.02%	0.003%
58	10.141	2814	2815	2823	rVB2	402	345	0.03%	0.004%
59	10.183	2823	2828	2829	rBV	362	263	0.02%	0.003%
60	10.238	2833	2845	2863	rVV	375575	593528	53.72%	6.902%
61	10.373	2883	2887	2889	rBV	476	452	0.04%	0.005%
62	10.572	2946	2949	2953	rBV2	321	242	0.02%	0.003%
63	10.595	2953	2956	2960	rBV2	410	334	0.03%	0.004%
64	10.846	3031	3034	3037	rBV2	380	232	0.02%	0.003%
65	11.016	3084	3087	3089	rBV	389	193	0.02%	0.002%
66	11.083	3103	3108	3110	rBV3	485	477	0.04%	0.006%
67	11.206	3142	3146	3154	rVB4	1562	1584	0.14%	0.018%
68	11.270	3154	3166	3189	rBV	547287	846196	76.59%	9.840%
69	11.646	3271	3283	3302	rBV	577848	919694	83.24%	10.694%
70	11.997	3389	3392	3394	rBV3	398	234	0.02%	0.003%
71	12.360	3503	3505	3507	rBV	397	223	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031720\
Data File : VV014998.D
Acq On : 18 Mar 2020 01:34
Operator : SY/MD
Sample : L1940-13
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DA7

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Title : VOC Analysis

72	13.283	3784	3792	3803	rBV3	13828	21795	1.97%	0.253%
73	13.427	3831	3837	3838	rBV3	456	502	0.05%	0.006%


Sum of corrected areas: 8599962

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV031720\
Data File : VV014998.D
Acq On : 18 Mar 2020 01:34
Operator : SY/MD
Sample : L1940-13
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DA7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

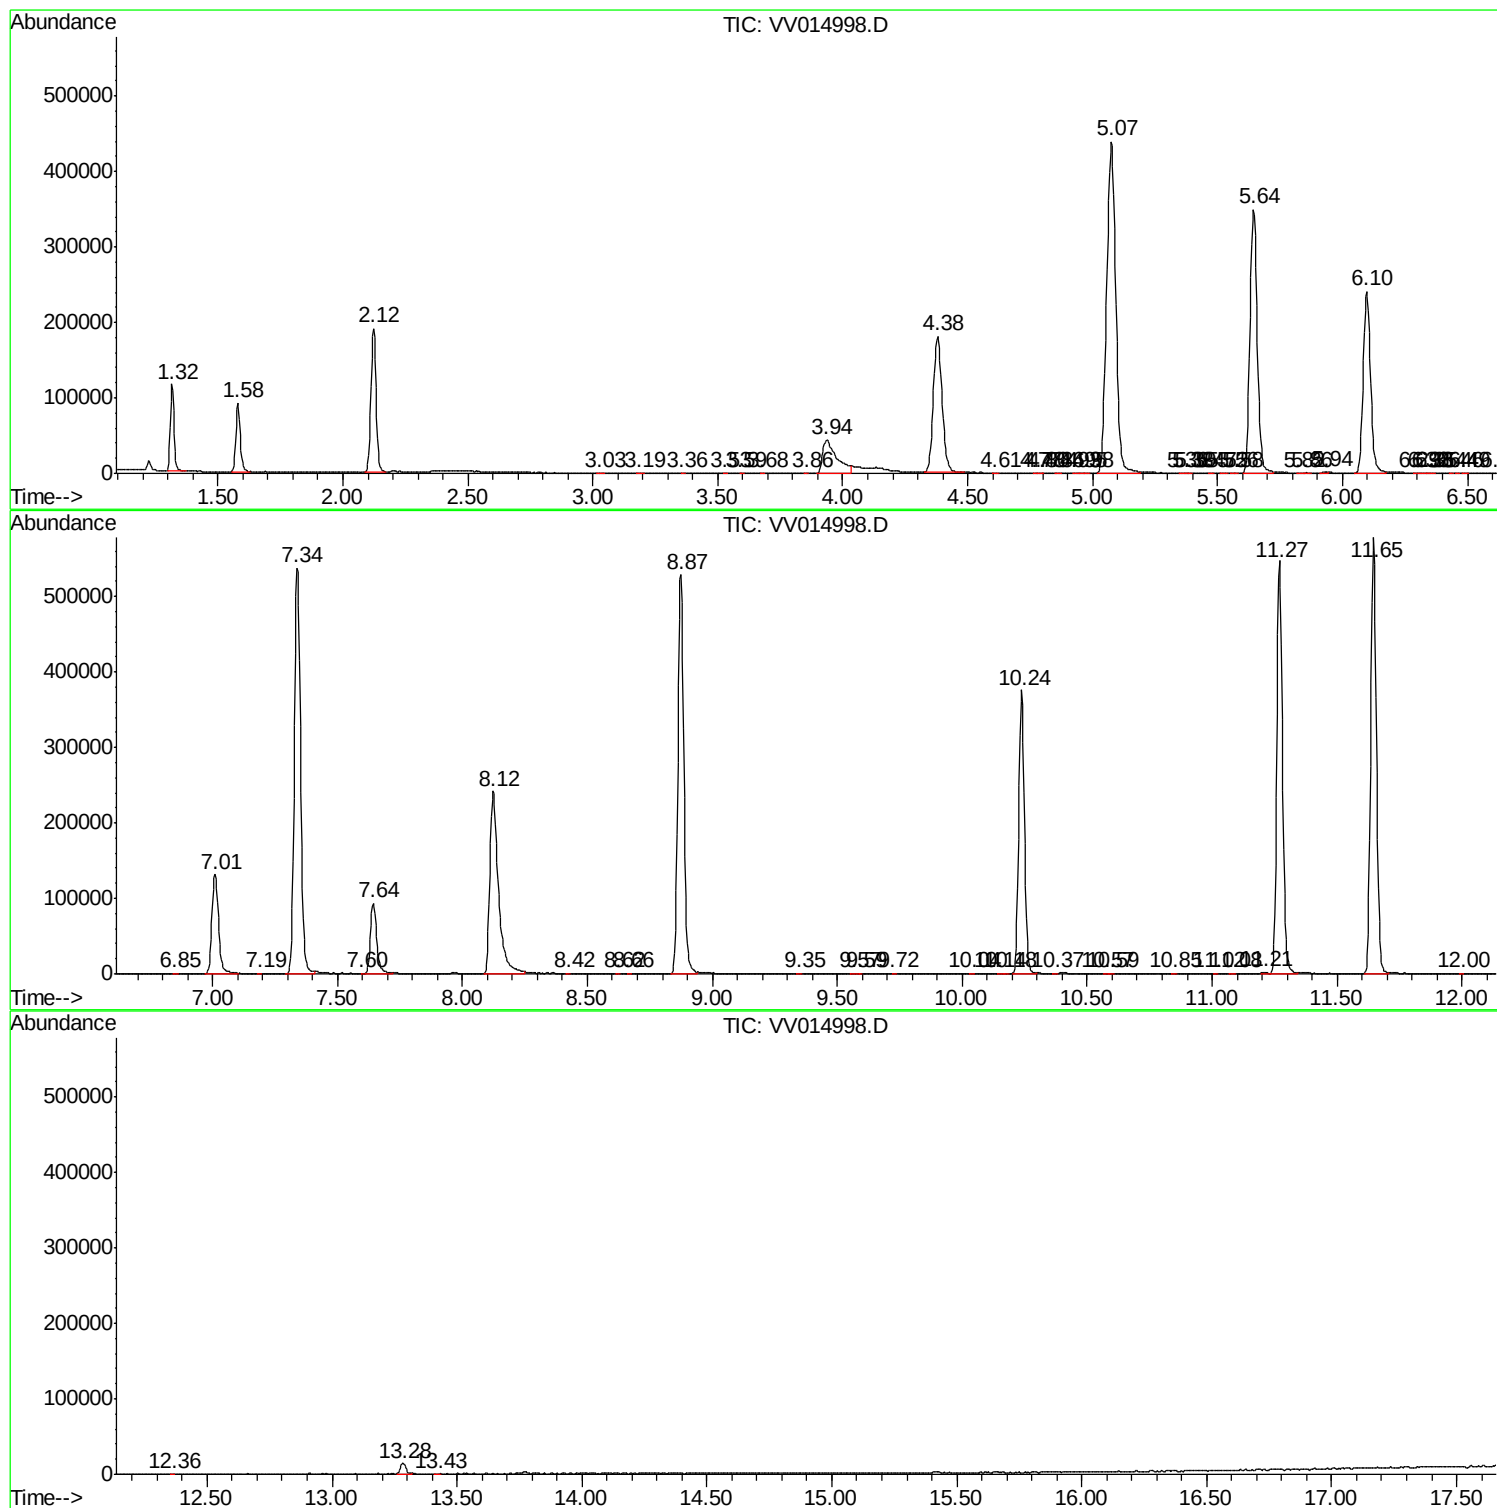

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV031720\
Data File : VV014998.D
Acq On : 18 Mar 2020 01:34
Operator : SY/MD
Sample : L1940-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DA7

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV031720\
Data File : VV014998.D
Acq On : 18 Mar 2020 01:34
Operator : SY/MD
Sample : L1940-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DA7

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc