

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031720\
 Data File : VV014999.D
 Acq On : 18 Mar 2020 01:58
 Operator : SY/MD
 Sample : L1940-15
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DB0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.222	37	41	48	rVB2	16409	15814	1.43%	0.183%
2	1.315	64	70	84	rVB	112650	117874	10.69%	1.361%
3	1.579	145	152	168	rVB	88621	109040	9.89%	1.259%
4	2.123	312	321	340	rVB	187198	272354	24.70%	3.145%
5	2.962	579	582	583	rBV	456	259	0.02%	0.003%
6	3.029	600	603	607	rVB	423	196	0.02%	0.002%
7	3.084	616	620	622	rBV	167	118	0.01%	0.001%
8	3.126	629	633	636	rBV3	411	300	0.03%	0.003%
9	3.142	636	638	641	rBV2	126	66	0.01%	0.001%
10	3.206	654	658	660	rBV	602	440	0.04%	0.005%
11	3.293	683	685	689	rBV2	130	112	0.01%	0.001%
12	3.399	715	718	721	rVB2	348	192	0.02%	0.002%
13	3.434	727	729	734	rVB	394	182	0.02%	0.002%
14	3.460	735	737	739	rBV	153	55	0.00%	0.001%
15	3.569	769	771	772	rBV	104	48	0.00%	0.001%
16	3.717	814	817	819	rBV	170	147	0.01%	0.002%
17	3.769	831	833	835	rVB	191	55	0.00%	0.001%
18	3.843	854	856	861	rVB2	224	100	0.01%	0.001%
19	3.891	870	871	873	rVB	147	33	0.00%	0.000%
20	3.933	873	884	917	rBV2	44981	184417	16.73%	2.129%
21	4.380	1006	1023	1049	rBV	184958	456437	41.40%	5.270%
22	4.585	1084	1087	1092	rBV2	337	242	0.02%	0.003%
23	4.708	1120	1125	1128	rBV2	376	358	0.03%	0.004%
24	4.737	1132	1134	1136	rVB2	173	54	0.00%	0.001%
25	4.807	1154	1156	1158	rBV	183	85	0.01%	0.001%
26	4.817	1158	1159	1163	rVB2	208	123	0.01%	0.001%
27	4.920	1188	1191	1193	rBV3	199	135	0.01%	0.002%
28	4.933	1193	1195	1196	rVV3	227	97	0.01%	0.001%
29	4.942	1196	1198	1203	rVB	462	273	0.02%	0.003%
30	4.997	1214	1215	1217	rVB	260	96	0.01%	0.001%
31	5.074	1218	1239	1282	rBV2	429549	1102622	100.00%	12.732%
32	5.322	1313	1316	1317	rBV	466	247	0.02%	0.003%
33	5.351	1322	1325	1331	rBV2	253	267	0.02%	0.003%
34	5.489	1360	1368	1369	rBV2	362	426	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031720\
 Data File : VV014999.D
 Acq On : 18 Mar 2020 01:58
 Operator : SY/MD
 Sample : L1940-15
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DB0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
 Title : VOC Analysis

35	5.595	1399	1401	1403	rBV	213	85	0.01%	0.001%
36	5.643	1403	1416	1434	rBV	343233	683514	61.99%	7.892%
37	5.878	1486	1489	1492	rBV	366	223	0.02%	0.003%
38	5.929	1497	1505	1510	rBV4	1020	1474	0.13%	0.017%
39	6.097	1542	1557	1582	rBV	241812	491158	44.54%	5.671%
40	6.273	1609	1612	1615	rBV2	504	400	0.04%	0.005%
41	6.318	1624	1626	1629	rVB2	289	142	0.01%	0.002%
42	6.537	1692	1694	1698	rBV2	299	226	0.02%	0.003%
43	6.595	1709	1712	1714	rBV2	199	140	0.01%	0.002%
44	6.753	1758	1761	1764	rBV	250	197	0.02%	0.002%
45	6.849	1787	1791	1792	rBV	344	160	0.01%	0.002%
46	6.949	1819	1822	1825	rBV2	393	254	0.02%	0.003%
47	7.010	1829	1841	1861	rBV	131583	237205	21.51%	2.739%
48	7.151	1883	1885	1886	rBV	366	174	0.02%	0.002%
49	7.187	1892	1896	1897	rBV	296	182	0.02%	0.002%
50	7.228	1907	1909	1911	rVB	268	132	0.01%	0.002%
51	7.241	1911	1913	1915	rBV	277	144	0.01%	0.002%
52	7.254	1915	1917	1920	rVB2	336	199	0.02%	0.002%
53	7.270	1920	1922	1923	rBV	320	149	0.01%	0.002%
54	7.338	1930	1943	1964	rBV	540298	935221	84.82%	10.799%
55	7.643	2022	2038	2056	rBV	92698	157866	14.32%	1.823%
56	7.762	2071	2075	2078	rBV4	458	442	0.04%	0.005%
57	7.778	2078	2080	2081	rBV	261	86	0.01%	0.001%
58	7.826	2091	2095	2096	rBV	349	244	0.02%	0.003%
59	7.865	2105	2107	2111	rBV3	230	156	0.01%	0.002%
60	7.962	2129	2137	2146	rVB4	1642	2505	0.23%	0.029%
61	8.122	2175	2187	2224	rBV2	251076	560400	50.82%	6.471%
62	8.495	2301	2303	2305	rBV	293	139	0.01%	0.002%
63	8.627	2342	2344	2350	rVB3	381	214	0.02%	0.002%
64	8.682	2357	2361	2363	rBV2	238	235	0.02%	0.003%
65	8.743	2378	2380	2386	rVB	335	264	0.02%	0.003%
66	8.772	2386	2389	2392	rBV	179	110	0.01%	0.001%
67	8.826	2402	2406	2407	rBV	334	206	0.02%	0.002%
68	8.875	2408	2421	2450	rVV	520031	865886	78.53%	9.998%
69	9.097	2488	2490	2493	rVB	446	196	0.02%	0.002%
70	9.116	2493	2496	2500	rBV3	317	280	0.03%	0.003%
71	9.244	2533	2536	2537	rBV	312	130	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031720\
 Data File : VV014999.D
 Acq On : 18 Mar 2020 01:58
 Operator : SY/MD
 Sample : L1940-15
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DB0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
 Title : VOC Analysis

72	9.405	2583	2586	2587	rBV	306	148	0.01%	0.002%
73	9.428	2591	2593	2594	rBV	343	85	0.01%	0.001%
74	9.527	2622	2624	2627	rVB	186	65	0.01%	0.001%
75	10.051	2785	2787	2789	rBV2	161	44	0.00%	0.001%
76	10.064	2789	2791	2792	rBV	163	68	0.01%	0.001%
77	10.125	2808	2810	2815	rVB	487	195	0.02%	0.002%
78	10.154	2817	2819	2824	rBB2	355	219	0.02%	0.003%
79	10.238	2832	2845	2865	rBV	373921	588749	53.40%	6.798%
80	10.363	2881	2884	2887	rBV3	373	218	0.02%	0.003%
81	10.675	2979	2981	2983	rBV2	253	104	0.01%	0.001%
82	10.942	3061	3064	3069	rBV2	399	304	0.03%	0.004%
83	11.016	3085	3087	3091	rBV	240	145	0.01%	0.002%
84	11.058	3098	3100	3101	rBV	207	75	0.01%	0.001%
85	11.206	3141	3146	3154	rVB3	3402	4409	0.40%	0.051%
86	11.270	3154	3166	3188	rBV	539652	880566	79.86%	10.168%
87	11.444	3218	3220	3223	rBV	288	212	0.02%	0.002%
88	11.537	3247	3249	3250	rBV	168	38	0.00%	0.000%
89	11.559	3251	3256	3259	rBV3	426	470	0.04%	0.005%
90	11.646	3271	3283	3308	rBV	597585	951889	86.33%	10.991%
91	11.772	3320	3322	3328	rVB4	724	564	0.05%	0.007%
92	11.965	3377	3382	3384	rBV	485	425	0.04%	0.005%
93	12.244	3466	3469	3471	rBV	280	116	0.01%	0.001%
94	12.627	3584	3588	3592	rBV3	520	620	0.06%	0.007%
95	12.672	3595	3602	3608	rVV5	1431	2210	0.20%	0.026%
96	12.916	3676	3678	3682	rBV2	333	244	0.02%	0.003%
97	13.283	3784	3792	3804	rBV	16165	22993	2.09%	0.265%
98	13.958	3999	4002	4004	rBV2	592	335	0.03%	0.004%
99	14.138	4054	4058	4059	rBV3	528	347	0.03%	0.004%
100	14.411	4141	4143	4145	rBV2	786	461	0.04%	0.005%


Sum of corrected areas: 8660320

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV031720\
Data File : VV014999.D
Acq On : 18 Mar 2020 01:58
Operator : SY/MD
Sample : L1940-15
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DB0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

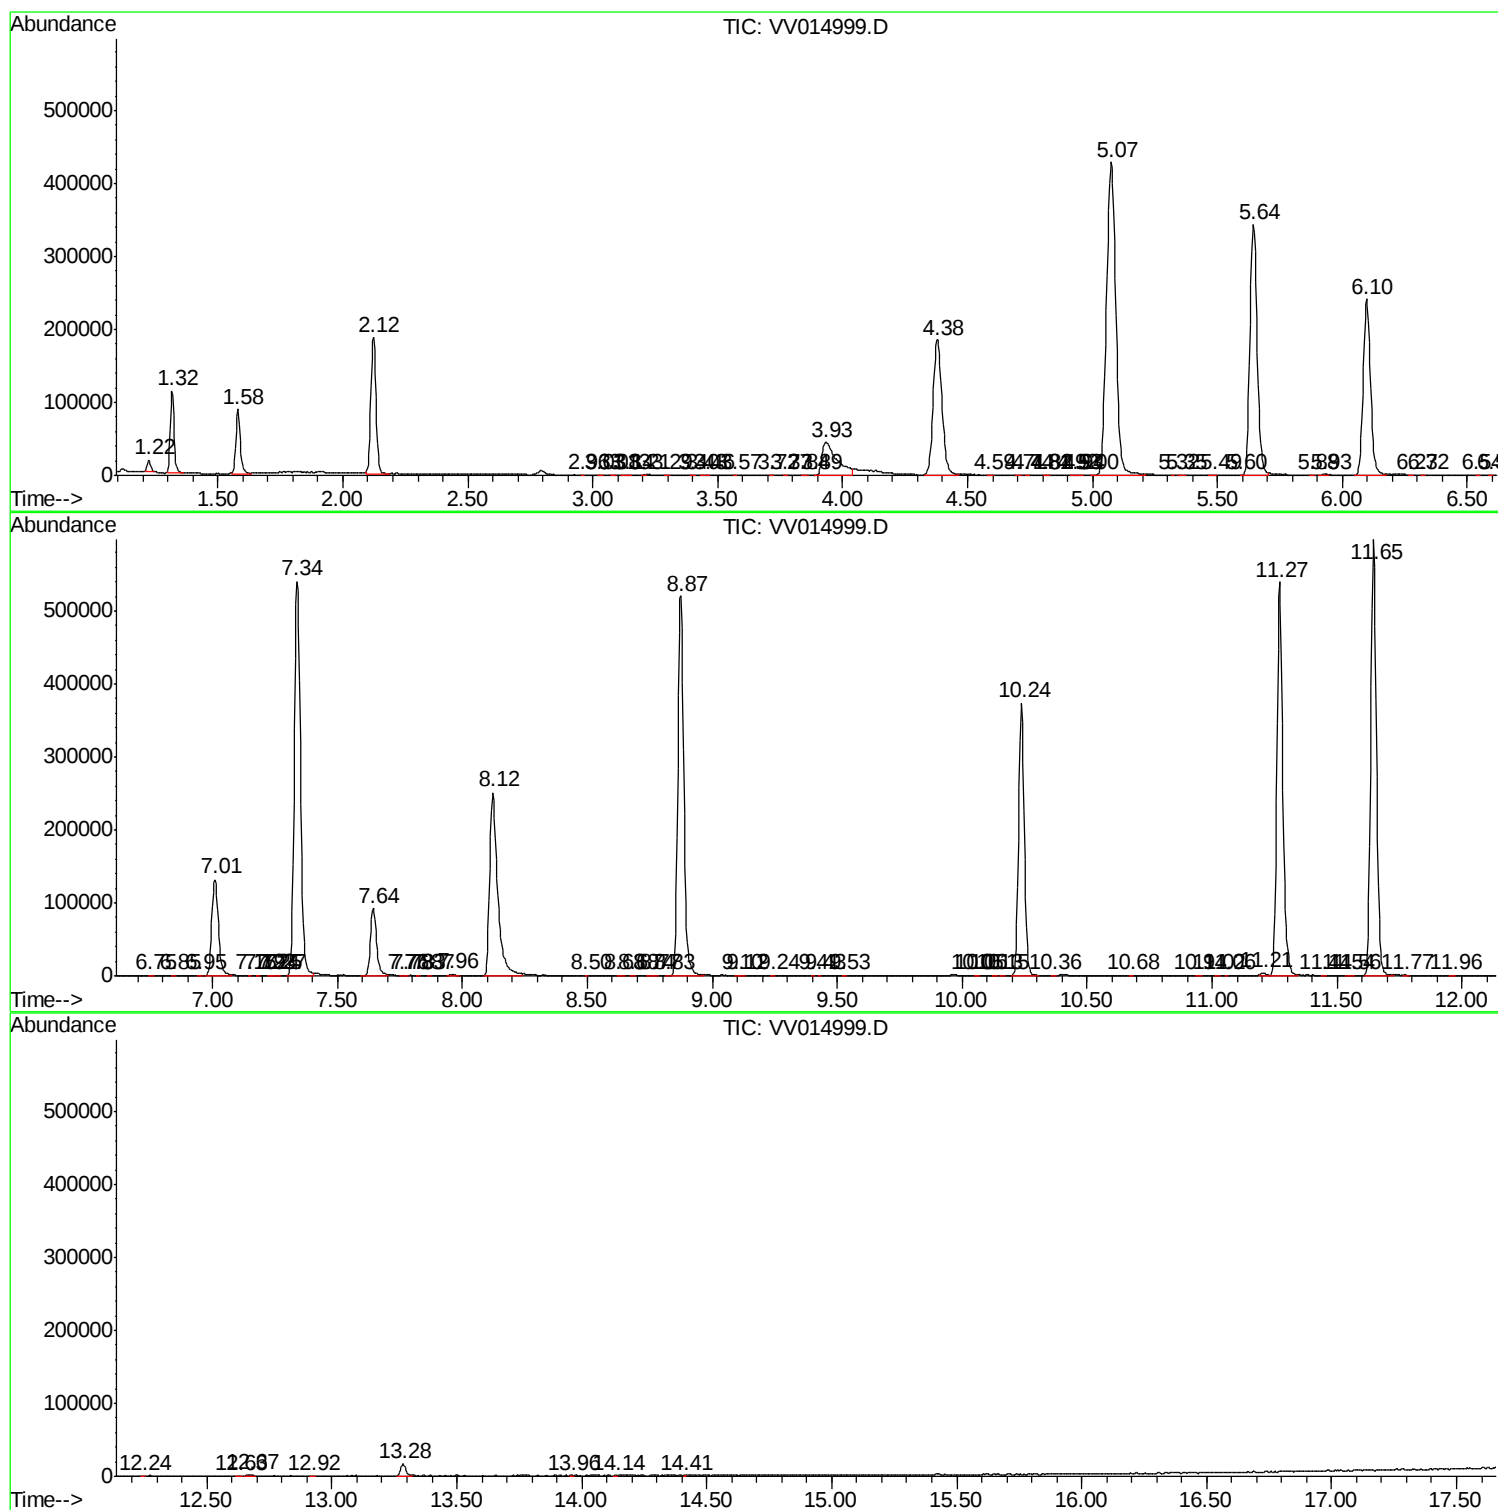

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV031720\
Data File : VV014999.D
Acq On : 18 Mar 2020 01:58
Operator : SY/MD
Sample : L1940-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DB0

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV031720\
Data File : VV014999.D
Acq On : 18 Mar 2020 01:58
Operator : SY/MD
Sample : L1940-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DB0

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc