

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031720\
 Data File : VV015000.D
 Acq On : 18 Mar 2020 02:23
 Operator : SY/MD
 Sample : L1940-17
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DC1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	82	rVB	117509	121289	9.57%	1.292%
2	2.122	313	321	335	rVB	191435	276427	21.82%	2.944%
3	3.212	658	660	663	rBV2	340	154	0.01%	0.002%
4	3.286	678	683	685	rBV2	197	195	0.02%	0.002%
5	3.325	691	695	699	rBV	332	319	0.03%	0.003%
6	3.370	703	709	711	rBV2	321	372	0.03%	0.004%
7	3.412	720	722	727	rBV2	194	81	0.01%	0.001%
8	3.486	742	745	750	rBV3	303	242	0.02%	0.003%
9	3.656	797	798	800	rVB	287	58	0.00%	0.001%
10	3.682	802	806	809	rBV	229	167	0.01%	0.002%
11	3.708	812	814	817	rBV	168	94	0.01%	0.001%
12	3.765	829	832	835	rVB	237	104	0.01%	0.001%
13	3.788	836	839	841	rBV2	287	178	0.01%	0.002%
14	3.833	851	853	854	rVB	24	9	0.00%	0.000%
15	3.846	854	857	859	rBV	390	257	0.02%	0.003%
16	3.933	871	884	926	rBV2	44557	192317	15.18%	2.048%
17	4.380	1006	1023	1050	rBV	182766	443307	34.99%	4.721%
18	4.579	1083	1085	1086	rVB	317	85	0.01%	0.001%
19	4.595	1086	1090	1093	rVB2	559	390	0.03%	0.004%
20	4.711	1124	1126	1130	rVB2	261	165	0.01%	0.002%
21	4.727	1130	1131	1132	rBV2	131	35	0.00%	0.000%
22	4.743	1133	1136	1142	rVV2	392	334	0.03%	0.004%
23	4.804	1152	1155	1156	rBV	258	100	0.01%	0.001%
24	4.913	1186	1189	1192	rBV2	186	157	0.01%	0.002%
25	4.955	1200	1202	1205	rVB	239	94	0.01%	0.001%
26	4.994	1209	1214	1217	rBV2	229	282	0.02%	0.003%
27	5.074	1220	1239	1251	rBV2	426467	1096481	86.55%	11.676%
28	5.363	1326	1329	1332	rBV2	356	289	0.02%	0.003%
29	5.383	1332	1335	1337	rVV2	470	251	0.02%	0.003%
30	5.495	1368	1370	1371	rBV	393	161	0.01%	0.002%
31	5.550	1385	1387	1393	rBV	231	175	0.01%	0.002%
32	5.643	1402	1416	1448	rBV	346040	688414	54.34%	7.331%
33	5.839	1474	1477	1485	rVB3	444	552	0.04%	0.006%
34	5.884	1485	1491	1492	rBV2	617	456	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031720\
 Data File : VV015000.D
 Acq On : 18 Mar 2020 02:23
 Operator : SY/MD
 Sample : L1940-17
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DC1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
 Title : VOC Analysis

35	5.926	1500	1504	1509	rBV4	899	1096	0.09%	0.012%
36	5.965	1514	1516	1517	rBV4	193	78	0.01%	0.001%
37	6.035	1537	1538	1542	rVB2	304	134	0.01%	0.001%
38	6.097	1542	1557	1579	rBV	240644	488700	38.57%	5.204%
39	6.312	1621	1624	1627	rVB	383	212	0.02%	0.002%
40	6.347	1633	1635	1638	rVB	254	108	0.01%	0.001%
41	6.367	1638	1641	1645	rVB2	322	225	0.02%	0.002%
42	6.418	1654	1657	1660	rVB	352	200	0.02%	0.002%
43	6.502	1681	1683	1690	rVB2	316	272	0.02%	0.003%
44	6.833	1785	1786	1787	rBV	191	70	0.01%	0.001%
45	6.859	1793	1794	1799	rVB	276	121	0.01%	0.001%
46	7.010	1829	1841	1870	rBV	120563	217244	17.15%	2.313%
47	7.158	1885	1887	1892	rVB3	633	380	0.03%	0.004%
48	7.228	1906	1909	1912	rBV2	298	168	0.01%	0.002%
49	7.289	1925	1928	1930	rBV	303	181	0.01%	0.002%
50	7.338	1930	1943	1966	rBV	533687	933021	73.64%	9.936%
51	7.643	2027	2038	2058	rBV	78150	135208	10.67%	1.440%
52	7.785	2079	2082	2084	rBV3	369	206	0.02%	0.002%
53	7.852	2100	2103	2106	rVB3	510	309	0.02%	0.003%
54	7.894	2113	2116	2119	rBV2	308	236	0.02%	0.003%
55	7.952	2129	2134	2136	rBV	689	609	0.05%	0.006%
56	8.122	2175	2187	2216	rBV	235280	543614	42.91%	5.789%
57	8.421	2276	2280	2283	rBV2	362	290	0.02%	0.003%
58	8.527	2311	2313	2315	rBV2	193	88	0.01%	0.001%
59	8.669	2355	2357	2361	rBV	499	294	0.02%	0.003%
60	8.762	2381	2386	2390	rBV2	360	320	0.03%	0.003%
61	8.788	2390	2394	2399	rBV3	349	400	0.03%	0.004%
62	8.875	2408	2421	2426	rBV	546732	922006	72.77%	9.818%
63	9.276	2544	2546	2549	rBV	291	170	0.01%	0.002%
64	9.450	2598	2600	2603	rBV	177	80	0.01%	0.001%
65	9.508	2611	2618	2620	rBV	229	323	0.03%	0.003%
66	9.588	2641	2643	2647	rVV2	232	102	0.01%	0.001%
67	9.608	2647	2649	2651	rVB	213	88	0.01%	0.001%
68	9.817	2709	2714	2717	rBV2	255	251	0.02%	0.003%
69	9.862	2726	2728	2729	rBV2	193	58	0.00%	0.001%
70	9.968	2758	2761	2763	rBV	332	156	0.01%	0.002%
71	10.077	2794	2795	2796	rBV	137	40	0.00%	0.000%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031720\
 Data File : VV015000.D
 Acq On : 18 Mar 2020 02:23
 Operator : SY/MD
 Sample : L1940-17
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DC1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
 Title : VOC Analysis

72	10.238	2832	2845	2864	rBV	375842	587133	46.34%	6.252%
73	10.402	2893	2896	2907	rVB4	1691	2386	0.19%	0.025%
74	10.482	2918	2921	2922	rBV	208	116	0.01%	0.001%
75	10.739	2998	3001	3003	rBV2	282	155	0.01%	0.002%
76	10.749	3003	3004	3005	rBV2	323	95	0.01%	0.001%
77	10.910	3051	3054	3055	rBV	324	147	0.01%	0.002%
78	11.202	3136	3145	3155	rBV	32341	49964	3.94%	0.532%
79	11.270	3155	3166	3190	rVB2	568286	1164702	91.93%	12.403%
80	11.405	3206	3208	3214	rVB4	549	419	0.03%	0.004%
81	11.450	3220	3222	3227	rBV2	459	262	0.02%	0.003%
82	11.498	3234	3237	3238	rBV2	240	146	0.01%	0.002%
83	11.553	3252	3254	3261	rVB3	703	492	0.04%	0.005%
84	11.646	3268	3283	3305	rBV2	649146	1266936	100.00%	13.492%
85	12.350	3498	3502	3505	rBV2	523	457	0.04%	0.005%
86	12.498	3544	3548	3557	rBV3	370	496	0.04%	0.005%
87	12.643	3590	3593	3595	rBV2	592	412	0.03%	0.004%
88	12.820	3646	3648	3650	rBV	225	122	0.01%	0.001%
89	12.910	3674	3676	3679	rBV	307	166	0.01%	0.002%
90	13.283	3782	3792	3809	rVB2	124132	191116	15.08%	2.035%
91	13.640	3900	3903	3905	rBV	446	349	0.03%	0.004%
92	13.768	3933	3943	3955	rBV2	35065	53411	4.22%	0.569%


Sum of corrected areas: 9390531

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV031720\
Data File : VV015000.D
Acq On : 18 Mar 2020 02:23
Operator : SY/MD
Sample : L1940-17
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DC1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

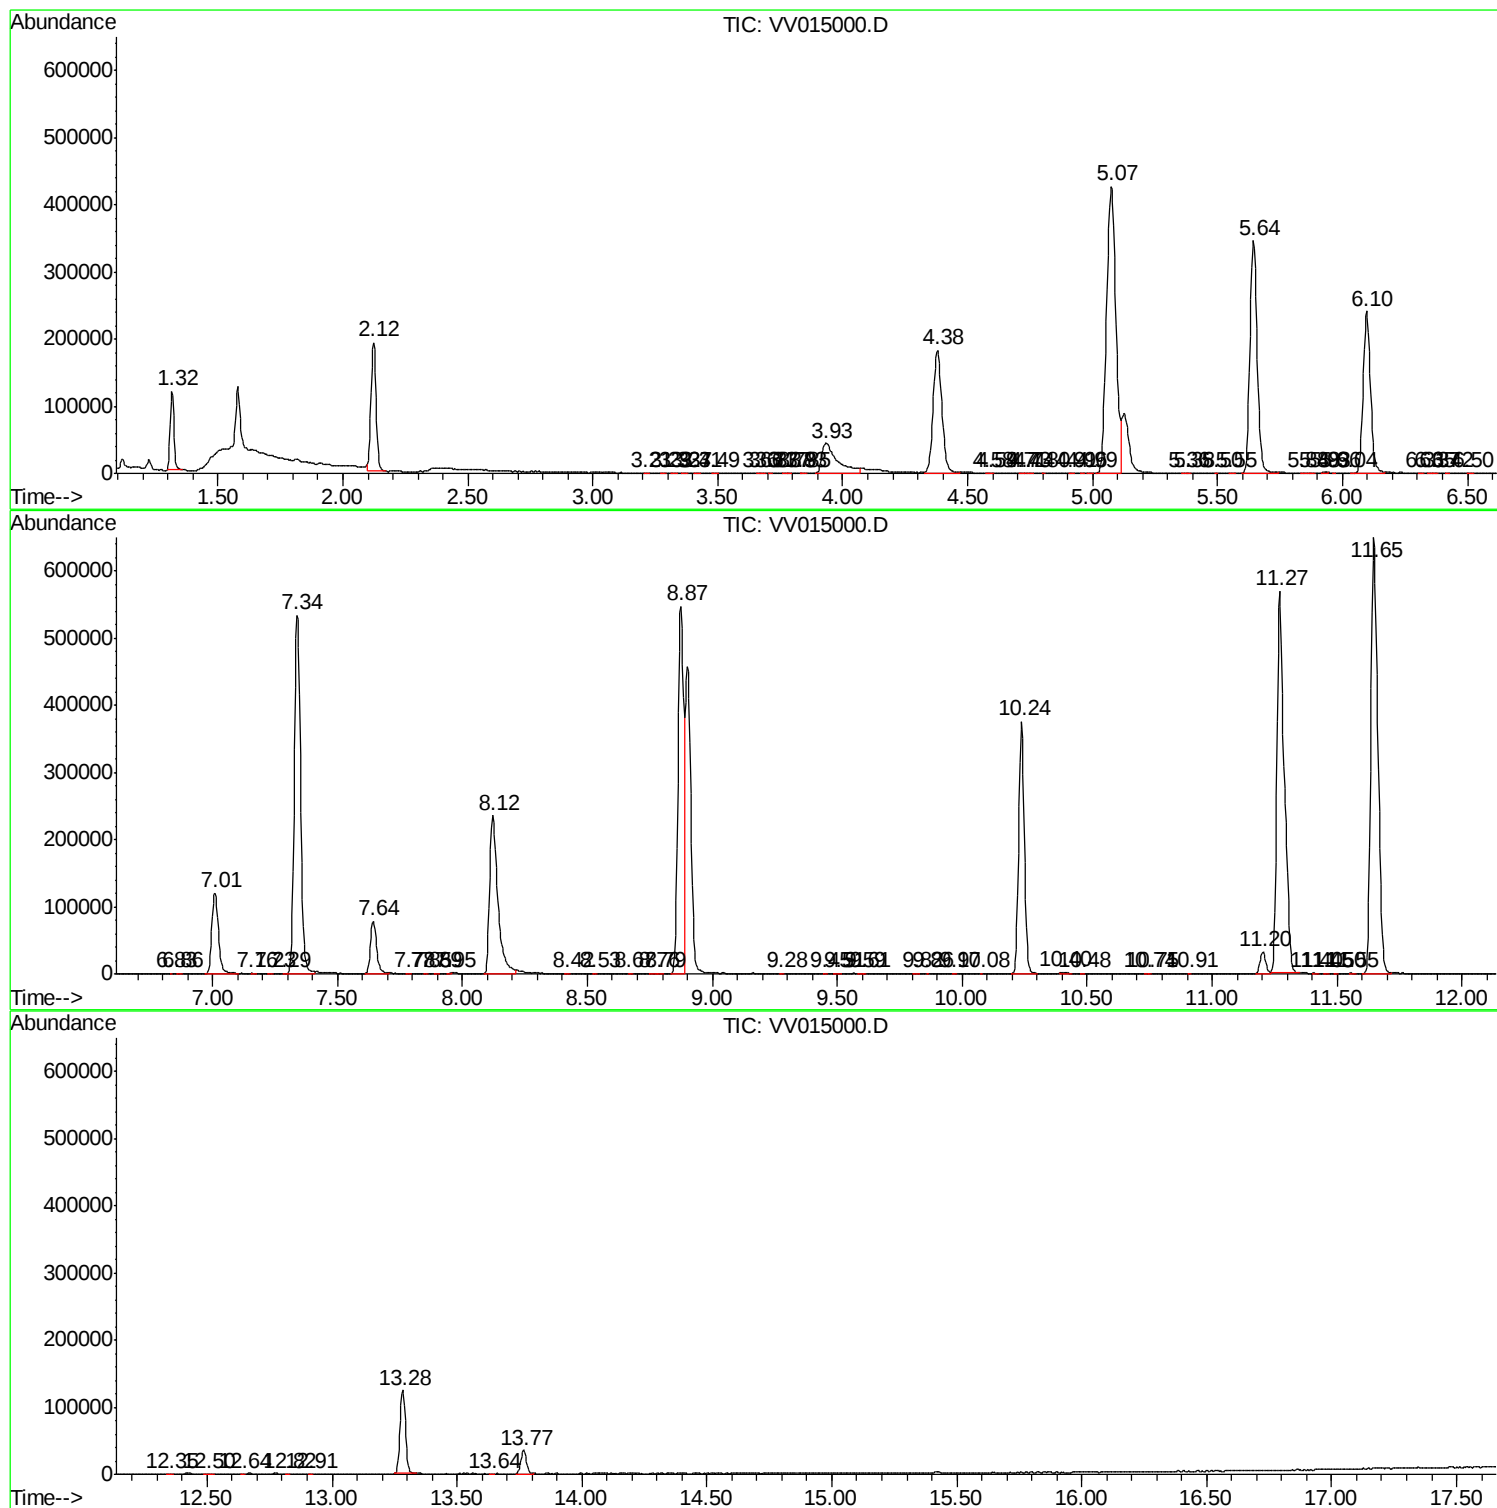

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV031720\
Data File : VV015000.D
Acq On : 18 Mar 2020 02:23
Operator : SY/MD
Sample : L1940-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DC1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV031720\
Data File : VV015000.D
Acq On : 18 Mar 2020 02:23
Operator : SY/MD
Sample : L1940-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DC1

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc