

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031720\
 Data File : VV015001.D
 Acq On : 18 Mar 2020 02:47
 Operator : SY/MD
 Sample : L1890-13
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DG0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	86	rVB	112978	116029	10.77%	1.378%
2	1.579	145	152	163	rBV	89904	104944	9.74%	1.246%
3	2.119	312	320	337	rVB	179784	263885	24.50%	3.133%
4	2.859	548	550	552	rBV2	461	248	0.02%	0.003%
5	3.103	624	626	628	rVB	458	142	0.01%	0.002%
6	3.116	628	630	636	rVB2	457	364	0.03%	0.004%
7	3.151	636	641	643	rBV3	439	357	0.03%	0.004%
8	3.196	653	655	658	rBV	251	102	0.01%	0.001%
9	3.257	667	674	676	rBV2	310	383	0.04%	0.005%
10	3.309	688	690	692	rBV	136	49	0.00%	0.001%
11	3.556	765	767	768	rBV	184	101	0.01%	0.001%
12	3.939	872	886	916	rBV2	41927	173528	16.11%	2.060%
13	4.376	1006	1022	1047	rBV2	178223	441430	40.98%	5.241%
14	4.640	1102	1104	1107	rBV2	260	133	0.01%	0.002%
15	4.833	1159	1164	1167	rBV2	523	380	0.04%	0.005%
16	4.926	1191	1193	1194	rBV2	165	52	0.00%	0.001%
17	4.965	1203	1205	1209	rVB2	224	102	0.01%	0.001%
18	5.074	1221	1239	1262	rBV2	425583	1077201	100.00%	12.789%
19	5.328	1316	1318	1321	rBV3	239	167	0.02%	0.002%
20	5.412	1342	1344	1346	rBV	318	173	0.02%	0.002%
21	5.643	1399	1416	1436	rBV	343322	683097	63.41%	8.110%
22	5.929	1500	1505	1512	rBV4	1124	1338	0.12%	0.016%
23	6.026	1533	1535	1536	rBV	207	90	0.01%	0.001%
24	6.097	1542	1557	1582	rBV	235777	485325	45.05%	5.762%
25	6.344	1632	1634	1636	rBV	205	77	0.01%	0.001%
26	6.489	1677	1679	1681	rBV	296	118	0.01%	0.001%
27	6.589	1708	1710	1713	rBV	271	156	0.01%	0.002%
28	6.762	1762	1764	1765	rBV	126	50	0.00%	0.001%
29	6.817	1779	1781	1784	rBV3	366	145	0.01%	0.002%
30	7.010	1829	1841	1866	rBV	125572	226278	21.01%	2.687%
31	7.161	1886	1888	1893	rVB3	607	384	0.04%	0.005%
32	7.264	1917	1920	1924	rVB	379	228	0.02%	0.003%
33	7.338	1930	1943	1965	rBV	529425	919969	85.40%	10.922%
34	7.643	2027	2038	2069	rVB	86457	150657	13.99%	1.789%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031720\
 Data File : VV015001.D
 Acq On : 18 Mar 2020 02:47
 Operator : SY/MD
 Sample : L1890-13
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DG0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
 Title : VOC Analysis

35	7.775	2076	2079	2082	rBV2	297	197	0.02%	0.002%
36	7.801	2086	2087	2090	rBV	348	104	0.01%	0.001%
37	7.859	2102	2105	2107	rBV	271	181	0.02%	0.002%
38	7.910	2119	2121	2124	rBV	329	127	0.01%	0.002%
39	7.958	2132	2136	2137	rBV	759	497	0.05%	0.006%
40	8.010	2149	2152	2155	rVB	369	271	0.03%	0.003%
41	8.035	2155	2160	2165	rBV2	480	551	0.05%	0.007%
42	8.122	2176	2187	2222	rBV	242631	555975	51.61%	6.601%
43	8.315	2244	2247	2249	rBV2	603	352	0.03%	0.004%
44	8.486	2298	2300	2304	rVB	530	304	0.03%	0.004%
45	8.508	2304	2307	2310	rBV2	299	182	0.02%	0.002%
46	8.875	2408	2421	2447	rBV	518476	862328	80.05%	10.238%
47	9.161	2504	2510	2518	rBV4	574	827	0.08%	0.010%
48	9.338	2562	2565	2568	rBV2	227	193	0.02%	0.002%
49	9.559	2631	2634	2641	rBV3	463	535	0.05%	0.006%
50	9.608	2648	2649	2650	rBV3	246	59	0.01%	0.001%
51	9.707	2677	2680	2683	rBV	352	193	0.02%	0.002%
52	9.949	2753	2755	2758	rBV	377	175	0.02%	0.002%
53	10.238	2833	2845	2864	rBV	372862	584014	54.22%	6.934%
54	10.373	2883	2887	2891	rBV2	492	479	0.04%	0.006%
55	10.408	2891	2898	2904	rVV5	1331	1640	0.15%	0.019%
56	10.804	3019	3021	3023	rBV2	228	120	0.01%	0.001%
57	10.878	3041	3044	3045	rBV	370	218	0.02%	0.003%
58	11.026	3088	3090	3092	rBV	280	113	0.01%	0.001%
59	11.270	3154	3166	3189	rBV	537102	839729	77.95%	9.970%
60	11.646	3270	3283	3303	rBV	568161	904900	84.00%	10.744%
61	11.775	3321	3323	3325	rBV	488	250	0.02%	0.003%
62	11.839	3342	3343	3346	rBV	286	104	0.01%	0.001%
63	12.373	3506	3509	3510	rBV	340	191	0.02%	0.002%
64	12.421	3522	3524	3525	rBV	258	80	0.01%	0.001%
65	12.688	3604	3607	3608	rBV	370	201	0.02%	0.002%
66	13.170	3754	3757	3760	rBV	528	396	0.04%	0.005%
67	13.286	3784	3793	3807	rVB5	10591	16781	1.56%	0.199%
68	13.768	3937	3943	3953	rBV7	1915	2785	0.26%	0.033%


Sum of corrected areas: 8422734

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV031720\
Data File : VV015001.D
Acq On : 18 Mar 2020 02:47
Operator : SY/MD
Sample : L1890-13
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DG0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

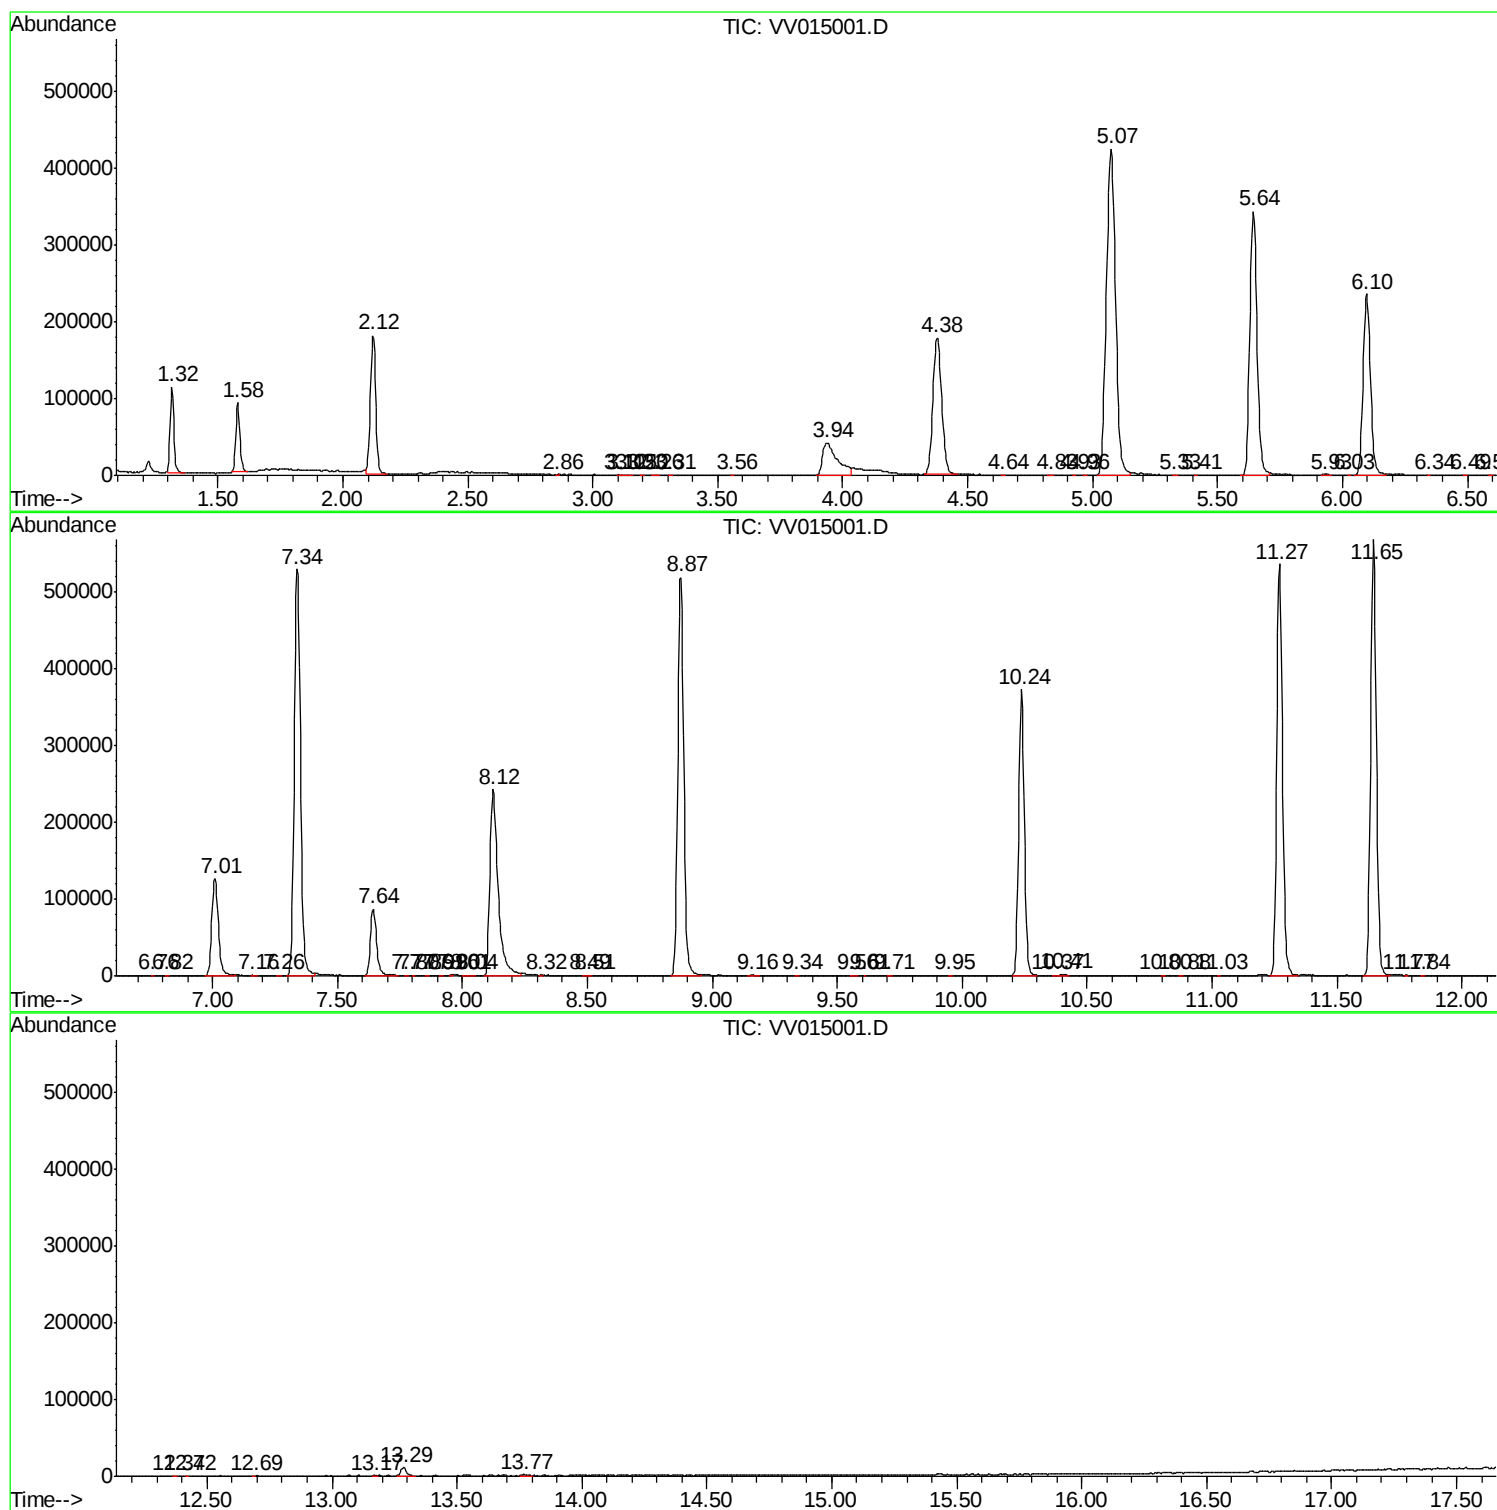

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV031720\
Data File : VV015001.D
Acq On : 18 Mar 2020 02:47
Operator : SY/MD
Sample : L1890-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DG0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV031720\
Data File : VV015001.D
Acq On : 18 Mar 2020 02:47
Operator : SY/MD
Sample : L1890-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DG0

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
