

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031720\
 Data File : VV015003.D
 Acq On : 18 Mar 2020 03:35
 Operator : SY/MD
 Sample : L1890-14
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DG1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	87	rVB	106689	112076	10.42%	1.351%
2	1.579	145	152	166	rVB	88457	106321	9.89%	1.282%
3	2.122	311	321	333	rBV	179182	254394	23.66%	3.067%
4	3.007	594	596	600	rBV2	359	300	0.03%	0.004%
5	3.093	618	623	627	rBV3	522	587	0.05%	0.007%
6	3.286	678	683	689	rBV2	408	415	0.04%	0.005%
7	3.338	695	699	700	rBV	267	162	0.02%	0.002%
8	3.376	706	711	712	rBV	353	247	0.02%	0.003%
9	3.399	716	718	720	rVB	274	112	0.01%	0.001%
10	3.595	777	779	780	rBV	218	85	0.01%	0.001%
11	3.846	855	857	859	rBV	202	72	0.01%	0.001%
12	3.894	869	872	873	rBV	332	172	0.02%	0.002%
13	3.933	873	884	905	rBV	42466	152242	14.16%	1.836%
14	4.380	1008	1023	1047	rVB	175306	432811	40.25%	5.218%
15	4.688	1117	1119	1125	rVB3	510	394	0.04%	0.005%
16	4.714	1125	1127	1128	rBV3	249	78	0.01%	0.001%
17	4.724	1128	1130	1131	rBV	143	41	0.00%	0.000%
18	4.875	1175	1177	1182	rVB2	382	280	0.03%	0.003%
19	4.894	1182	1183	1184	rBV	129	38	0.00%	0.000%
20	4.945	1197	1199	1200	rBV	197	93	0.01%	0.001%
21	4.955	1200	1202	1205	rVV	269	167	0.02%	0.002%
22	4.990	1211	1213	1217	rVB2	394	212	0.02%	0.003%
23	5.007	1217	1218	1219	rBV2	347	120	0.01%	0.001%
24	5.074	1221	1239	1268	rBV2	429574	1075185	100.00%	12.964%
25	5.289	1303	1306	1309	rBV4	484	294	0.03%	0.004%
26	5.341	1320	1322	1324	rBV	337	165	0.02%	0.002%
27	5.444	1352	1354	1357	rBV2	211	134	0.01%	0.002%
28	5.460	1357	1359	1360	rBV	128	32	0.00%	0.000%
29	5.508	1369	1374	1376	rBV3	489	363	0.03%	0.004%
30	5.643	1403	1416	1436	rBV	339056	671300	62.44%	8.094%
31	5.855	1480	1482	1485	rBV	503	267	0.02%	0.003%
32	5.894	1491	1494	1495	rBV2	353	181	0.02%	0.002%
33	6.096	1542	1557	1581	rBV	235362	482390	44.87%	5.816%
34	6.264	1607	1609	1610	rBV	305	150	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031720\
 Data File : VV015003.D
 Acq On : 18 Mar 2020 03:35
 Operator : SY/MD
 Sample : L1890-14
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DG1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
 Title : VOC Analysis

35	6.486	1676	1678	1681	rBV2	184	100	0.01%	0.001%
36	6.543	1694	1696	1699	rBV2	293	168	0.02%	0.002%
37	6.762	1761	1764	1767	rBV3	217	145	0.01%	0.002%
38	6.788	1771	1772	1775	rVB2	223	65	0.01%	0.001%
39	6.846	1788	1790	1792	rBB	207	77	0.01%	0.001%
40	7.010	1829	1841	1856	rBV	127328	227151	21.13%	2.739%
41	7.138	1877	1881	1883	rBV4	461	325	0.03%	0.004%
42	7.241	1911	1913	1917	rBV2	253	123	0.01%	0.001%
43	7.260	1917	1919	1926	rBV2	332	282	0.03%	0.003%
44	7.338	1930	1943	1981	rBV	528597	920262	85.59%	11.096%
45	7.553	2008	2010	2013	rBV2	408	258	0.02%	0.003%
46	7.592	2017	2022	2026	rBV3	537	470	0.04%	0.006%
47	7.643	2026	2038	2057	rBV	90572	153559	14.28%	1.851%
48	7.785	2079	2082	2085	rVB2	305	146	0.01%	0.002%
49	7.817	2090	2092	2095	rVB	311	125	0.01%	0.002%
50	7.910	2118	2121	2124	rVB	484	244	0.02%	0.003%
51	8.022	2153	2156	2159	rBV2	344	197	0.02%	0.002%
52	8.122	2175	2187	2222	rBV2	243729	562026	52.27%	6.776%
53	8.309	2244	2245	2250	rBV3	541	353	0.03%	0.004%
54	8.415	2275	2278	2280	rBV2	373	206	0.02%	0.002%
55	8.662	2353	2355	2361	rVB	382	284	0.03%	0.003%
56	8.707	2366	2369	2371	rBV	255	207	0.02%	0.002%
57	8.807	2397	2400	2403	rBV3	335	239	0.02%	0.003%
58	8.875	2408	2421	2440	rBV	511417	836884	77.84%	10.090%
59	9.035	2469	2471	2474	rBV3	641	487	0.05%	0.006%
60	9.138	2501	2503	2504	rBV	239	77	0.01%	0.001%
61	9.222	2527	2529	2531	rVB	175	48	0.00%	0.001%
62	9.315	2556	2558	2560	rBV	254	100	0.01%	0.001%
63	9.521	2618	2622	2625	rBV	291	256	0.02%	0.003%
64	9.871	2728	2731	2735	rBV2	320	303	0.03%	0.004%
65	10.238	2833	2845	2864	rBV	367766	584011	54.32%	7.042%
66	10.321	2869	2871	2875	rBV	448	309	0.03%	0.004%
67	10.386	2889	2891	2893	rBV	370	243	0.02%	0.003%
68	10.556	2942	2944	2946	rVB	367	83	0.01%	0.001%
69	10.701	2987	2989	2992	rBV	229	73	0.01%	0.001%
70	10.791	3015	3017	3019	rBV	252	166	0.02%	0.002%
71	10.871	3040	3042	3046	rVB	471	222	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031720\
 Data File : VV015003.D
 Acq On : 18 Mar 2020 03:35
 Operator : SY/MD
 Sample : L1890-14
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DG1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
 Title : VOC Analysis

72	10.919	3055	3057	3058	rBV	238	51	0.00%	0.001%
73	11.048	3095	3097	3098	rBV	317	106	0.01%	0.001%
74	11.177	3135	3137	3138	rBV	184	64	0.01%	0.001%
75	11.270	3154	3166	3185	rBV	520548	807509	75.10%	9.736%
76	11.479	3228	3231	3234	rBV2	318	205	0.02%	0.002%
77	11.559	3253	3256	3257	rBV	683	313	0.03%	0.004%
78	11.646	3270	3283	3304	rBV	575854	895010	83.24%	10.791%
79	12.035	3402	3404	3408	rBV	281	177	0.02%	0.002%
80	12.096	3420	3423	3426	rVB2	419	245	0.02%	0.003%
81	12.228	3462	3464	3469	rBV	396	247	0.02%	0.003%
82	12.505	3547	3550	3554	rBV2	384	306	0.03%	0.004%
83	12.617	3584	3585	3586	rBV2	223	66	0.01%	0.001%
84	12.672	3599	3602	3607	rBV4	426	411	0.04%	0.005%
85	13.286	3786	3793	3803	rVB5	4617	6920	0.64%	0.083%


Sum of corrected areas: 8293784

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV031720\
Data File : VV015003.D
Acq On : 18 Mar 2020 03:35
Operator : SY/MD
Sample : L1890-14
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DG1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

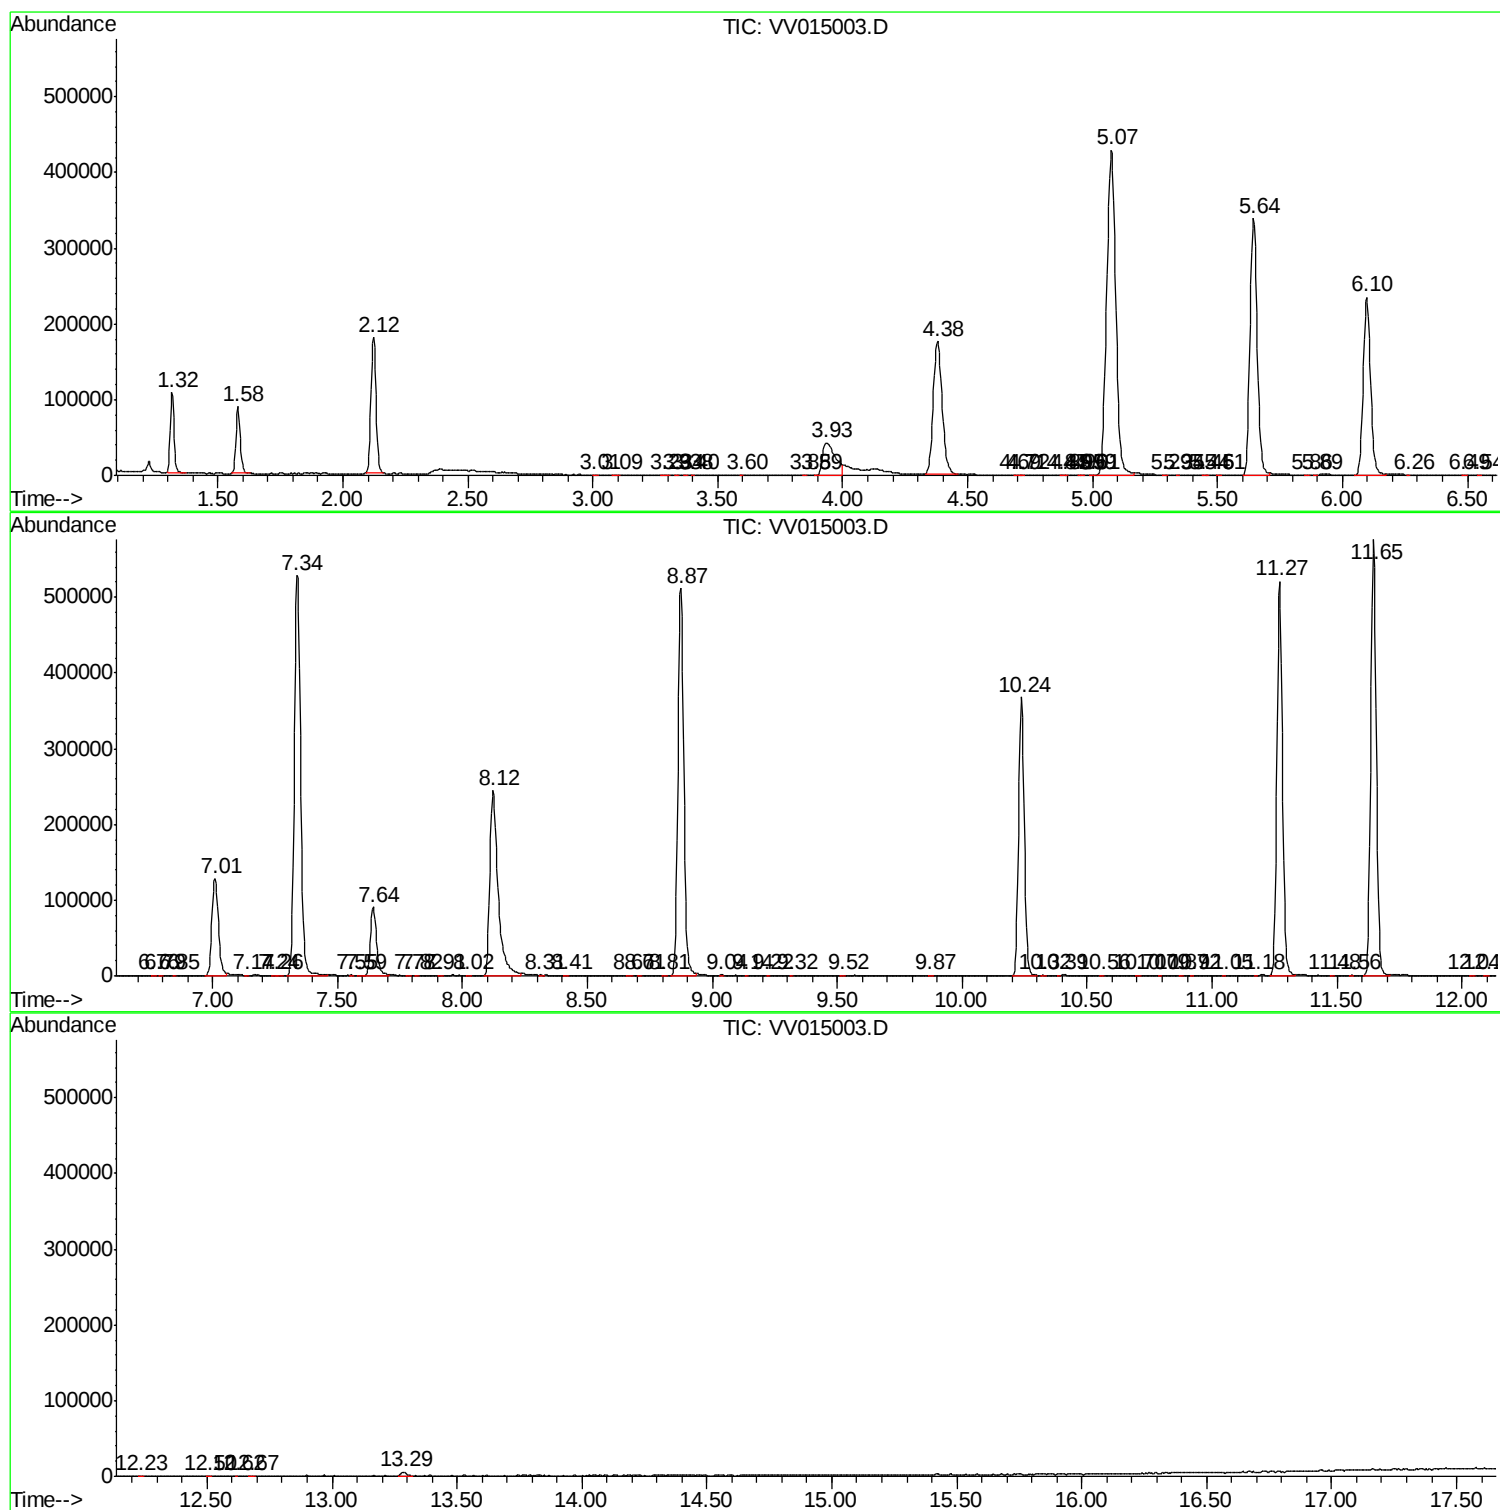

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV031720\
Data File : VV015003.D
Acq On : 18 Mar 2020 03:35
Operator : SY/MD
Sample : L1890-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DG1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV031720\
Data File : VV015003.D
Acq On : 18 Mar 2020 03:35
Operator : SY/MD
Sample : L1890-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DG1

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc