

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031720\
 Data File : VV015006.D
 Acq On : 18 Mar 2020 04:48
 Operator : SY/MD
 Sample : L1940-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D88

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	84	rVB	127670	132825	11.64%	1.540%
2	1.579	145	152	166	rVB	98673	119628	10.48%	1.387%
3	2.122	310	321	337	rBV	207735	299069	26.21%	3.467%
4	3.116	627	630	635	rBV2	459	421	0.04%	0.005%
5	3.209	657	659	661	rVB2	560	223	0.02%	0.003%
6	3.219	661	662	664	rBV	351	170	0.01%	0.002%
7	3.257	672	674	676	rBV	298	151	0.01%	0.002%
8	3.273	676	679	681	rVV	266	147	0.01%	0.002%
9	3.425	724	726	729	rBV	233	113	0.01%	0.001%
10	3.441	729	731	734	rBV2	239	180	0.02%	0.002%
11	3.656	797	798	801	rBV2	275	185	0.02%	0.002%
12	3.830	849	852	853	rBV	220	138	0.01%	0.002%
13	3.881	866	868	872	rBV2	228	144	0.01%	0.002%
14	3.933	873	884	903	rBV2	40658	142885	12.52%	1.657%
15	4.379	1008	1023	1050	rVB2	182748	460010	40.32%	5.333%
16	4.579	1082	1085	1087	rBV	309	208	0.02%	0.002%
17	4.698	1120	1122	1125	rVB2	352	135	0.01%	0.002%
18	4.717	1125	1128	1129	rBV2	281	160	0.01%	0.002%
19	4.791	1149	1151	1153	rBV	220	133	0.01%	0.002%
20	4.846	1166	1168	1171	rBV	122	73	0.01%	0.001%
21	4.865	1171	1174	1176	rBV	249	203	0.02%	0.002%
22	4.897	1181	1184	1186	rBV	247	125	0.01%	0.001%
23	4.910	1186	1188	1189	rBV	328	115	0.01%	0.001%
24	5.074	1219	1239	1266	rBV2	443363	1140946	100.00%	13.228%
25	5.299	1306	1309	1312	rBV2	676	526	0.05%	0.006%
26	5.402	1339	1341	1342	rBV	332	138	0.01%	0.002%
27	5.441	1352	1353	1355	rVB	343	92	0.01%	0.001%
28	5.553	1383	1388	1392	rBV	282	327	0.03%	0.004%
29	5.643	1402	1416	1441	rBV	356266	703051	61.62%	8.151%
30	5.926	1499	1504	1507	rBV4	956	1114	0.10%	0.013%
31	5.981	1519	1521	1523	rVB	277	76	0.01%	0.001%
32	6.096	1543	1557	1581	rBV	248526	504856	44.25%	5.853%
33	6.309	1621	1623	1626	rBV	258	104	0.01%	0.001%
34	6.367	1638	1641	1645	rVB	588	431	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031720\
 Data File : VV015006.D
 Acq On : 18 Mar 2020 04:48
 Operator : SY/MD
 Sample : L1940-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D88

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
 Title : VOC Analysis

35	6.389	1645	1648	1650	rBV	372	224	0.02%	0.003%
36	6.450	1666	1667	1671	rVB2	322	94	0.01%	0.001%
37	6.537	1692	1694	1696	rBV2	258	120	0.01%	0.001%
38	6.672	1734	1736	1737	rBV	227	82	0.01%	0.001%
39	6.714	1747	1749	1752	rVB	281	133	0.01%	0.002%
40	6.733	1752	1755	1757	rBV	216	141	0.01%	0.002%
41	6.781	1768	1770	1774	rBV	235	184	0.02%	0.002%
42	7.010	1830	1841	1860	rBV	123733	223117	19.56%	2.587%
43	7.167	1886	1890	1893	rBV2	415	300	0.03%	0.003%
44	7.202	1899	1901	1903	rBV2	268	126	0.01%	0.001%
45	7.338	1930	1943	1972	rBV	562307	985646	86.39%	11.428%
46	7.559	2008	2012	2014	rBV2	351	316	0.03%	0.004%
47	7.643	2026	2038	2052	rBV	82476	145277	12.73%	1.684%
48	7.791	2082	2084	2085	rVB	207	49	0.00%	0.001%
49	7.842	2097	2100	2103	rVB2	316	166	0.01%	0.002%
50	7.874	2108	2110	2112	rVB	408	163	0.01%	0.002%
51	7.903	2117	2119	2123	rVB	372	132	0.01%	0.002%
52	8.000	2147	2149	2150	rBV	138	43	0.00%	0.000%
53	8.010	2150	2152	2153	rBV	204	59	0.01%	0.001%
54	8.122	2175	2187	2214	rBV2	236020	543396	47.63%	6.300%
55	8.399	2271	2273	2276	rVB3	412	239	0.02%	0.003%
56	8.437	2282	2285	2288	rBV2	434	301	0.03%	0.003%
57	8.874	2408	2421	2444	rBV	530741	869246	76.19%	10.078%
58	9.170	2507	2513	2518	rVB4	591	677	0.06%	0.008%
59	9.231	2530	2532	2533	rBV	220	54	0.00%	0.001%
60	9.315	2553	2558	2561	rBV2	358	326	0.03%	0.004%
61	9.543	2627	2629	2636	rVB2	395	293	0.03%	0.003%
62	9.575	2637	2639	2642	rBV2	164	94	0.01%	0.001%
63	9.788	2702	2705	2707	rBV	437	265	0.02%	0.003%
64	9.845	2722	2723	2725	rBV	251	80	0.01%	0.001%
65	9.964	2758	2760	2762	rBV	292	158	0.01%	0.002%
66	10.045	2784	2785	2787	rBV	249	90	0.01%	0.001%
67	10.083	2793	2797	2800	rBV	454	310	0.03%	0.004%
68	10.238	2832	2845	2864	rBV	373578	583286	51.12%	6.763%
69	10.479	2917	2920	2924	rBV2	266	190	0.02%	0.002%
70	10.993	3078	3080	3084	rVB	317	168	0.01%	0.002%
71	11.016	3084	3087	3088	rBV	229	118	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031720\
Data File : VV015006.D
Acq On : 18 Mar 2020 04:48
Operator : SY/MD
Sample : L1940-01
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0D88

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Title : VOC Analysis

72	11.199	3140	3144	3152	rVB3	472	720	0.06%	0.008%
73	11.270	3154	3166	3184	rBV	539509	834905	73.18%	9.680%
74	11.562	3252	3257	3259	rBV2	560	513	0.04%	0.006%
75	11.646	3270	3283	3303	rBV	587071	923177	80.91%	10.703%
76	11.884	3355	3357	3359	rBV	413	194	0.02%	0.002%
77	12.019	3396	3399	3404	rVB2	359	307	0.03%	0.004%
78	12.607	3580	3582	3587	rVB2	404	239	0.02%	0.003%
79	13.035	3713	3715	3717	rBV2	364	226	0.02%	0.003%


Sum of corrected areas: 8625046

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV031720\
Data File : VV015006.D
Acq On : 18 Mar 2020 04:48
Operator : SY/MD
Sample : L1940-01
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0D88

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

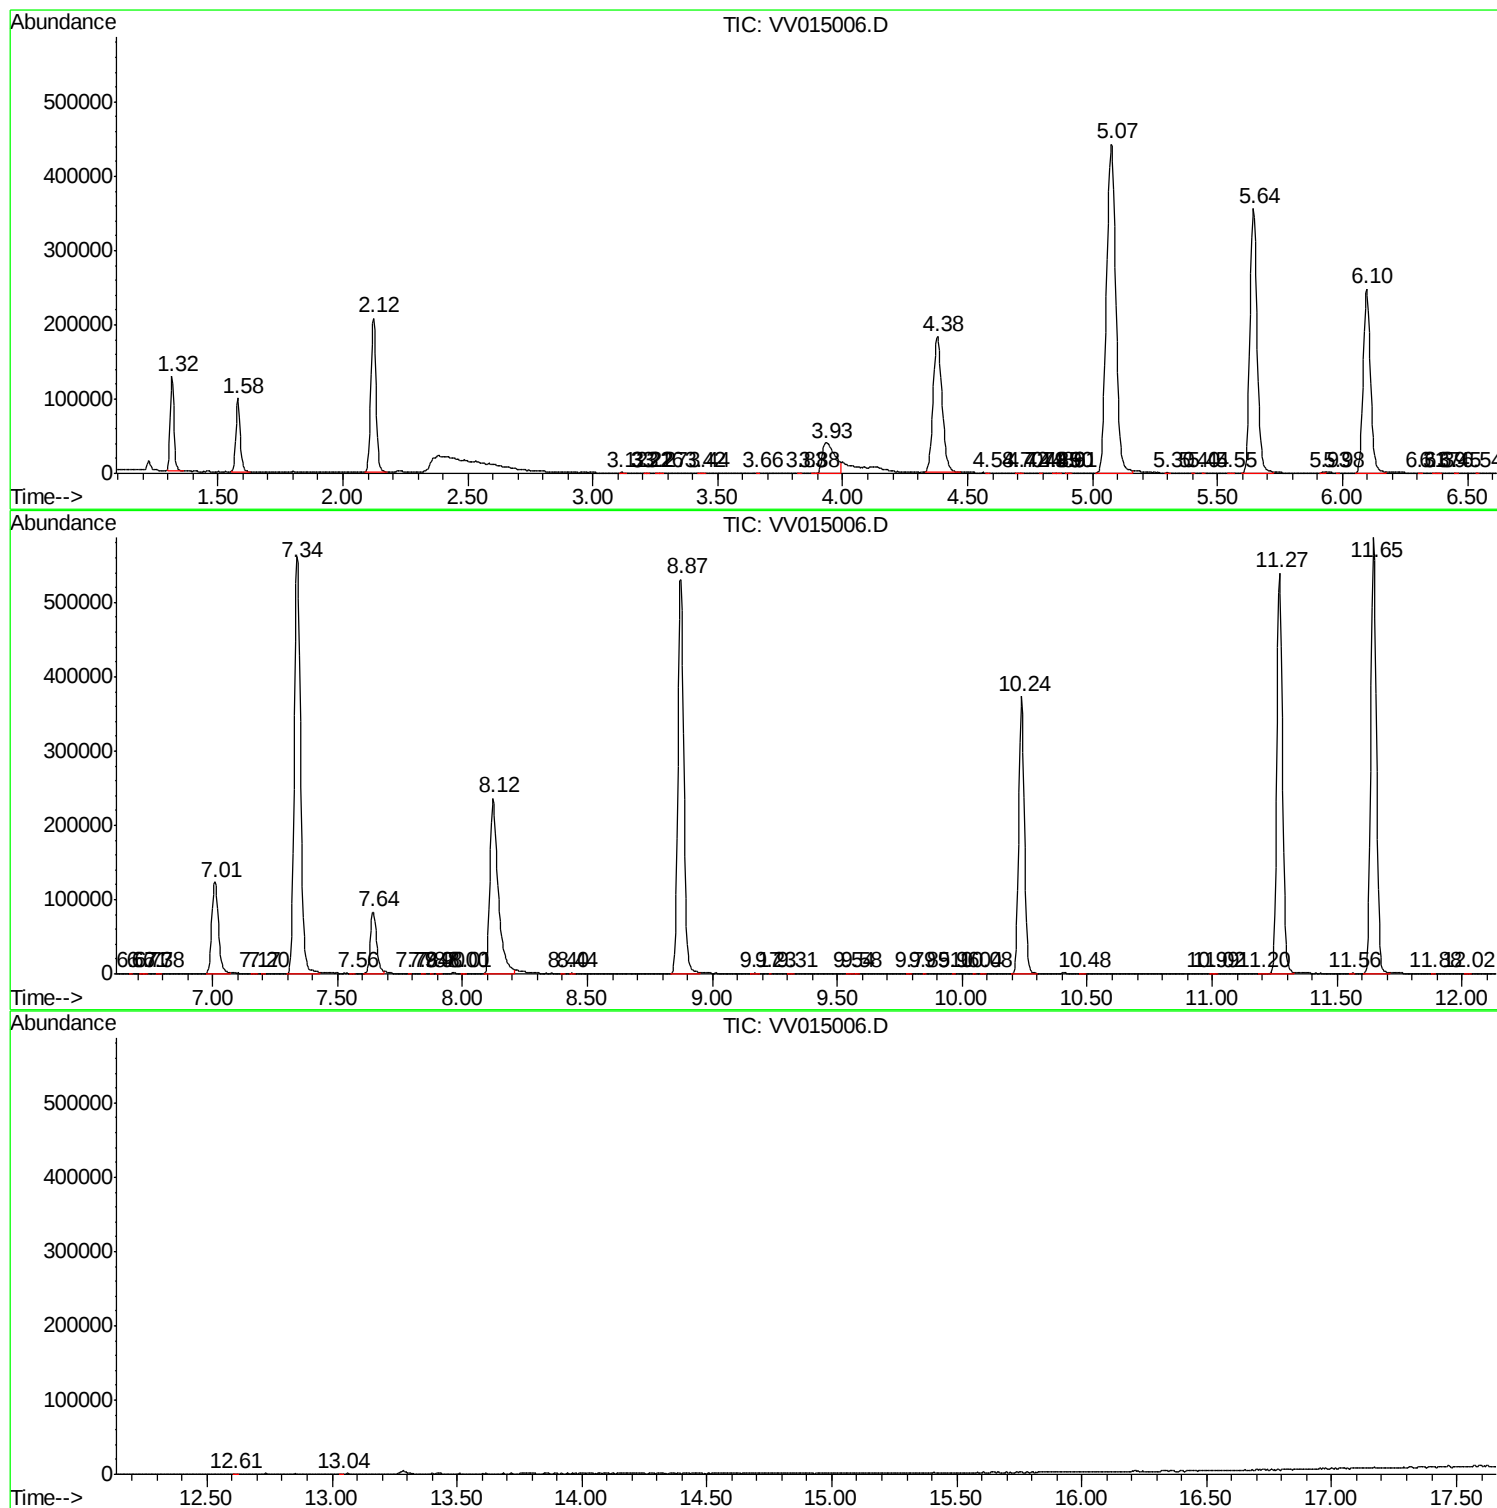

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV031720\
Data File : VV015006.D
Acq On : 18 Mar 2020 04:48
Operator : SY/MD
Sample : L1940-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0D88

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV031720\
Data File : VV015006.D
Acq On : 18 Mar 2020 04:48
Operator : SY/MD
Sample : L1940-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0D88

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc